


DESI Technical Design Report
Part II: Instrument Design
June 1, 2015

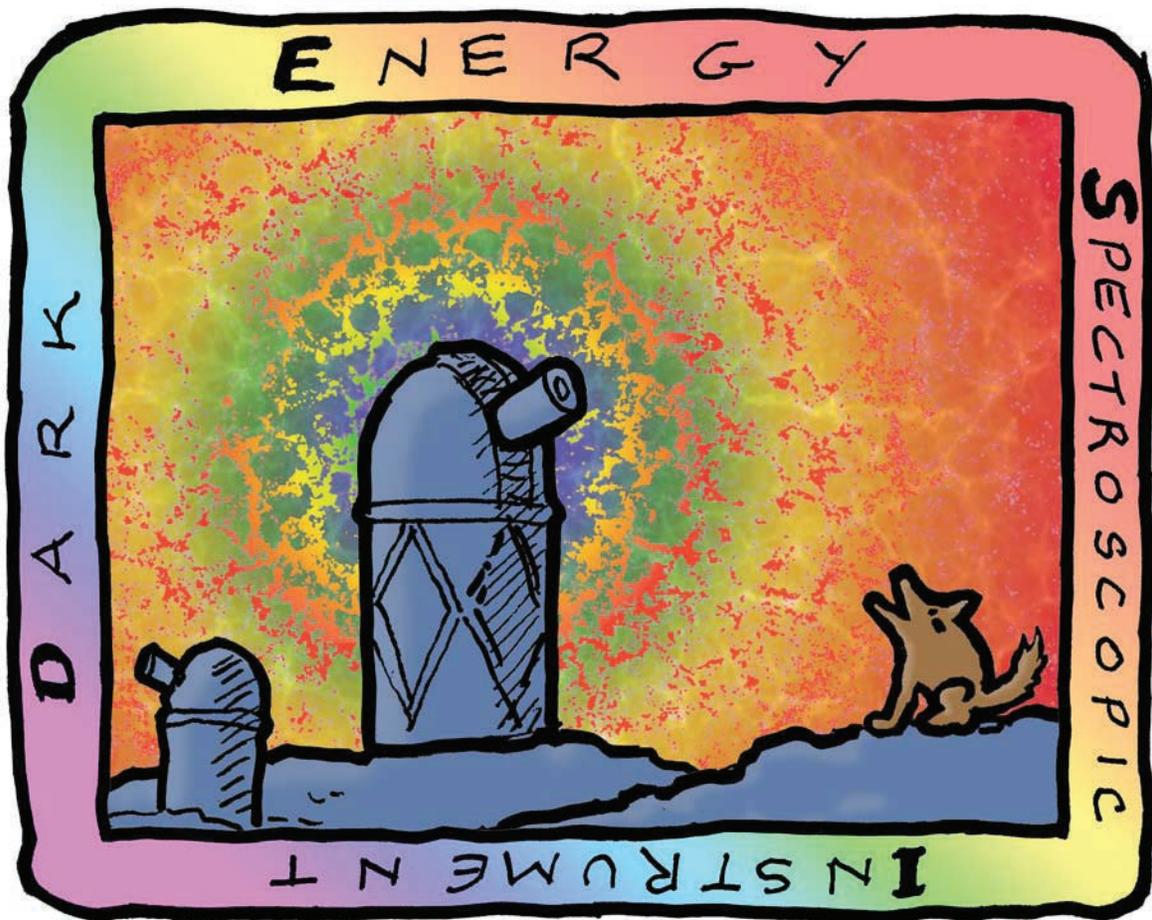

CD-2 Director's Review Version
2015-06-17

Compiled: 2015-06-02 16:57
DESI-1125 Part II

Contents

1	Overview	1
1.1	DESI Scope	1
1.2	DESI Subsystems	2
1.3	DESI Design Fulfills Requirements	2
1.3.1	Corrector Optics	4
1.3.2	Focal plane	5
1.3.3	Optical Fiber System	5
1.3.4	Spectrographs	5
1.3.5	Real-Time Control and DAQ	5
1.3.6	Data Management	5
1.4	Integration and Performance	5
2	Corrector	7
2.1	Corrector Optics Design	7
2.1.1	Atmospheric Dispersion Compensator	8
2.1.2	Material Optical Properties	9
2.1.3	Lens Tolerancing and Alignment	11
2.1.4	Focal Surface	11
2.1.5	Ghosts	11
2.1.6	Corrector Lens Acquisition and Polishing	13
2.2	Corrector Mechanical Design	14
2.2.1	Lens Cells	14
2.2.1.1	Lens Cell Design	16
2.2.1.2	Radial and Axial Pad Design	17
2.2.1.3	FEA Analysis	17
2.2.2	Barrel	18
2.2.2.1	Barrel Design	19
2.2.2.2	FEA Analysis	22
2.2.2.3	Comparing FEA Results with Specifications	22
2.2.3	Lens Cells and Barrel Alignment	23
2.2.3.1	Alignment of Lenses to Cells	23
2.2.3.2	Alignment of Cells to Barrel	25
2.2.4	Hexapod	25
2.2.5	Prime Focus Cage	26
2.2.5.1	End Rings	27
2.2.5.2	Hexapod Structure	27
2.2.5.3	Material and Coatings	27
2.2.6	Telescope Top End	28
2.2.6.1	Spider Vanes	28
2.2.6.2	Outer Ring	28
2.2.7	Prime Focus System Integration	28

3	Focal Plane System	30
3.1	Focal Plane Mechanical Design	31
3.2	Full-scale Demonstrator Petal	33
3.3	Fiber Positioners	34
3.3.1	Positioner Requirements	34
3.3.2	Positioner Interfaces	35
3.3.2.1	Mechanical Envelopes and Patterning	35
3.3.2.2	Mounting	37
3.3.2.3	Mass and Materials	38
3.3.2.4	Fiber, Power and Signal Services	38
3.3.2.5	Thermal budget	39
3.3.3	Positioner Mechanical Design	39
3.3.4	Positioner Electrical Design	41
3.3.5	Positioner Software	42
3.3.6	Fiber Interface	43
3.4	Guide-Focus-Alignment	43
3.4.1	Sensor Selection	44
3.4.2	Packaging	44
3.4.3	Electronics	45
3.4.4	Illuminated Fiducials	46
3.4.5	Acquisition and Guiding	46
3.4.6	Focus and Alignment	47
3.4.7	Stellar Density	48
3.4.8	Signal-to-Noise Studies via Simulation	49
3.4.9	Commissioning	50
3.5	Fiducial Illuminators	50
3.6	Fiber View Camera	51
3.6.1	Fiber View Camera Design	53
3.6.2	Development Program	53
3.6.3	Camera Control System	55
3.7	Thermal Management	55
3.8	Alignment, Integration, and Test	56
3.9	ProtoDESI	57
3.9.1	Introduction	57
3.9.2	Purpose	58
3.9.3	Additional Benefits	58
3.9.4	Performance Goal	58
3.9.5	ProtoDESI Elements	58
3.9.5.1	Focal plate	58
3.9.5.2	Positioners	58
3.9.5.3	Positioner Collision Avoidance	59
3.9.5.4	Fiber Photometry Camera	59
3.9.5.5	Fiber Back-Illumination System	59
3.9.5.6	Field Illuminated Fiducials	59
3.9.5.7	Guide/Focus/Alignment Sensor Module	60
3.9.5.8	Metrology	60
3.9.5.9	Ancillary Hardware	60
3.9.5.10	Integration	61

3.9.5.11	Fiber View Camera	61
3.9.5.12	Instrument Control System	61
3.9.6	Mayall	61
3.9.6.1	Telescope Control System	61
3.9.6.2	Electrical Power	61
3.9.6.3	Control Room Annex	62
3.9.6.4	Data	62
3.9.6.5	Mechanical/Architectural	62
3.9.7	Targeting and Observing Plan	62
4	Fiber System	63
4.1	Overview	63
4.2	Optical Fibers	63
4.2.1	Bulk Fiber Losses	63
4.2.2	Focal Ratio Degradation	65
4.2.3	Near Field Stability	67
4.3	Positioner Fiber Assembly	69
4.4	Fiber Management	71
4.4.1	Top-End Guides	71
4.4.2	Fiber Cables	72
4.4.3	Fiber Connection	74
4.5	Spectrograph Slit	75
4.5.1	Science Slits	75
4.5.2	Calibration Slits	77
4.5.2.1	PSF calibration Slit	77
4.5.2.2	Flatfield Slit	77
4.5.3	Mechanical Design	77
4.6	Fiber System Assembly and Integration	79
4.6.1	Component Level Testing	79
4.6.2	Engineering Model Level Testing	79
4.6.3	Production Level Testing	79
5	Spectrographs	81
5.1	Spectrograph Optical Design	81
5.1.1	Fiber Slit	83
5.1.2	Collimator	83
5.1.3	Dichroics	83
5.1.4	Gratings	84
5.1.5	Camera	85
5.1.6	Tolerancing and Simulation	89
5.2	Spectrograph Mechanical and Electrical Design	92
5.3	Spectrograph Integration and Test	97
5.4	Cryostats	97
5.4.1	Cryostat Design and Interfaces	98
5.4.1.1	Mechanical Design	98
5.4.1.2	Cryostat Vessels	99
5.4.2	Cryogenic System and Performance	99
5.4.2.1	LPT Cryocooler	100

5.4.2.2	Device Monitoring and Temperature Regulation	101
5.4.2.3	Cryocoolers and Vacuum Maintenance	102
5.4.3	Prototype Cryostat Measurements and Model Validation	102
5.4.4	Cryostat Control System	103
5.4.5	Cryostats Integration and Tests	105
5.5	Sensors and Electronics	106
5.5.1	CCDs	106
5.5.2	LBNL CCD Packaging	108
5.5.3	CCD Characterization	109
5.5.4	Electronics	111
5.6	Calibration System	111
5.6.1	Lamps	111
5.6.2	Sky Lines	112
5.6.3	Stars	113
5.6.4	CCD Flat Field Illuminator	113
6	Instrument Readout and Control System	114
6.1	Observation Control	116
6.2	Exposure Sequence	116
6.2.1	Active Optics System	119
6.2.2	Plate Maker	119
6.2.3	Guider	120
6.2.4	Exposure Time Calculator	122
6.3	Readout and Dataflow	123
6.3.1	Quality Assessment	125
6.4	Operations Database	125
6.4.1	Guider Image Data Management	126
6.4.2	Technology Choices, Reliability and Development Status	127
6.5	Instrument Monitor and Control System	127
6.6	Telescope Operations Interface	128
6.7	Online Software	129
6.7.1	Infrastructure Software	129
6.7.2	Configuration	130
6.7.3	Application Framework	130
6.7.4	User Interfaces and Observer Console	131
6.8	Readout and Control System Hardware	132
6.9	Integration and Testing	133
7	Data Systems	135
7.1	Target Selection Pipeline	137
7.2	Survey Planning, Fiber Assignment, and Operations	138
7.2.1	Fiber Assignment	138
7.2.1.1	Merged Target List	138
7.2.1.2	Key Project Target Fiber Assignment	139
7.2.1.3	Performance of Tiling and Fiber Assignment	140
7.2.1.4	Calibration Target Fiber Assignment	141
7.2.1.5	Ancillary Program Target Fiber Assignment	141
7.2.1.6	Target Assignment Bookkeeping	141

7.2.1.7	Bright Time Survey Fiber Assignment	142
7.2.2	Next Field Selector	142
7.2.3	Quicklook Extraction Pipeline	142
7.2.4	Survey Simulations	143
7.2.5	Survey Quality Assurance Interface	144
7.2.6	Planning for Commissioning and Science Verification	144
7.3	Data Processing	145
7.3.1	Spectroscopic Data Reduction Pipeline	145
7.3.1.1	Pixel-level Calibration and Preprocessing	146
7.3.1.2	2D PSF Calibration	147
7.3.1.3	Spectral Extraction and Sky Subtraction	148
7.3.1.4	Flux Calibration and Coaddition	149
7.3.1.5	Classification and Redshift Measurement	149
7.3.1.6	Progress and Quality Assurance Tracking	150
7.3.1.7	Prototype Spectroscopic Pipeline Results	151
7.3.2	Software Development	152
7.4	Data Transfer, Archive, and Distribution	153
7.4.1	Raw Data Transfer	153
7.4.2	Operational Data Archiving	153
7.4.3	Processed Data Distribution	153
7.4.4	Data Releases	154
7.5	Large Scale Structure Catalog	154
7.5.1	Angular Selection Function and Angular Systematics	155
7.5.2	Radial Selection Function and Radial Systematics	155
7.5.3	Effects of Fiber Assignment	156
7.6	Simulations	156
7.6.1	Cosmological Simulations	157
7.6.2	Operations Simulations	159
7.6.3	Target Spectral Templates	159
7.6.4	Instrument Simulations	159
7.6.4.1	desimodel	161
7.6.4.2	Quicksim	161
7.6.4.3	Specter Pixel-Level Simulations	162
7.6.5	DESI Oerformance Studies	162
7.6.5.1	ELG Signal-to-Noise	162
7.6.5.2	Redshift Success Rates	164
7.6.5.3	Trade Studies	164
7.6.6	DESI End-to-End Survey Simulations	165
7.7	Computing Requirements	166
7.7.1	Target Selection	167
7.7.2	Cosmological Simulations	168
7.7.3	Instrument Simulations	169
7.7.4	Spectroscopic Data Processing	169
7.7.5	Science Analysis for Cosmology	170
7.7.6	Computing Requirements Summary	171
7.8	Collaboration Tools	171

8	Integration and Test	172
8.1	Instrument Integration and Test	172
8.1.1	Corrector Barrel/Corrector Optics/ADC Rotators	173
8.1.2	Telescope Fixed Top End Structure/Hexapod	173
8.1.3	Focal Plane/Fiber System	174
8.1.3.1	Pre-Shipment	174
8.1.3.2	Post-Delivery	175
8.1.4	Spectrographs/Cryostats	175
8.1.5	Instrument Control System	176
8.1.5.1	Fiber View Camera	176
8.2	Mayall Preparation	176
8.2.1	Measurements	177
8.2.1.1	Laser Tracker Measurement of M1 Surface	177
8.2.1.2	Environmental Monitoring	177
8.2.2	Observatory Facility Modifications	178
8.2.2.1	Cooling System Modifications	178
8.2.2.2	Electrical System Modifications	180
8.2.2.3	Telescope Modifications	181
8.2.2.4	Spectrograph Room Modifications	182
8.2.2.5	Mayall Control Room Annex	182
8.2.2.6	Calibration System	183
8.2.2.7	Computer Room	184
8.2.2.8	Ground Floor Garage	184
8.2.3	Installation Planning	185
8.2.4	Installation Equipment Preparation	185
8.3	Installation	186
8.3.1	Removal of Existing Telescope Hardware	187
8.3.1.1	Preparation of Top End for Removal	187
8.3.1.2	Bottom End Disassembly	189
8.3.1.3	Top End Removal	189
8.3.2	Installation of DESI Hardware	190
8.3.2.1	Initial Assembly and Installation of New Telescope Top End	191
8.3.2.2	Re-Assembly of Telescope Bottom End	192
8.3.2.3	Top End Mechanical Alignment	193
8.3.2.4	DESI Fiber Cable and Cooling Hose Installation	193
8.3.2.5	Telescope Motion Tests and Final Alignment Check	195
8.3.2.6	Spectrographs	195
8.3.2.7	Computer Equipment	196
8.3.2.8	Support to Other DESI Subsystem Tests	196
8.3.2.9	Telescope Re-Verification	196
8.4	Safety	197
8.4.1	Environmental, Health and Safety Plans	197
8.4.1.1	Compliance with Regulations, Codes and Standards	197
8.4.1.2	Environmental, Health and Safety Plan Responsibilities	198
8.4.1.3	EHS Plan Expectations	198
8.4.1.4	Contractor Safety and Health Plans	198
8.4.1.5	EHS Plan Availability to Personnel	199
8.4.2	Safety Reviews and Hazard Analysis	199

8.4.2.1	Safety Reviews	199
8.4.2.2	Job Hazard Analysis	199
8.4.3	Safety Management	200
8.4.3.1	Kitt Peak Safety Manager	200
8.4.3.2	NOAO Associate Director for Kitt Peak	200
8.4.3.3	NOAO DESI Project Manager	201
8.4.3.4	NOAO Safety Team	201
8.4.3.5	Team Members	201
8.4.4	Design for Safe Installation and Operation	201
9	Commissioning	203
9.1	Overview	203
9.2	Functional Verification	203
9.3	Commissioning	204
9.4	Science Verification	205
9.5	Commissioning Strategy	205
9.6	Commissioning Roles	206
9.7	Summary	206
A	Acronyms	207
	References	213

1 Overview

1.1 DESI Scope

DESI, the first Stage IV dark energy experiment, will use the redshifts of 25 million galaxies to probe the nature of dark energy and test General Relativity. DESI builds on the successful Stage-III BOSS redshift survey, which has established BAO as a precision technique for dark energy exploration. DESI will make an order-of-magnitude advance over BOSS in volume observed and galaxy redshifts measured by using 5,000 robotically controlled fiber-positioners to feed a collection of spectrographs covering 360 nm to 980 nm. Newly designed optics for the 4-m Mayall telescope at Kitt Peak, Arizona, will provide an 8-square-degree field of view.

DESI is an important component of the DOE Cosmic Frontier program, meeting the need for a wide-field spectroscopic survey identified in the 2011 “Rocky-III” dark energy community planning report. It complements the imaging surveys Dark Energy Survey (DES, operating 2013-2018) and the Large Synoptic Survey Telescope (LSST, planned start early in the next decade). In addition to providing Stage-IV constraints on dark energy, DESI will provide new measurements that can constrain theories of modified gravity and inflation, and will provide cutting-edge limits on the sum of neutrino masses. The DESI collaboration will also deliver a spectroscopic pipeline and data management system to reduce and archive all data for eventual public use.

The DESI collaboration is planning a five-year spectroscopic survey covering 14,000 deg², targeting three classes of galaxies identified from imaging data. We will measure luminous red galaxies (LRGs) up to $z = 1.0$, extending the BOSS LRG survey in both redshift and survey area. To probe to even higher redshift, DESI will target bright [O II] emission-line galaxies (ELGs) up to $z = 1.7$. Quasars will be targeted both as direct tracers of the underlying dark matter distribution and, at higher redshifts ($2.1 < z < 3.5$), for the Ly- α forest absorption features in their spectra, which will be used to track the distribution of neutral hydrogen. More than 20 million galaxy and quasar redshifts will be obtained to measure the BAO feature and determine the matter power spectrum, including redshift space distortions. In this document we consider primarily this baseline survey. We also provide numbers for a reduced survey spanning 9,000 deg², which is still sufficient to meet the requirements of a Stage-IV project.

DESI will obtain more than 30 independent distance-vs-redshift measurements, a powerful probe of the nature of dark energy. This can be quantified with the Dark Energy Task Force figure of merit (DETF FoM [1]), which measures the combined precision on the present day dark energy equation of state, w_0 , and the rate of its evolution with redshift, w_a . DESI galaxy BAO measurements achieve a DETF FoM of 125, more than a factor of three better than the DETF FoM of all Stage-III galaxy BAO measurements combined. The FoM increases to 152 with the inclusion of Ly- α forest BAO, and 326 including galaxy broadband power spectrum to $k = 0.1 h \text{ Mpc}^{-1}$. DESI thus satisfies the DETF criteria for a Stage-IV experiment, generally taken as a factor of three increase over Stage-III. Moreover, the FoM grows to 756 when the galaxy broadband power spectrum data out to $k < 0.2 h \text{ Mpc}^{-1}$ are included.

DESI’s science reach will extend beyond dark energy. It will measure the sum of neutrino masses with an uncertainty of 0.017 eV (for $k_{\text{max}} < 0.2 h \text{ Mpc}^{-1}$), sufficient to make a direct non-zero detection of the sum of the neutrino masses at 3- σ significance. If the neutrino masses are minimal, and the hierarchy is normal, the inverted hierarchy will be ruled out at 99% CL. DESI will also place significant constraints on theories of modified gravity by measuring redshift space distortions, and on theories of inflation by measuring the spectral index n_s and its running with wavenumber, α_s .

DESI will provide an unprecedented multi-object spectroscopic capability for the U.S. using

an existing NSF telescope facility. Many other science objectives can be addressed with the DESI wide-field survey dataset, bright time survey, and piggy-back observation programs. Much as with SDSS, a rich variety of projects will be enabled with the legacy data from the DESI survey.

DESI will overlap with the DES and LSST survey areas, which are primarily in the southern hemisphere but which will have equatorial and northern ecliptic regions. DESI will be a pathfinder instrument for the massive spectroscopic follow-up required for future large area imaging surveys such as LSST.

This Technical Design Report summarizes the DESI scientific goals, the instrument and optical design, the target selection, the integration and test plan, and the data management plan. The companion Science Requirements Document provides information that guides the design. The DESI construction management plan is presented in the accompanying Project Execution Plan. Likewise, project cost and schedule are available in relevant Project Office documents.

1.2 DESI Subsystems

The DESI subsystems comprise

1. Prime focus corrector optics.
2. Focal plane with robotic fiber positioners.
3. Optical fiber system.
4. Spectrographs.
5. Real-time control and data acquisition system.
6. Data management system.

Each subsystem has a specification, including performance requirements. Tests will be developed to demonstrate that the subsystems meet these requirements prior to shipment to the Mayall. After delivery to the Mayall, a subset of the pre-ship tests will be repeated to verify survival of shipping along with general system function.

A critical aspect of each element of the instrument is its interface or interfaces with other elements. The system block diagram (Figure 1.1) is used to identify interfaces between elements from different suppliers. Figure 1.2 shows a high-level DESI Interface Matrix (or N-squared matrix), illustrating the locations and types of interfaces between the major elements of the DESI instrument, as integrated with the Mayall Telescope. Each of these interfaces will be managed with an Interface Control Document (ICD).

1.3 DESI Design Fulfills Requirements

The design of the DESI instrument is set by the key science project and operational requirements defined in the DESI Level 1 through Level 3 Requirements Document [2]. Instrument subsystem impacted by these requirements are outlined below.

- A. Field of view (effective) not less than 7 square degrees [Corrector optics, Focal plane].
- B. $S/N > 7$ for the detection of an [O II] flux of 8×10^{-17} erg/s/cm² in ELGs [Fiber optics, Spectrographs].
- C. A baseline 14,000 deg² survey, with a minimum-requirements of 9,000 deg² [Data management, Corrector optics].

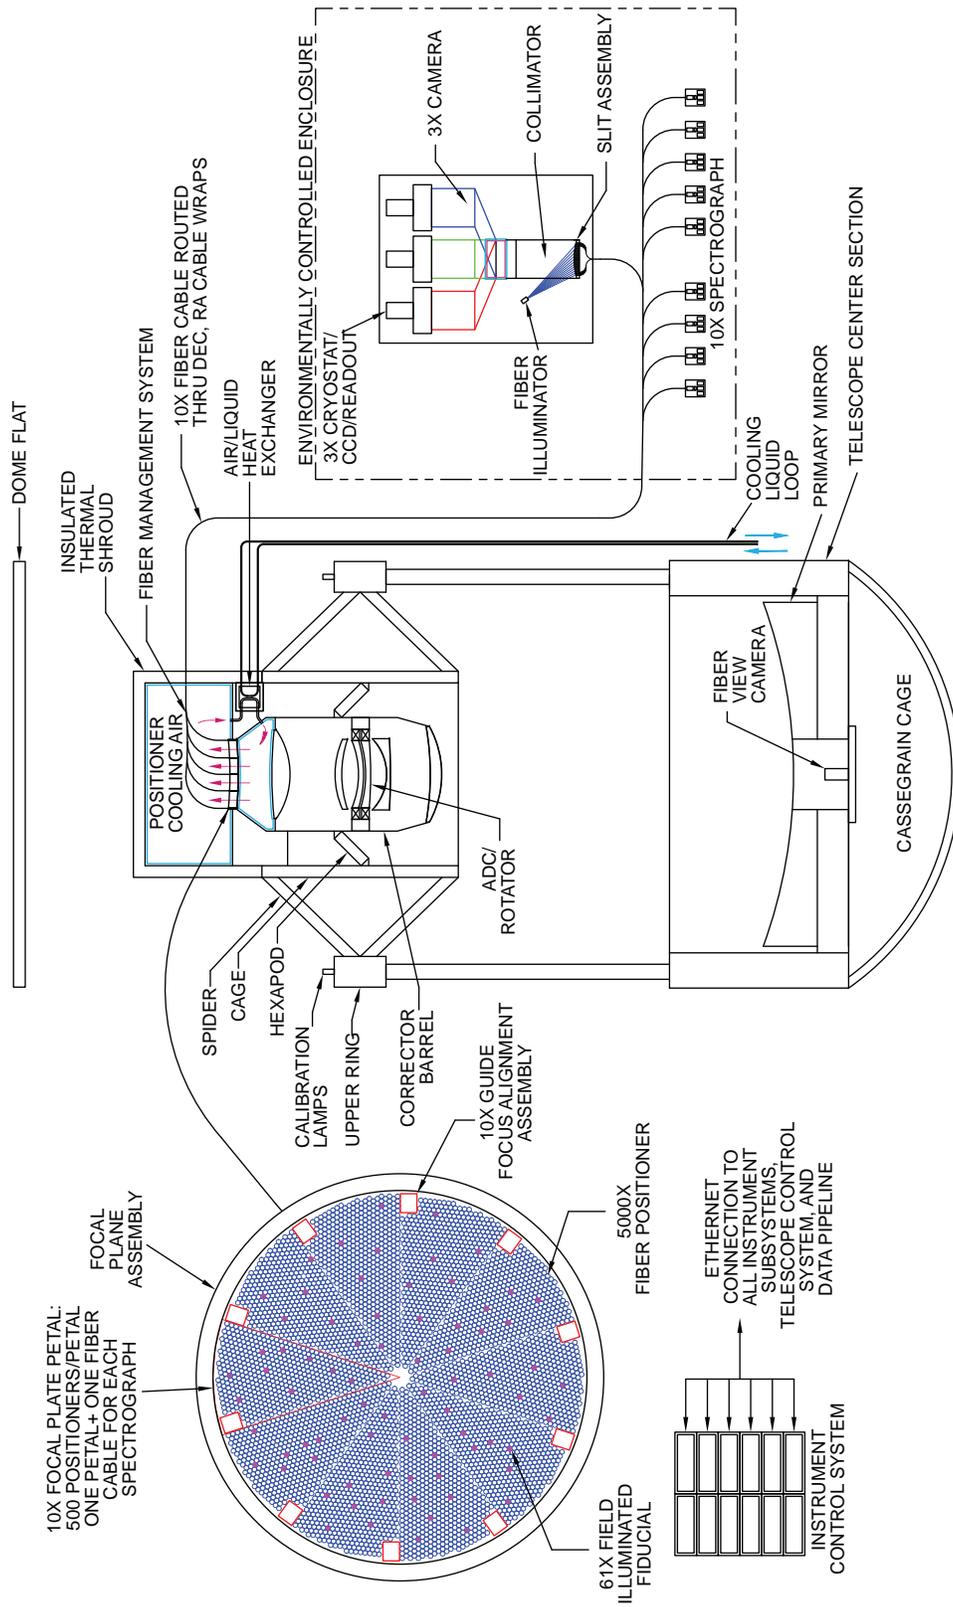


Figure 1.1: DESI block diagram.

1000 seconds, this is sufficient to cover the 14,000 square degree footprint approximately five times, enough to guarantee approximately 25 million successful spectra from a larger target list, with multiple exposures of certain targets [C,D].

1.3.2 Focal plane

The 5,000 positioners instrument 7.5 square degrees of the 8 available [A], giving a fiber density of 667/square degree [F]. The focal plane also hosts field fiducials and Guide, Focus, and Alignment (GFA) sensors, located at the periphery of the instrumented focal plane. The positioners are arranged in a hexagonal pattern with a 10.4 mm pitch between centers. Each positioner has two rotational degrees of freedom allowing it to reach any point within a 6 mm radius. The focal plane is divided into ten pie-slice-shaped petals.

1.3.3 Optical Fiber System

Optical fibers run 38 m from each positioner to the spectrographs. The core diameter of the fiber is 107 μm . The fiber system throughput varies from 0.499 at 360 nm to 0.838 at 980 nm [B,G].

1.3.4 Spectrographs

Two dichroics split the output of the optical fibers into three channels. The throughput for the dichroics is greater than 95% throughout the full wavelength range, except for the dichroic transition intervals (747-772 nm) and (566-593 nm), where it still exceeds 90%. Volume phase holographic gratings provide dispersion in the three channels, [360-593 nm], [566-772 nm], and [747-980 nm] [G], with resolutions greater than 2000, 3200, and 4100 respectively [H]. The blue arm of the spectrographs use CCDs from Imaging Technologies Lab, while the red and NIR channels use LBNL CCDs. All will be 4k x 4k with 15 μm pixels [B].

1.3.5 Real-Time Control and DAQ

DESI real-time control and DAQ components such as the dynamic exposure time calculator, the realtime data quality assessment, and complex algorithms to convert on-sky target coordinates to fiber positions on the focal plane are based on the SDSS-III/BOSS online system. The time between exposures will be less than 120 seconds [E].

1.3.6 Data Management

An initial list of targets will be assembled from imaging completed prior to the survey, with criteria designed to select LRGs, ELGs, and QSOs. The 14,000 square degree footprint will be covered by about 10,600 tiles, providing average coverage of each spot of $10,600 \times 8\text{sq. deg.} / 14,000\text{sq. deg.} = 6$ times [E].

1.4 Integration and Performance

A block diagram of DESI at the Mayall telescope is shown in Figure 1.1. The Mayall is a 4-m telescope capable of supporting a 3.2-degree diameter field of view, which DESI achieves with a new prime focus optic, lens barrel, support cage with hexapod adjusters, and a new ring attachment to the top of the telescope.

Careful management of all the elements that contribute to overall light throughput is a systems engineering activity. There are 70+ DESI elements that affect throughput presently being

tracked against current estimates (DESI-0347). These instrument performance parameters are combined with sky, atmospheric, galaxy, and survey parameters to simulate and predict DESI performance (see Section 7.6.4.1). These in turn drive the exposure time range describe in TDR Part I, Section 4.4.2. Rollup values from the instrument throughput tracking spreadsheet are shown in Table 1.1 and we briefly describe the items below. Note that all values are field-weighted averages.

Blur. Includes contributions to spot size at the fiber tip from intrinsic blur of the corrector optics prescription, manufacturing and alignment errors in the corrector, alignment errors of the corrector relative to the mirror, and defocus due to gravity, manufacturing and alignment errors. Note that the blur tabulated below does not include atmospheric effects or telescope jitter or tracking errors. These effects are accounted for in the simulations modeling the delivered image quality.

Lateral errors. Summarizes inaccuracies in placing the target centroid onto the center of the optical fiber, including effects such as fiber positioner inaccuracies, fiber view camera inaccuracies, uncompensated atmospheric refraction, focal plane thermal and gravity distortions, metrology errors between guiders and fibers, and misalignments of the corrector relative to the mirror. Note that the blur tabulated below does not include atmospheric effects, telescope jitter, or telescope tracking errors. Again, these effects are accounted for in the simulations modeling the delivered image quality.

Telescope to Fiber Input Throughput. Accounts for losses due to primary mirror reflectivity, corrector lens absorption and anti-reflectance coatings, corrector vignetting, and scattering in the corrector optics.

Fiber System. Includes losses due to fiber bulk absorption, reflections at entrance and exit, and focal ratio degradation (FRD). FRD effects include losses due to fiber construction, end polishing, bends/twists, and tilt of the chief ray relative to the fiber normal.

Spectrograph. Spectrograph losses, including collimator reflectivity, dichroic effectiveness, grating efficiency, camera glass absorption and detector quantum efficiency are considered in the spectrograph row.

Instrument throughput. Sky throughput is a measure of the net throughput of the instrument from light at the aperture to electronic signals from the detectors. It is the product of the telescope-to-fiber-input, fiber system, and spectrograph throughputs. It does not include the atmosphere, obscurations, or galaxy effects, nor does it include losses due to blur or lateral errors, which are separately reported.

Table 1.1: DESI throughput current best estimates rollup (DESI-0347).

	Wavelength (nm)						
	360	450	550	650	750	850	980
Blur (μm 1-D sigma)	15.6	14.3	13.4	13.9	14.8	15.4	15.6
Lateral Errors (μm)	13.4	11.7	11.0	12.3	13.0	12.7	12.9
Telescope to Fiber Input Throughput (%)	56.5	71.8	74.2	67.1	68.4	70.4	69.9
Fiber System Throughput (%)	49.7	70.0	78.0	81.1	82.4	82.7	83.6
Spectrograph Throughput (%)	39.4	73.1	68.5	74.5	67.4	77.5	55.3
Instrument Throughput (%)	11.1	36.8	39.6	40.6	38.0	45.2	32.4

2 Corrector

The DESI multi-object spectrograph uses the existing primary mirror at the Mayall telescope with a newly developed prime focus corrector that allows $\sim 5,000$ robotically positioned fibers to be arranged 8 deg^2 .

2.1 Corrector Optics Design

Optical requirements as well as predicted performance of the baseline DESI Prime Focus Corrector (Echo 22) (DESI-0329) are listed in Table 2.1. The design includes four large fused silica elements. The two smaller lenses have aspheres on one surface each; all other silica surfaces are spherical. The lens specifications are within the capabilities of multiple vendors. An atmospheric dispersion compensator (ADC) is included in the design, in order to meet blur requirements at off-zenith angles. This compensator includes two large wedged borosilicate lenses; all surfaces are spherical. The layout of the optical corrector elements is shown in Figure 2.1.

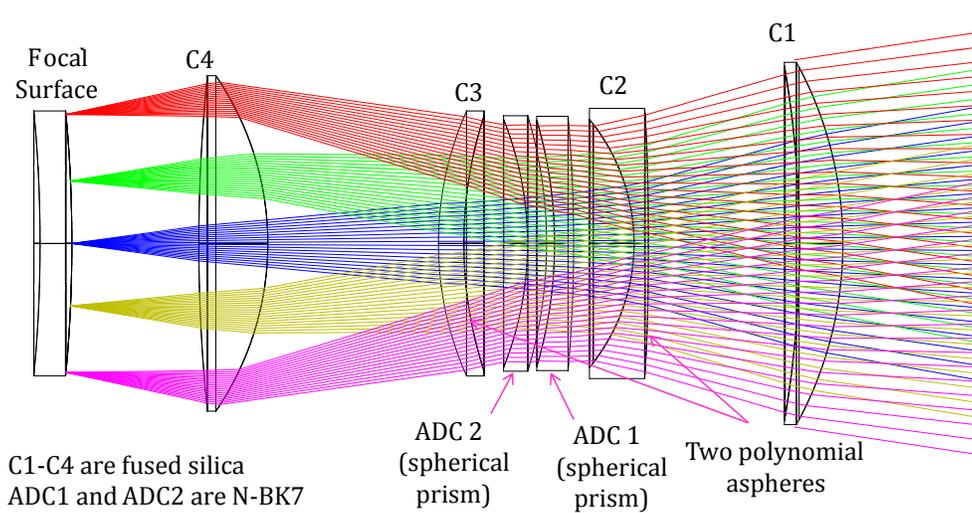


Figure 2.1: Optical layout of Echo 22.

The Mayall telescope primary mirror (M1) is 3.8 m diameter, has a radius of curvature of 21.3 m, and a focal length of 10.7 m. This physical structure sets the scale for a corrector with a linear 3.2° FOV, corresponding to a diameter of ~ 812 mm at prime focus. Table 2.2 is a summary of the DESI corrector optical design parameters. Because optical elements are placed between the prime focus and M1, optical elements are as large as 1140 mm in diameter. Table 2.3 shows manufacturing details of the six corrector elements, including mass, materials and dimensions. The large size of these elements reduces the pool of potential vendors, but DESI has successfully contracted for the production of all lenses with reliable vendors. The blanks for lenses C1 and C4 are provided by Corning, and are polished by L3 Brashear. The blanks for lenses C2 and C3 are provided by Ohara, and are polished by Arizona Optical Systems. The blanks for the ADC lenses are provided one each by Schott and Ohara, and are polished by Rayleigh Optical Corporation.

Vendors recommended that aspheric departure slope should be limited to values less than 30 mrad ($\mu\text{m}/\text{mm}$), to allow interferometric testing with better than Nyquist fringe sampling. The peak aspheric slope departures of lenses C2 and C3 are <15 and <11 , respectively.

Table 2.1: Prime Focus Corrector Requirements (DESI-0478). Blurs are FWHM, maximums are for any field position, and means are field averaged.

Requirement	Value	Note
Optical design	Compatible with Mayall 4 m primary mirror	Mayall telescope selected for DESI.
Wavelength band	360–980 nm	Required for z range of Ly- α QSOs and ELGs
Design residual blur (arcsec)	zenith: 360–450 nm: <0.4 mean, 0.60 max 450–980 nm: <0.4 mean, 0.50 max 60 deg from zenith: 360–450 nm: 0.4 mean, 0.75 max 450–980 nm: 0.4 mean, 0.6 max	360–450 nm: required for QSO/LRG system throughput 450–980 nm: required for LRG/ELG system throughput
Field of view	> 3° diametral	Required for Poisson statistics of targets.
f/# variation	f/3.7 to f/4.3	f/# number variation is allowed, but must be constrained.
Focal surface diameter	Sufficiently large to contain $\geq 5,000$ fiber positioners	Verified by the focal plate layout simulator.
Focal surface curvature	Radius of curvature (convex), greater than 3000 mm	Focal plate may be curved, with aspheric shape, but maximum curvature is constrained for actuator packaging.
Aspheric departure slope	<30 mrad	Manufacturability; Aspheres are permissible on one surface of smaller, non-ADC elements.
Chief ray deviation	< 0.5° average, < 1.0° maximum	Required for system throughput. This is to be met at all field points, and thus all f/ratios.
Glass throughput of combined elements	> 75% at 360 nm > 88% at 375 nm > 94% at 400 nm > 95% for > 450 nm	Required for system throughput.
Vignetting	0% up to 1.45°; < 1% elsewhere	Required for system throughput.
Ghosting	< 1% of observation region contaminated by ghosts brighter than $0.01 \times$ Night sky.	Focal and pupil ghosts must not contaminate a large fraction of the survey region.
Glass mass	< 900 kg	To ensure barrel and mount the lenses and telescope can support the corrector
Lens diameter	≤ 1175 mm	Required for obscuration

Table 2.2: DESI Corrector Optical Design Summary . Refer to DESI-0329 for details about the optical design.

Parameter	Value
Primary Mirror diameter	3.8 meters circular
Field of View	3.2 degrees circular 811.8 mm at the focal plane
F/#	3.68 on-axis 3.86 average over FOV
Plate scale	243.0 mm/deg on-axis 254.8 mm/deg, average over FOV

2.1.1 Atmospheric Dispersion Compensator

The ADC includes two monolithic N-BK7 elements, each with two spherical surfaces and an internal wedge angle. ADC elements are monolithic, and have no bonded joints. Although designs exist

Table 2.3: Echo 22 corrector lenses. Total mass of corrector glass is 864 kg.

Lens	Diam (mm)	Mass (kg)	Material	Index	Vertex Thick (mm)	Edge Thick (mm)	Total Lens Thick (mm)
C1	1140	201	Silica	1.46	136.4	39.9	186.0
C2	850	151	Silica	1.46	45	204.7	216.5
ADC1	800	102	N-BK7	1.52	60	102.1	119.7
ADC2	804	89	N-BK7	1.52	60	80.7	140.0
C3	834	84	Silica	1.46	80	59.9	148.3
C4	1034	237	Silica	1.46	217	34.9	216.9
Focal	811.8		Al 6061	—			

which use fused silica for all lens elements, curved N-BK7 ADC elements allow better control of lateral color on the blue end of the DESI band. The lens elements have a slight ($\sim 0.25^\circ$) internal wedge angle, which leads to predictable lateral color. The net dispersion magnitude and direction is set by rotating the ADC elements (Figure 2.2) in opposite directions, along the corrector optical axis. Thin ring Kaydon[®] bearings (similar to those used on the One Degree Imager for WIYN) are employed to support the ADC lens cells, and allow independent rotation of the ADC elements. When oriented in opposite directions, the wedges introduce minimal chromatic aberrations. Opposite direction rotations introduce increasing dispersion, while identical rotation of the elements changes the direction of dispersion (required for an equatorial mount telescope).

Due to the wedge angle of the spherical ADC elements, the system has no optical symmetries. Blur distributions cannot be represented as simple radial distributions, but must be quantized over the entire focal surface. In the figures below, the full width, half maximum (FWHM) of the geometric blur for the perfect system is plotted. This includes design residual phase error, but does not include estimates of system performance with manufacturing errors. Figure 2.3 shows blur at zenith, 30° , and 60° after correction by the ADC.

2.1.2 Material Optical Properties

The lenses of Echo 22 are large, but not of unprecedented size. Larger diameter lenses are currently envisioned for the LSST camera and a 1.5 m diameter fused silica conformal window was produced by Heraeus and Corning for the ABL project. In the case of DESI, capable vendors with a history of successful deliveries have been chosen from a limited pool to provide the fused silica and N-BK7 blanks. The main question is the impact of homogeneity grades on delivered image quality. Optical modeling of the DESI design suggests that variation in the refractive index of the raw material mainly affects wavefront distortion in low-order Zernike modes, i.e., variations up to about three cycles per lens diameter.

A statistical (Monte Carlo) study of the effects of various homogeneity grades was performed, and contributions to the blur budget investigated. Cost of glass increases with improved homogeneity, but this cost may be balanced against polishing cost, as transmissive multi-pass optical testing allows the effects of homogeneity to be polished out, but at greater polishing cost. Results of this study, in conjunction with programmatic considerations, have allowed procurement of appropriate-value optical substrates for DESI.

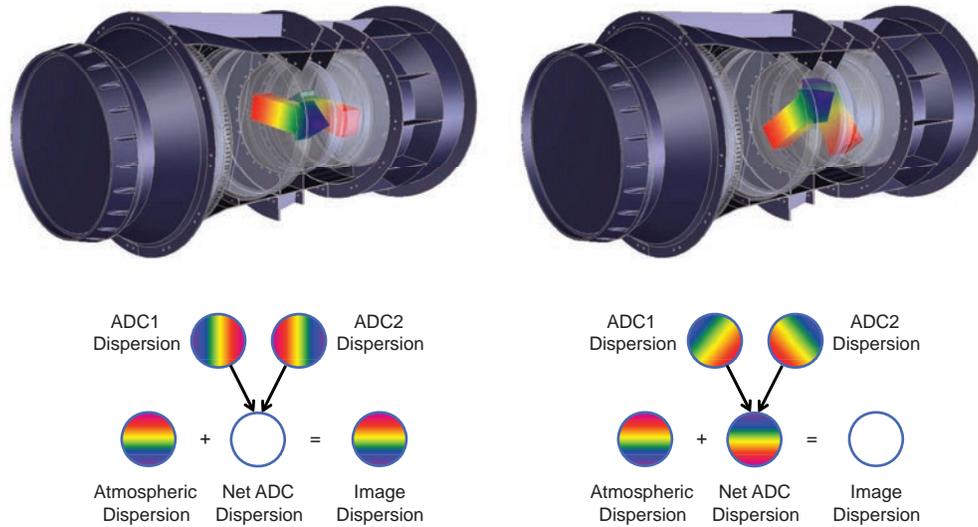


Figure 2.2: The atmospheric dispersion compensator consists of two oppositely oriented prisms (figures at left) which produce leftward and rightward dispersions that exactly cancel each other. Prism pairs can be rotated in opposite directions to produce a net dispersion opposite to that of the atmospheric contribution. Left and right components still cancel (figures at right), but allow a variable net dispersion that can be selected to negate atmospheric dispersion.

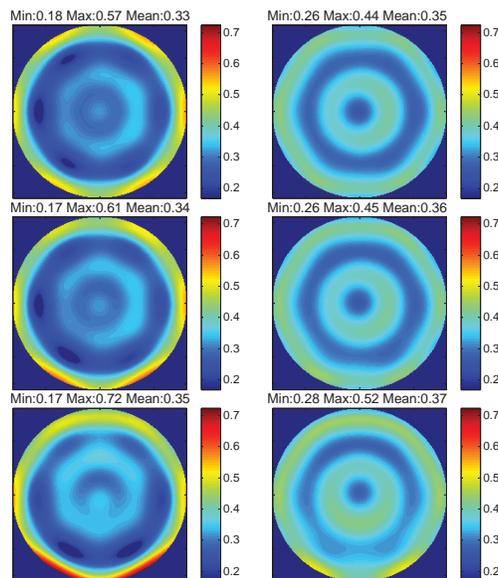


Figure 2.3: Geometric blur is shown as a function of zenith angle. Top figures: zenith. Middle figures: 30° zenith angle. Bottom figures: 60° zenith angle. Numbers above figures are FWHM blur in arcsec.

2.1.3 Lens Tolerancing and Alignment

Preliminary manufacturing tolerance studies have been performed (DESI-0335) on the individual lens elements. The studies show that given melt data from the fused silica and N-BK7 suppliers, bulk index of refraction variations are easily compensated by small changes to the lens spacings.

Instead of specifying tight tolerances on the lens thickness and radii of curvature, a compensation scheme is employed that allows lens spacings to be adjusted based on as-built measurements of lens thickness and radii. A Monte Carlo inverse analysis was performed to determine the sensitivity of blur performance on compensated lens parameters. Given this, manufacturing tolerances can be specified using values that are readily met.

Lenses are held in lens cells, which are in turn held by the barrel assembly. Errors in the positions of the lenses result from a stackup of tolerances including lens mount, cell mounts, corrector barrel thermal and mechanical distortion. Allowable limits for decenter and tilt were established by Monte Carlo simulation. These tolerances assume 5-DOF compensation by the hexapod and perfect knowledge of the misalignment (wavefront errors are budgeted elsewhere). This budget is parceled out to the various contributing components in DESI-0335.

2.1.4 Focal Surface

While maintenance of the focal array assembly is not required, it is possible that the assembly will be required to be removed after installation at some point. For that reason, a repeatable mount (pins or semi-kinematic mounts) is being considered for the focal plate interface to the corrector barrel adapter. Tolerances for the focal plate mount, relative to the optical axis, are $\pm 150 \mu\text{m}$ lateral and $\pm 75 \mu\text{m}$ tip/tilt (across the diameter).

The design of Echo 22 included constraints on the maximum tilt of the chief ray. The chief ray should be aligned with the fiber axis for maximum injection efficiency. Generally in an optical system, the chief ray will not be normal to the local surface. The relatively large field of view of this optical corrector exacerbates the issue, and the chief ray must be constrained to a manageable level in the optimization merit function. Because the actuator mounting holes are drilled by a 5-axis CNC machine, holes can be tilted to match the chief ray direction. This technique, and effects on actuator packaging are discussed in the focal plate section of this report. Figure 2.4 shows the residual chief ray tilt as a function of field angle.

Figure 2.5 shows the anamorphic (non-symmetric) distortion of the $f/\#$ cone that is present as a function of focal plate coordinate. Note, the cone narrows and the plate scale increases in the meridional plane, which means the circular fiber subtends less sky in that direction. Sagittal and meridional $f/\#$'s are plotted and averaged.

2.1.5 Ghosts

Ghost reflections between the optical surfaces of the corrector, including lenses, M1, and focal array sensors are unavoidable. Management of the degrading effects of these reflections involves non-sequential ray tracing to determine the peak irradiance of ghost reflections, and quantization of the brightness of these ghost features on the focal surface for a given stellar input. Focal, pupil and sensor reflection ghosts are detailed in DESI-0358, which analyzes possible double reflections amongst all surfaces in the corrector. The brightest ghost results from a two-bounce reflection between the ADC lens elements. This feature has a diameter of $\sim 13 \text{ mm}$, or about 0.024 deg^2 on the sky. According to Hanuschik [3], near-infrared sky background flux is $1 \times 10^{-17} \text{ erg/cm}^2/\text{s}/(\text{sq arcsec})/\mu\text{m}$, or $400 \text{ photons/m}^2/\text{s}/(\text{arcsec}^2)/\mu\text{m}$ at $0.8 \mu\text{m}$. With an assumed reflectivity of 2% per surface, the 1575 brightest stars in the *Hipparcos2* I-band catalog will have a ghost reflection

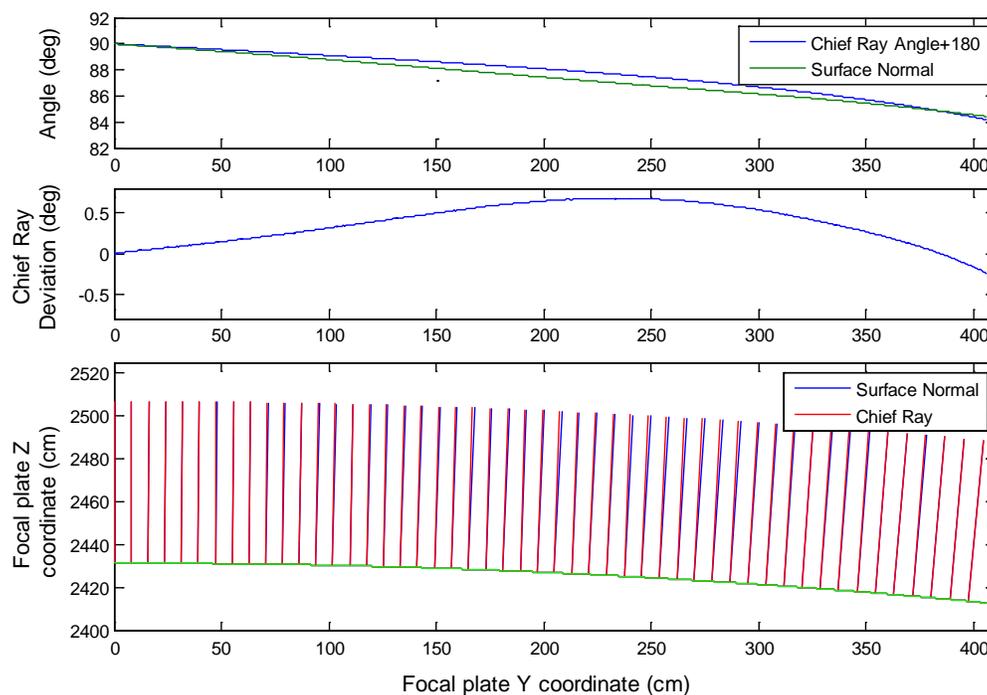


Figure 2.4: Chief rays are generally not normal to the local surface. The upper figure shows the absolute angle of the chief ray and local surface normal, while the middle figure shows the difference between the two. The bottom figure shows schematically direction of the ray deviation.

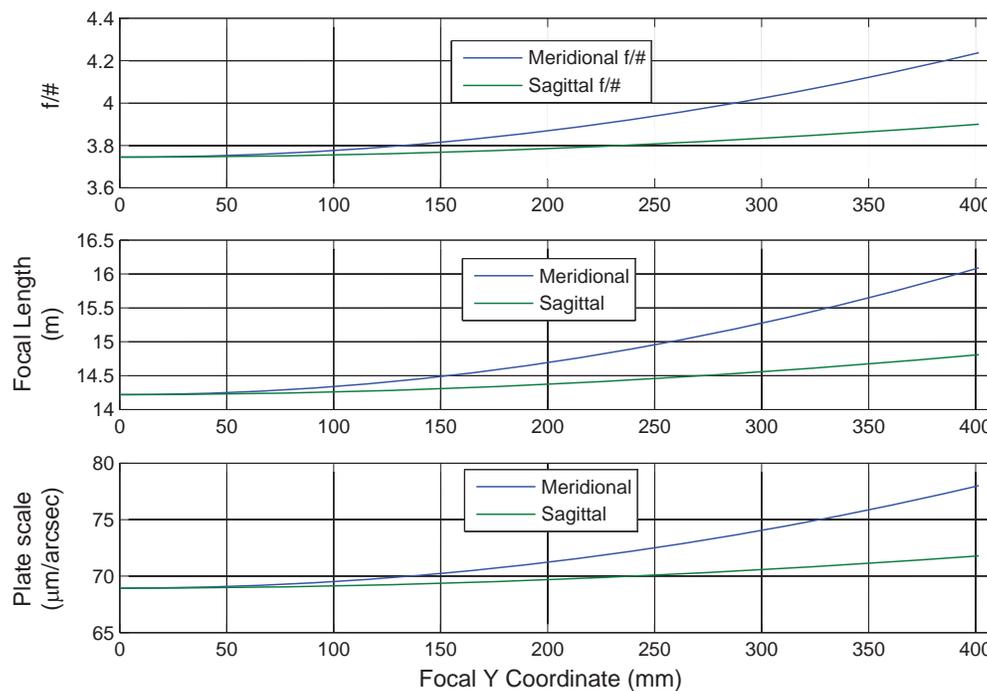


Figure 2.5: Anamorphic pupil distortion of Echo 22.

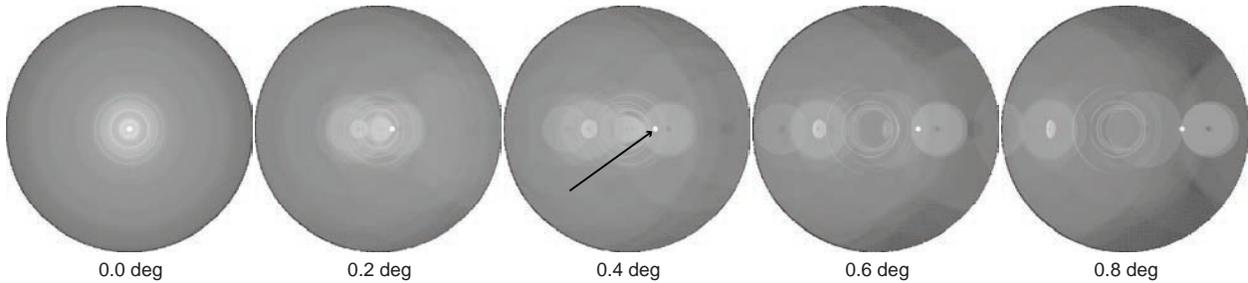


Figure 2.6: Images showing the complete set of two-bounce focal ghosts present at the Echo 22 focal surface for five field points. The arrow points toward the brightest focal ghost feature, a reflection between the two ADC lenses. In a 14,000 degree survey, reflections of the 1575 brightest stars along this ghost path contaminates 0.036% of the sky area with irradiance greater than 1% of NIR sky background.

greater than 1% of the NIR sky background. Aggregate area of these ghosts is 4.8 deg^2 , or 0.036% of the $14,000 \text{ deg}^2$ survey. The ghosts are shown at three field angles in Fig 2.6.

2.1.6 Corrector Lens Acquisition and Polishing

The DESI project has purchased the optical glass blanks and provided them to the chosen optical fabrication shop. Contracts have been issued to the optical fabricators with detailed instructions on final figure and surface quality specifications. Here we outline the main specifications for the blank procurement and the optical fabrication to meet blur requirements (see DESI-0338).

As described above, correction lens elements C1-C4 are made of fused silica, and atmospheric dispersion correctors ADC1-ADC2 are made of N-BK7. The materials for C1-C2 and ADC1-ADC2 are required to be homogeneous to 3 ppm and C3 and C4 to 4 ppm. Inclusions are expected to be less than 0.1 mm^2 in cross section and less than 0.28 mm in size (0.15 mm for ADC1-ADC2). Inhomogeneity introduces optical aberrations in much the same manner as a lens figure error by introducing a non-uniform optical path difference across the beam. Effects of inhomogeneity were modeled as random Zernike modes over limited bands, with magnitudes scaled to the maximum thickness of the lens, and specified inhomogeneity, in order to determine the effects of random inhomogeneity distributions in the lens substrate material. The magnitudes were then flowed into the specifications for all of the lens blanks. For the four of six lens blanks already procured, the actual measured homogeneity is analyzed in the Zemax corrector model and found to be sufficiently small enough to meet blur requirements.

All non-optical surfaces, edges, chamfers and flat faces are to be fine ground to a surface equivalent to a 600-mesh SiC loose abrasive surface texture, 1.5 to $2.5 \mu\text{m}$ roughness amplitude. All optical surfaces are to be ground to a better than 320-mesh SiC loose abrasive surface texture, $8 \mu\text{m}$ roughness amplitude. There shall be no hairline, conchoidal or other fractures or gouges in any surface.

The axis of rotation of the figure of revolution should pass through the mechanical axis of the lens with an error not exceeding 0.1 mm. The tilt between the two lens faces surfaces should not be more than 0.1 mm (across the diameter) and the run out between the two surfaces should not be more than 0.1 mm.

The diameters are to be ground to size, but the lens faces require additional material left on for the optical fabricator to fine grind and refine the surface prior to polishing. The amount of material to remain is to be left to the optical fabricator but it is not more than 1 mm nor less than 0.5 mm per face.

The optical surfaces shall be polished to a 2 nm Ra surface texture or better. The Ra is to be measured at 50 mm intervals from center to edge using a Wyko RST 500 or similar type of non-contact surface profiler. Test results are to be given over a 1 mm² area of surface. The scratch dig allowance shall be over the entire clear aperture. The allowance will vary from optic to optic. Surface form and tolerance on radius of curvature will be stated for each optical surface. Tilt, decenter and wedge will be stated for each optical element. Clear instructions are given on the marking of the maximum wedge angle position, as it is very important to know this for the alignment of the complete system. A detailed test procedure including any ray trace models for each optical surface has been supplied by each respective vendor.

The lenses will be coated to maximize system throughput. Based on the experiences of DECam, the lenses will be coated with hard multilayer coatings.

2.2 Corrector Mechanical Design

The six lenses of the DESI optical corrector require mounting into their respective lens cells, which then are mounted into the barrel of the camera. The four lenses C1-C4 will be mounted in individual cells with flexure systems to provide essentially athermal performance. The two atmospheric dispersion corrective lenses ADC1-ADC2 will be housed in rotating cells.

The total decentering and tip/tilt specifications for the lenses and Focal Plane are outlined in the first part of Table 2.4 (DESI-0612). The static tolerance, columns 4 and 5 in the table, refer to the maximum errors introduced in the process of aligning the cells in the barrel. The dynamic tolerances, columns 6 and 7, refer to the barrel deflections plus the errors introduced by the ADC rotation mechanism. These performance requirements apply over a range of Zenith angles from 0 to 60°. The total tolerances in the table are subdivided into allocations for the barrel and the cell subassemblies, which is detailed in DESI-0335.

The second part of Table 2.4 contains the barrel material, weight limits for the barrel and the cells, and the assembly/disassembly repeatability. The barrel and cage mass specifications are from DESI-0617. Table 2.5 shows the specification for the cage and the hexapod that are relevant for this writeup. These specifications are also from document DESI-0617.

2.2.1 Lens Cells

The lens cell provides the interface between the lens and the barrel of the wide field corrector. Lenses can be mounted to the cell in a variety of ways. One of the simplest is to use an elastomeric mount where the lens to cell interface is an RTV (room temperature vulcanized) rubber-like material. RTV rubbers have much higher coefficient of thermal expansion (CTE) values than typical glass and metals, with common materials ranging from 200 to 300 ppm/°C. RTV rubbers are essentially incompressible, and exhibit varying effective stiffness and CTE, depending on boundary conditions (constrained and free surfaces determine where the rubber can expand under load). Elastomeric mounts can be made to be essentially athermal with a suitable choice of elastomer thickness (i.e., there is little induced stress in the components with temperature change). This solution has been adopted by several of the current large wide field correctors on telescopes such as the Blanco, CFHT, LBT and MMT.

The design chosen for DESI is to use discrete pads of RTV for both radial and axial support (Figure 2.7). This method, which was adopted by both the MMT and DECam projects, has the advantage that the pads can be manufactured to high dimensional accuracy and consistency before mounting. The pads can be connected to inserts, made of the same material as the cells, which are inserted through holes in the side of the lens cell and screwed into place. The pads themselves

Table 2.4: Alignment and deflection requirements on Lens cells and Focal Plane, weight requirements on Barrel/Cage and Cells and assembly/disassembly repeatability requirements.

Element	Total tolerances		Static tolerances		Dynamic tolerances	
	Lateral ($\pm\mu\text{m}$)	Tilt ($\pm\mu\text{rad}$)	Lateral ($\pm\mu\text{m}$)	Tilt ($\pm\mu\text{rad}$)	Lateral ($\pm\mu\text{m}$)	Tilt ($\pm\mu\text{rad}$)
C1	200	123	20	18	50	45
C2	75	176	20	22	15	53
ADC1	200	250	20	25	75	113
ADC2	200	175	20	25	75	68
C3	100	180	20	24	45	54
C4	200	105	20	19	50	14
Focal Plane	150	92	20	25	40	25
Barrel material	Carbon Steel					
Telescope top end mass	10,700 Kg					
Mass of outer ring/spiders/cage/ /hexapod/barrel	$\leq 7,000$ Kg					
Mass of cells/base rings/spacers	≤ 560 Kg					
Barrel assembly/disassembly repeatability	$\pm 5 \mu\text{m}$ per flange					
Flange flatness	15 μm					
Flange parallelism	15 μm					

Table 2.5: Relevant Cage and Hexapod requirements (DESI-0617).

Item	Current Design
Cage outer diameter	1.8 m
Hexapod resolution:	
Lateral motion	15 μm
Axial motion	10 μm
Tip, tilt and twist	2 arcsec
Roll	3 arcsec
Hexapod range:	
Lateral range	± 8 mm
Axial range	± 10 mm
Tip, tilt range	± 250 arcsec

are either glued to the lens with a thin layer of RTV (radial pads) or just pressed against the lens (axial pads). For each case the RTV will exhibit different properties, and this is taken into account in the design.

The cell material is an important choice in the design, since it affects the thickness of the radial pads, as discussed below. The radial pad thickness should not be too great, as this means the lens will not be held stiffly under a changing gravity vector. The thickness also should not be too small (less than ~ 1 mm) as this poses problems for attachment to the inserts.

Thermal stability is a key issue in the design. Ideally the lens cell would be made of the same material as the barrel, so that the expansion and contraction with temperature change is matched.

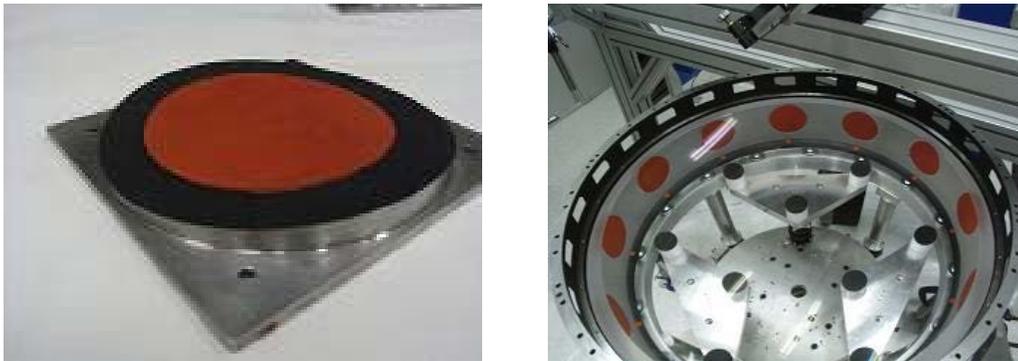


Figure 2.7: Mounting of the DECam optics. Shown at left is a pad and insert, and at right the radial and axial pads attached to the lens.

The choice of the barrel material is based on cost, ease of production and weight. In the DESI case the preferred choice of barrel material is steel. Steel, however, has a large coefficient of temperature expansion (CTE), ~ 12 ppm/ $^{\circ}\text{C}$. This is greatly different from that of fused silica, with a CTE of 0.5 ppm/ $^{\circ}\text{C}$, and somewhat different from that of N-BK7 with a CTE of 7.1 ppm/ $^{\circ}\text{C}$. If steel were used for the cell as well as the barrel, a strictly athermal cell design for a fused silica lens might require a thick layer of RTV (~ 9 mm) to compensate for the difference in CTE (though a thinner layer could be used as long as the thermal stresses stayed within certain allowances). This thickness would make it difficult to meet the system decentering tolerances.

An alternative material for the fused silica lens cell is nickel-iron alloy. This can have a low CTE, more closely matching the fused Silica CTE, allowing a thinner layer of RTV to be used in an athermal design. Invar is a well known nickel-iron alloy (36% nickel) with CTE of ~ 1 ppm/ $^{\circ}\text{C}$. However this choice of material for DESI fused silica lens actually leads to very thin radial pads (< 1 mm). An alternative is to use a nickel-iron alloy with a higher percentage of nickel. For DECam and the MMT designs, an alloy of nickel-iron with 38% nickel was chosen, giving a CTE of ~ 3 ppm/ $^{\circ}\text{C}$ which led to radial pad thicknesses of 1.4 to 2 mm. However, if Ni/Fe is used for the cell there will be a thermal mismatch between the cell and the barrel if the barrel is made of steel. To overcome this, a series of thin flexures can be used to connect the lens cell to the barrel. These flexures then compensate for the differential thermal expansion.

2.2.1.1 Lens Cell Design

A baseline design for the cells for the fused silica lenses is shown in Figure 2.8. It is similar to the one used for the DECam lenses with a few modifications. Both the axial and radial pads are mounted on inserts. These inserts can be precision machined and accurately positioned to meet the tight tolerances on the lens mating surfaces derived from the optical system alignment tolerances. The axial pad would be glued to the axial insert but not to the lens, whilst the radial pads would be glued both to the inserts and the lenses. A retaining ring and baffles would also be included; the retaining ring pads do not touch the lens so as not to over-constrain it. The Young's modulus of the pad is affected by both its S-factor and by whether the pad is glued either on one side or on both sides [4]. The allowable stresses in the lens is governed by the stress induced birefringence with a limit adopted of < 3 MPa. The target for the max cell stress is to be a factor of 2 below the yield strength (228 MPa). For C1, due to its position above the primary mirror, a safety factor of 4 would be required but this can be reduced to a factor of 2 for the stresses if additional backup safety constraints are installed on the cell (it is planned to install wire safety straps on cells connected

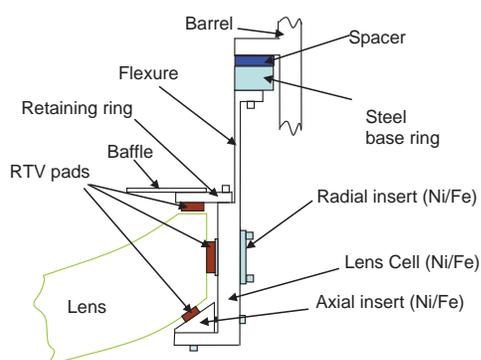


Figure 2.8: Schematic of fused silica lens cell design.

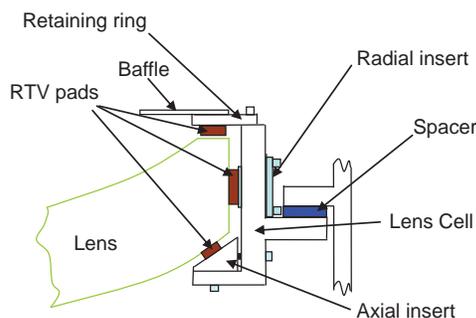


Figure 2.9: Schematic of N-BK7 lens cell design.

from the main body to the steel ring part of the cell).

The cell design for the C1 and C4 cells is slightly different to that of the C2 and C3 cells. The C1 and C4 cells have narrow slots (5mm width) between the flexures whilst the C2 and C3 cells have a more crenellated design with the gap between flexures being the same size as the flexure as in the designs for DECam. The thinner gaps for C1 and C4 allow for a stronger support for these heavier lenses and easier sealing of the cells to restrict airflow and dust ingress.

Due to the higher CTE of N-BK7 a steel cell design is proposed, yielding an athermal radial pad thickness of ~ 3.5 mm (Figure 2.9). This can meet the dynamic lens decentering tolerances. As both the cell and barrel structure are steel, the design does not need flexures between the two. Again the axial and radial pads are mounted on inserts.

2.2.1.2 Radial and Axial Pad Design

The axial and radial RTV pads provide the interface between the metal cell and the lens. The optimum radial pad thickness for an athermal behaviour can be calculated from equations given in Doyle, Michels & Genberg [5] and the thicknesses determined for each lens and cell are shown in the last column of Table 2.6.

The axial pads have two functions; one is to take up any irregularity of the lens pad surfaces (and hence lens cell surface) and ensure an even spread of the loading on the lens; the other is to be stiff enough to hold the lens so that a change in gravity vector does not produce too much tilt or decentering of the lens. (Of course the radial pads also provide a measure of resistance to tilt and decenter.) For DECam the axial pads for the C1 lens, which is directly comparable in size to the DESI lenses, were $10 \times 10 \times 1$ mm in size (S-factor of 2.5).

2.2.1.3 FEA Analysis

A finite element analysis (FEA) has been made of the lens/cell designs to investigate performance. The cells and barrel are to be assembled at 20°C and the survivability temperature range for the cells is -20°C to $+60^\circ\text{C}$. For survey operations the lens and cells need to meet the alignment requirements over zenith angles of 0 - 60° .

The FEA models used designs that were slightly simplified for ease of modeling. The radial pads are modeled as attached to a continuous cell and the axial pads are modeled as effectively stuck to the lens as well as the cell. This affects the value of the Young's modulus, which is accounted for by adjusting the material properties of the RTV. In all designs the cell wall thicknesses were 20 mm, the flexure lengths for the Ni/Fe cells were 42 mm, and the flexure thicknesses were 2 mm.

Figures 2.10 and 2.11 show examples of the FEA modelling results. Table 2.7 summarizes the predicted max stresses, tilts and decenters. These are small contributions to the overall budget in the requirements Table 2.4.

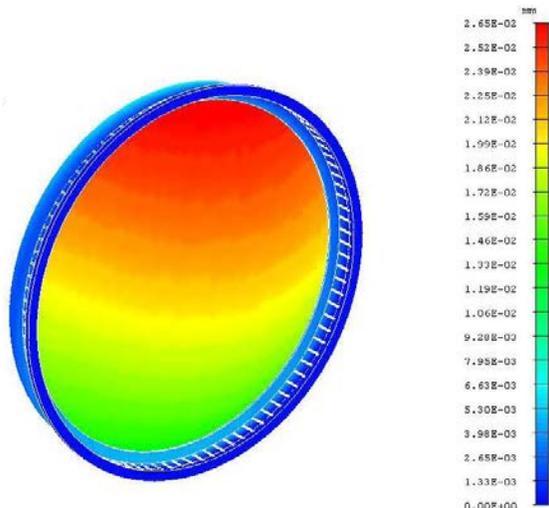


Figure 2.10: FEA model showing tilt of C4 lens and cell at a 60° Zenith angle.

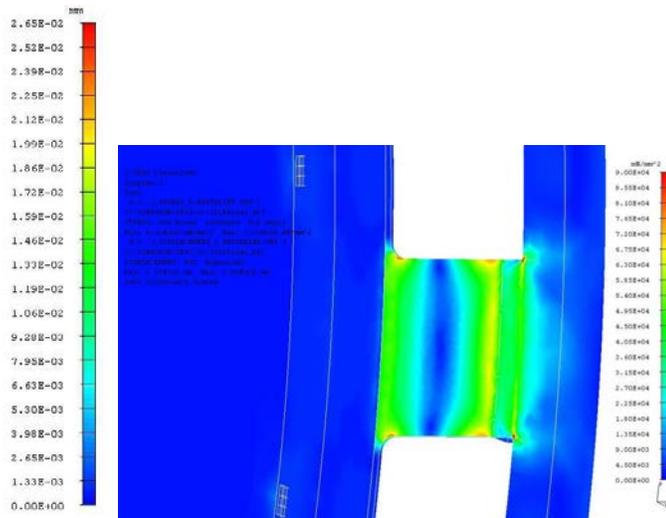


Figure 2.11: FEA model showing stresses in C2 flexure with a temperature change of 40°C.

2.2.2 Barrel

The details of the design of the barrel for the Echo 22 optics have been outlined in the document “Preliminary design of the DESI corrector barrel for the Echo 22 optics” [6]. Here we will summarize the main points of the design.

Three main concepts were followed in the design of the barrel:

- Use a single shell design as a way of using mass effectively (see DESI-0330) and to minimize primary mirror obscuration.
- Minimize the number of barrel sections. Right now the barrel has 3 sections (plus the Focal Plate Adaptor) in order to be able to insert one lens or ADC from either end of that section.

Table 2.6: Lens masses and pad parameters.

Lens	Mass kg	Axial Pad Size w, l, t (mm)	S Factor	No. Axial and Radial Pads	Radial Pad Size w, l, t (mm)
C1	201.3	10, 10, 1	2.5	48	32,32,2.17
C2	150.0	10, 10, 1	2.5	24	80,80,1.62
C3	83.2	10, 10, 1.5	1.67	24	45,45,1.60
C4	237	10, 10, 1	2.5	48	25,25,2.00
ADC1	101.9	10, 10, 1	2.5	24	60,60,3.50
ADC2	89.1	10, 10, 1.5	1.67	24	50,50,3.55

Table 2.7: Predicted lens cells stresses, lens tilt (across diameter) and lens and cell decenter tilt and decenters for 30° and 60° from zenith.

Lens	Max stress cell -40°C change MPa	Max stress cell 90° Zenith angle MPa	Lens tilt 60° Zenith angle μm	Lens and cell decenter 60° Zenith Angle μm
C1	91	5.8	12.7	6.0
C2	88	8.3	0.3	2.8
C3	76	4.1	5.2	2.3
C4	80	5.0	15.6	10.5
ADC1	<1.0	0.43	2.1	1.0
ADC2	<1.0	0.21	6.9	2.0

- Connect the hexapod through a single flange to the barrel. This reduces primary mirror obscuration and allows a cost, schedule and risk reduction by using essentially the same hexapod that were used in DES.

Figures 2.12 and 2.13 shows the barrel design for the Echo 22 optics. The order of the lenses from left to right is C1, C2, ADC1, ADC2, C3, and C4. The big flange in the middle is where the hexapod attach to the barrel, the last flange on the right is where the focal plane assembly attaches. The holes are shown open in the models in order to calculate deflections correctly, they will be covered in the real barrel.

2.2.2.1 Barrel Design

The current version of the barrel meets the general design concepts, the interface system requirements and the deflection requirements. The barrel design provides a minimum number of flanges and sections, a homogeneous shell thickness, and the interfaces for the hexapod and the cells.

The barrel consists of four main parts (left to right in Figure 2.12): the AFT section, the MID section, the FRONT section, and the SHROUD section. Also it includes an assortment of spacers for the C1, C2, C3, C4, ADC1 and ADC2 cells.

The After section (AFT section) is a thick shell which provides connection flanges on both ends and support rings for the cells. The shell provides six ports with an inner bore of 180 mm used to measure the lens spacing and also for final cleaning. The downstream flange is the interface connection with the Focal Plane Adaptor (FPD) and the upstream end provides the connection flange with the MID section. The AFT section is welded to the Hexapod Mounting Plate (HMP) which is the connection plate for the Hexapod System. The inner bore includes two thick rings welded to the shell used to support the C3 and C4 cell.

The Middle section (MID section) is the shortest section of the barrel which provides connection flanges on both ends similar to the AFT section and support rings. The downstream flange is used to connect the MID section to the AFT section and the upstream flange is the connection with the FRONT section. Two thick rings are welded to the inner bore to support the ADC1 and ADC2 rotating mechanisms. The overall length of the MID section covers both ADC1 and ADC2 lenses and the inner bore has a radial clearance of 86 mm to provide access during the installation of the ADC systems. A set of holes will be provided on the shell to accommodate the driver mechanism of the ADCs and the inner bore is optimized in order to leave a large volume for the ADC1 and ADC2 rotation mechanisms, see Figure 2.14.

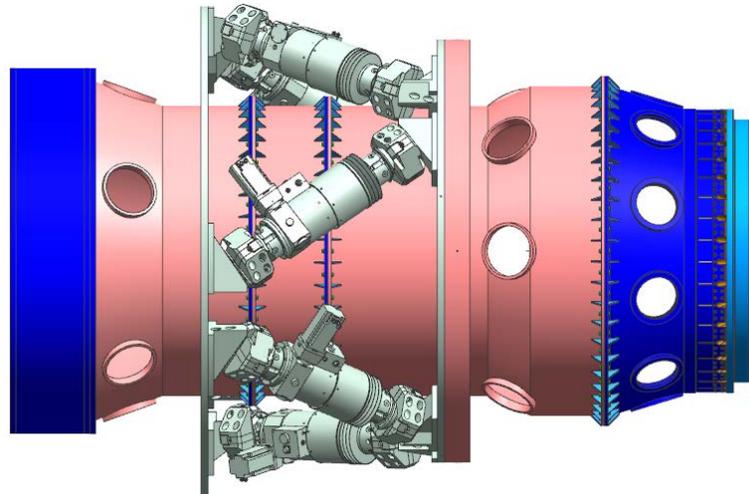


Figure 2.12: This picture shows the DESI corrector barrel with the DECam hexapod attached to the barrel. The hexapod configuration for the DESI barrel will be very similar to the one for DECam.

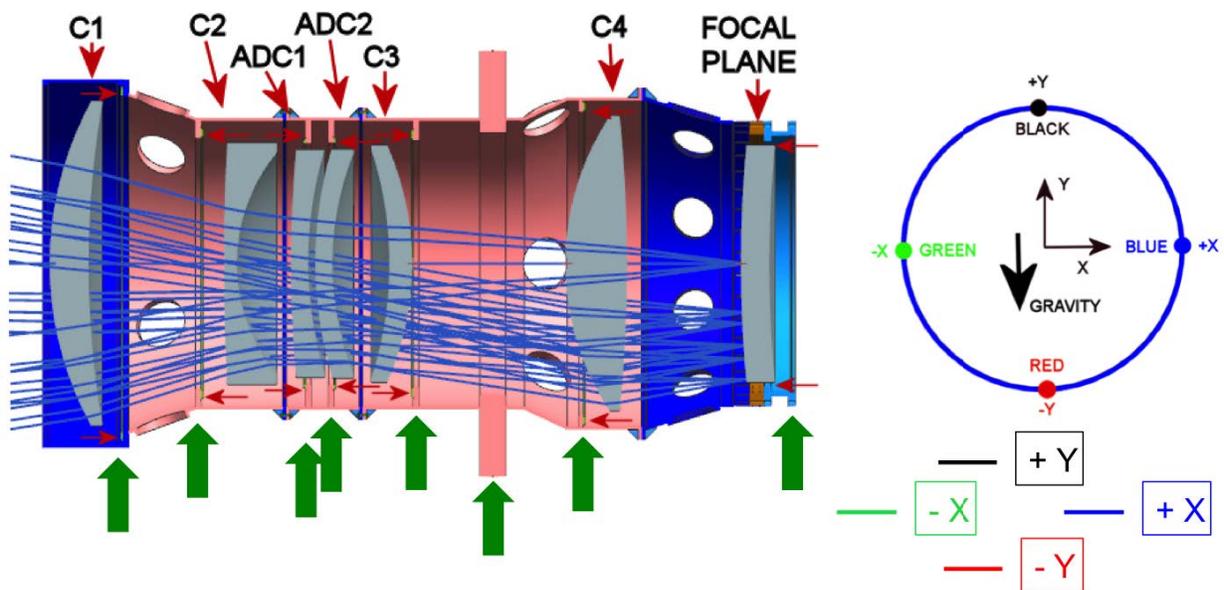


Figure 2.13: This figure shows the points that were tracked in the FEA analysis. Deflections were tracked at eight different planes located where the green arrows point to the barrel. In each plane four points were tracked as shown in the picture on the right hand side. The points are color coded as black +Y, blue +X, red -Y and green -X. This code was used in all the plots in this Section.

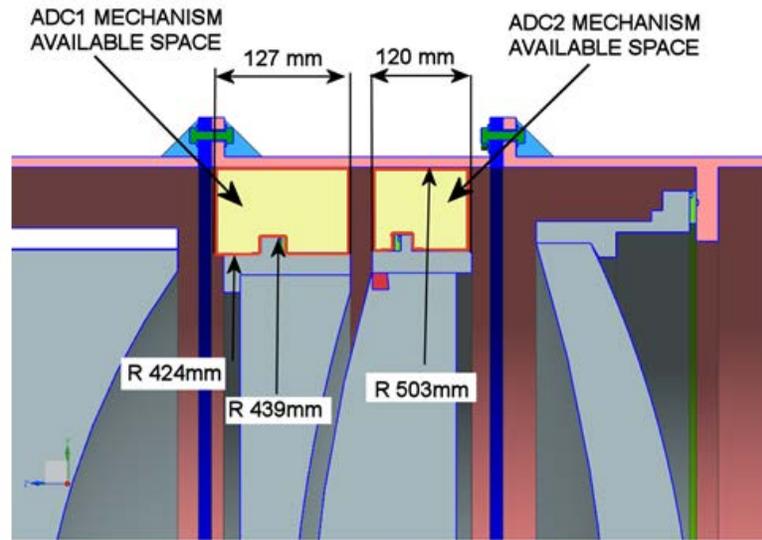


Figure 2.14: Available space to accommodate the ADC1 and ADC2 rotation mechanism.

The FRONT section consists of two welded pieces. The upstream piece has a conical shape where the large aperture is connected to the SHROUD section and the small aperture is welded to the lower FRONT section whereas the lower piece provides the connection with the MID section through a bolted flange. In addition the cone section provides six ports with an inner bore of 180 mm used to measure the lens spacing and also for final cleaning. A thick ring is welded to the end of the cone aperture and it supports the C1 cell.

The SHROUD section extends a few inches beyond the C1 cell with the purpose to protect the cell. Also the upstream side includes tapped holes used to install the protective cover. The other side is attached to the large side of the FRONT section cone through a bolted joint.

All the sections except the Shroud will provide a machined surface either on the outer surface or inner surface of the shell to be used as reference for the cell alignment process. Furthermore the AFT section will provide reference surfaces/holes to be used to align the FPD assembly to the corrector barrel.

The barrel shell was designed taking in considering the installation of the cells and the ADC rotating mechanisms. On the inner bore the radial contact width on the cell support ring is 38 mm for C1 - C4, 46 mm for C2 - C3, and 65 mm for ADC1 - ADC2.

All the bolted joints of the sections are designed with high stiffness using a single set of bolts. But to maintain an equal stiffness on different diameters the number of bolts has been changed, see details on Table 2.8. In addition to increase the local stiffness on behalf of high machining accuracy and low deflections the flanges are reinforced with gussets.

A set of tapped holes will be included on the barrel inner flanges to support the spacers and the cell base rings. The hole pattern will be very similar to the one used for DECam and it has been specified in DESI-0536. Barrel weights and materials are reported in Table 2.9.

As mentioned in the introduction the design of the barrel provides interfaces for the hexapod, the cells/lenses and the Focal Plane Assembly.

The hexapod is attached to the Hexapod Mounting Plate located within a range of ± 100 mm from the center of mass of the barrel with the purpose of minimizing the overall deflections. All the main components are included in the calculation of the center of mass such as the barrel sections,

the cells, the lens, the Focal Plane Assembly, see details on Table 2.10

All cells are designed to fit with the proper lens inside the barrel bore. Each cell surrounds the lens and provides the direct connection through bolted flanges to the barrel except for the ADC1 and ADC2 where the cell is supported by the rotating mechanism.

2.2.2.2 FEA Analysis

In this section we will describe the results of the FEA analysis. Using an FEA analysis program, deflections were tracked in eight different planes as shown by the green arrows in Figure 2.13. In each plane we tracked the deflections at four points. The points are also shown in Figure 2.13 in the plot on the right hand side. The points are color coded as black $+Y$, blue $+X$, red $-Y$ and green $-X$. This code was used in the plots shown in this Section. The plane tilt was calculated as the axial displacement of the top point minus the lower one divided by the diameter.

Figure 2.15 shows the results of the FEA analysis when the telescope is at 60 degrees from zenith and there is no rotation around the axis of the hexapod. The top left plot in this figure shows the vertical deflections calculated in the FEA analysis after subtracting the overall sag due to the deflections of the hexapod. The same deflections after an overall rotation of the barrel to make the average deflections at both ends equal are shown in the top right plot of Figure 2.15. The horizontal deformations are shown in the bottom left plot of the same figure. Finally the angular deflections after the barrel has been rotated are shown in the bottom right plot of Figure 2.15. Two other cases were also run in which the barrel was rotated 40 and 80 degrees around the axis of the hexapod. Due to the hexapod symmetry results will repeat after 120 degrees, so we studied three points between 0 and 120 degrees. The comparisons of the deflections of these cases with the specifications will be given in the following sections.

2.2.2.3 Comparing FEA Results with Specifications

In this section we will compare the FEA results of the previous section with the deflection requirements given in Table 2.4. The comparison of the FEA results for the barrel design with the specifications is shown in Figure 2.16 . In the figure, the full lens lateral and tilt requirements are shown with the light blue bars. The lateral and tilt requirements for the barrel due to barrel deflections are shown in blue. Then the barrel satisfies specs if deflection are inside the blue bars. The right hand plots are the same as the left hand ones but on a different scale. The top plots show the vertical deflections the lower ones the angular deflections. The black lines show the FEA results, that is the average of the deformations shown in the top right plot of Figure 2.15, for the vertical deflections, and the deformations shown in the lower right plot of the same figure for the angular deflections. We see that these black lines often lie outside of the blue bars. This is not a problem as the full camera can be rotated using the hexapod. This can be done because the optics only cares about deflections of the lenses relative to each other and to the focal plane. The green

Table 2.8: Bolted Joint Sizes.

	Bolt size	No. of Bolts	Joint Thickness (mm)
ADC1 Joint	M8	40	24
ADC2 Joint	M8	40	24
C4 Joint	M8	50	24

Table 2.9: Barrel Sections Weights.

Section	Weight (kg)	Material
1 FPA outer housing	31	Aluminum
2 FPA ring	15	Aluminum
3 FPD 1/8"	52	ASTM-A36
4 AFT section 3/8"	1052	ASTM-A36
5 MID section 3/8"	157	ASTM-A36
6 FRONT section 3/8"	209	ASTM-A36
7 SHROUD section	99	ASTM-A36
Total Mass	1615	

lines show the deflections after an over all rotation of the barrel as it would be performed with the hexapod. We see that in this case the the green lines satisfy the specifications. The values of the deflections given by these green lines are given in the third column of Table 2.11. Columns four and five of the same Table show the same FEA results but for the case in which the barrel has been rotated 40 and 80 degrees around its axis. We see that the specification are met in all cases.

2.2.3 Lens Cells and Barrel Alignment

Alignment of the six lenses of the DESI optical corrector will be achieved using mechanical and optical methods. The alignment of this corrector will be in keeping with the methods used for DECam corrector, which we will frequently refer to in describing the methods proposed for aligning the DESI corrector. Recall that corrector lenses C1–C4 will be mounted in individual cells with flexure systems, and atmospheric dispersion corrector lenses ADC1–ADC2 will be housed in rotating cells. The distances between optical elements will be controlled by steel spacers between the barrel shell segments, which can be ground to the required length.

2.2.3.1 Alignment of Lenses to Cells

The cells and the lenses will have to move relative to each other to facilitate central alignment. For adjustment in the x and y directions, a translation stage can be made from two sets of NSK Ltd. linear rails and bearings set at 90 degrees to each other mounted on flat plates. Lens movement in x and y can be accomplished with the aid of spring-loaded adjustment screws. The maximum travel required is of order ± 10 mm. Adjustment to the cell's translation can be made using push and pull screws mounted around the cell's periphery. These screws also can act as clamping bolts.

Moreover, the cells and the lenses will have to be aligned in tip and tilt relative to each other, and to balance any wedge angle that may have been introduced during the optical manufacture. On DECam, the fine adjustment mechanism consisted of LJ750 ThorLab jacks (capacity 90 kg). Each individual lens will require a different set of whiffletree plates for uniform support whilst being aligned. Nylon pads are to be mounted at the corners of the whiffletree plates and machined to the curvature of the optic. Viton[®] of 1 mm thickness will be glued onto the nylon pads to prevent damaging the lens surface. Handling fixtures will be required for the DESI lenses. These are expected to be similar to the DECam lens fixtures, which held the lens between two nylon rings that support the edges and face of the glass. These rings were bolted together using studding. Two aluminum plates were bolted to the nylon rings and held apart by aluminum posts. Later, after the lenses are mounted into their cells, the cells themselves can be used as lens handling fixtures.

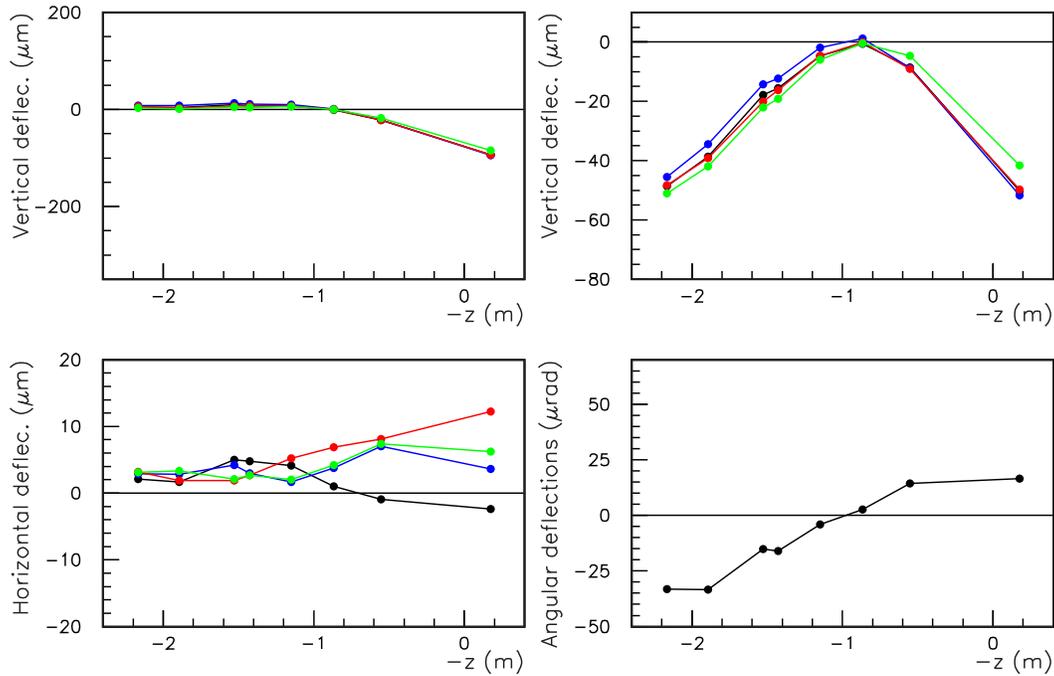


Figure 2.15: Deflections for the preliminary barrel design described in Section 2.2.2.1. The telescope is pointing at 60° from zenith and rotated 0° around the barrel axis. The plots show the vertical deflections produced by the FEA calculations after subtracting the sag due to the hexapod (top left), the same deflections after an overall rotation of the barrel to make the deflections at both ends equal (top right), the horizontal deformations (bottom left), and the angular deflections after the barrel has been rotated to make deflections at both ends equal (bottom right).

The measuring equipment required for the DESI lenses will be similar to that used for DECam alignment. Rotational symmetry and tip tilt will be measured using Sylvac digital dial gauge indicators mounted on adjustable stands. These indicators are repeatable to $1 \mu\text{m}$. Large bore gauges will be used to measure the distance between lens elements, along with a Faro Gage probe arm. Optical alignment measurements will be made using lasers, interferometers, CCD cameras and reference mirrors. A Micro-Epsilon laser sensor will be used to measure the placement of the RTV pads.

The alignment procedure is expected to be similar to that used for DECam. The first step is to align the lens with respect to a Rotary Precision Instruments air bearing table (10 tonnes capacity, sub-micron run out accuracy), to which is bolted a 1500 mm diameter aluminum plate.

Figure 2.17 shows the alignment setup for DECam lens C1. The lens is lifted using the handling fixture and soft slings. With the translation stage and bottle jacks bolted in position on the rotary table, the lens is lowered onto the support flanges of the jacks, which incorporate scratch-free load spreaders conforming to the optical surface. Thus supported, the lens may roughly be aligned simply by measuring from the translation stage to its rim. In an iterative process, by rotating the table and measuring the run out of the edge of the lens with the dial gauge indicator, adjustment to the lens position can be made using the translation stage and the Thorlab jacks.

Next the cell is raised into position and mated with the lens. Hydraulic jacks accomplish long distance travel and Thorlab jacks accomplish fine movement, monitored by dial gauges. As the cell nears its contact position with the lens, smaller and smaller increments (on the order of $20 \mu\text{m}$) are taken until the lens is seated on the RTV pads. As this is accomplished, the radial positions

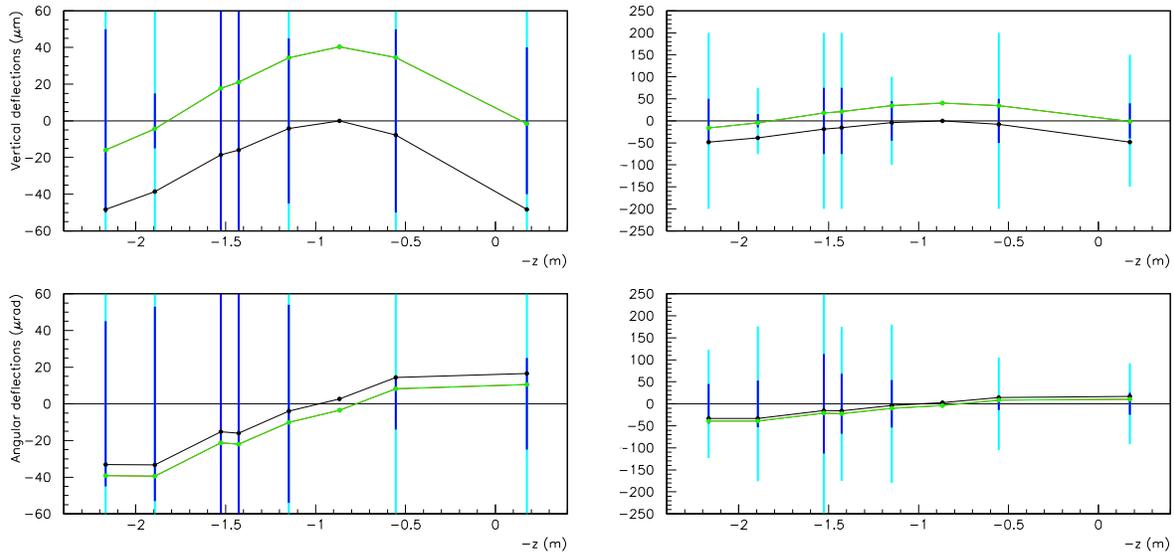


Figure 2.16: Comparison between requirements and the FEA analysis for the preliminary barrel design with the telescope pointing at 60° from zenith and a 0° rotation around the barrel axis. The full lens lateral and tilt requirements are shown in light blue. The lateral and tilt requirements due to barrel deflections are shown in blue. The top plots show the vertical deflections and the bottom plots show the angular deflections. The right hand side plots are the same as the left hand ones but on a different scale. The black lines show the average FEA results, the green line shows the deflections after an over all rotation of the barrel as if it would be performed with the hexapod.

of the lens and cell are monitored to maintain true alignment. Figure 2.18 shows the DECam C4 lens and cell alignment setup.

2.2.3.2 Alignment of Cells to Barrel

The procedure for aligning DESI cells to this barrel (DESI-0337) are similar to that employed on DECam. Using a large co-ordinate measuring machine, the FNAL-constructed barrel elements and UCL-fabricated lens cells will be carefully measured. Using data derived from these measurements, the cells are set at their optimal position for centering the lenses. The cells are drilled and doweled to facilitate their removal and subsequent replacement after the lenses are mounted in them. The accuracy of centering and realignment on the dowels is of order $\pm 10 \mu\text{m}$.

Doweled cells and barrel sections are shipped to UCL and the cells are aligned with their barrel sections. First, the main body and cells are aligned, then the cone and the main body and optics are united. Finally the two sections are combined. An optical laser alignment provides pencil beams used to check for any run out or tilt of the lenses. Elaborate checks are required to ensure that the laser beam runs true. The schematic in Figure 2.19 shows how the beams from the system are measured with a CCD camera. A crosscheck is made by mechanically measuring each lens as mounted into the barrel.

2.2.4 Hexapod

The hexapod system consists of six actuators, a mechanical joint with two degrees of freedom at both ends of each actuator, one stationary plate, a motion plate, and the control system. The system also comes with one spare actuator, the fixtures needed to change an actuator, and all



Figure 2.17: DECam C1 lens alignment setup.

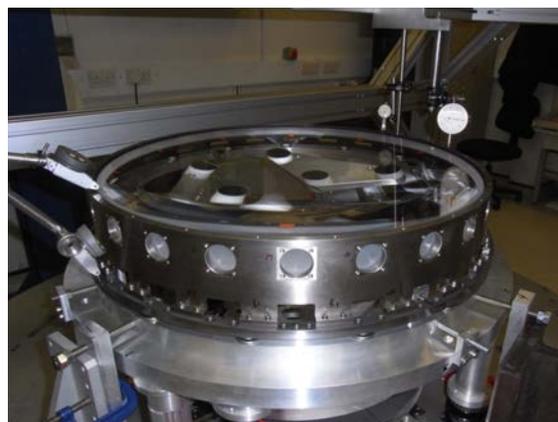


Figure 2.18: DECam C4 Lens and cell alignment setup.

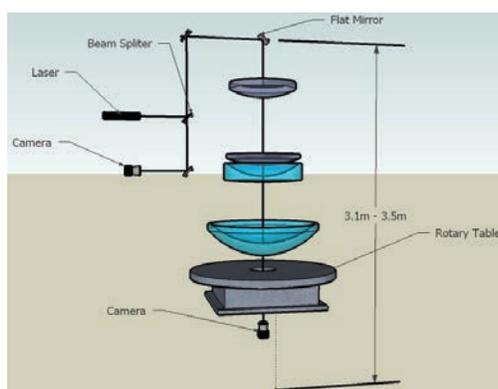


Figure 2.19: Laser alignment schematic.

documentation. The stationary plate bolts to the prime focus cage and the motion plate bolts to the barrel. The six actuators form three triangles. The triangle apex is located where two actuators meet at the motion plate. The actuators at the base of each triangle are attached to the stationary plate that is fixed to the cage. The hexapod effectively provides a three-point support to the motion plate.

The hexapod controller is equipped with manual controls to completely control hexapod motion in stand-alone, manual operation mode. The hexapod controller also has a remote operation mode. In remote operation mode, the controller is set up to move the hexapod according to the arbitrary position command it receives from a DESI control system. It is also setup to send hexapod operating status information to the same system in either the manual or the remote operating mode.

2.2.5 Prime Focus Cage

The Prime Focus Cage (PF Cage) is an assembly consisting of two end rings, a hexapod support structure and a cage shroud. The PF Cage will be attached to the telescope outer ring through a set of four fins as shown in Figure 2.20. All elements in the cage are made of low carbon steel.

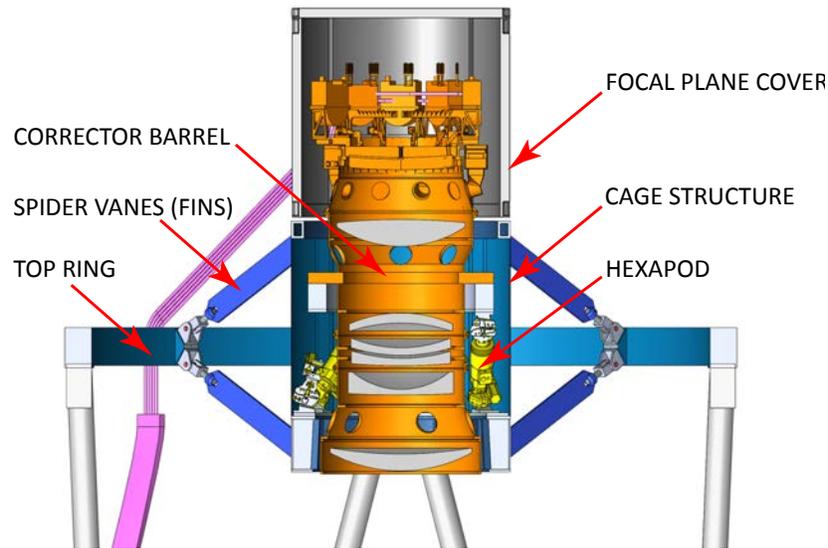


Figure 2.20: This figure shows the hexapod, the cage, the spider vanes (fins) and the telescope top end ring.

2.2.5.1 End Rings

The cage consists of a set of two end rings that interface with the ends of the four spider vanes. The outside circumferential dimensions of these rings match the original cage ring dimensions. These rings will be made out of steel. The rings will be attached to the fins with bolts and pins. Mating or attachment points between rings and fins will be left unpainted and protected with a light coating of grease. All other surfaces are painted with Aeroglaze[®] Z306 flat black paint for corrosion control. FEAs will be conducted to determine the appropriate ring cross-sectional configuration to best achieve the allowable assembled deflection as the cage moves through a varying gravitational loading.

2.2.5.2 Hexapod Structure

The hexapod structure is designed to provide support and attachment point for the barrel hexapod and to transfer the load to the cage.

The hexapod support structure will be fabricated from steel and coated with Aeroglaze Z306 paint. Mating faces will be left unpainted and protected with a light coating of grease.

2.2.5.3 Material and Coatings

The end rings, hexapod support structure, and covers are fabricated from ASTM A36 structural steel. The cage cover sections will provide wind and thermal radiation protection for the camera/corrector. Most surfaces are painted with an optical black paint as specified in the stray light analysis. The primer is Lord Corporation Aeroglaze 9947 and the top coat is Aeroglaze Z306 (flat black and low out gassing). Mating contact surfaces for the rings and fins are not painted. These surfaces are protected from corrosion by a light coat of grease.

2.2.6 Telescope Top End

The telescope top end consists of the telescope outer ring and the fins that attach the cage to that ring. Since DESI is not required to support operation of Cassegrain instruments, the inner flip ring in the original Mayall design is no longer required.

2.2.6.1 Spider Vanes

The spider vanes are of the same design as the fins in use on the Mayall telescope. The inboard end of the vanes are connected to the cage rails; the outboard ends are bolted to a bracket mount on the outer ring. The connection between each vane and the outer ring is the same connection type used in the Mayall telescope. Material for construction for the vanes is ASTM A36 structural steel. The current DESI design does not have the middle vanes used originally in the Mayall telescope as these were found to over-constrain the mounting system.

2.2.6.2 Outer Ring

The current two-ring system that attaches to the top of the telescope Serrurier truss will be replaced with a single fixed ring, saving 2250 kg in mass.

2.2.7 Prime Focus System Integration

As described above the lens cells are installed in the barrel assembly at University College London. This is then broken down into three barrel sections and shipped to the telescope. The barrel cage, hexapod system, fins, and upper ring telescope are shipped from FNAL to the telescope. At the telescope, the barrel section are reassembled and the completed barrel installed in cage-hexapod structure. The upper telescope ring and fins are install on the telescope, and then the barrel-cage assembly is installed.

Table 2.10: Cells, Focal Plane and Barrel section weights and center of gravity.

	Mass (Kg)	CoG Distance from (0,0,0) [mm]
C1	280	2294
C2	271	1750
ADC1	243	1523
ADC2	223	1414
C3	148	1228
HMP	870	745
C4	308	484
FP	707	-176
Barrel	1615	1393

Table 2.11: Tables showing the comparison between the specifications and the FEA results.

Element	Decenter $\pm\mu\text{m}$	Rot. around barrel axis		
		0°	40°	80°
C1	50	-15.9	-17.1	-18.1
C2	15	-4.4	-4.2	-3.2
ADC1	75	17.8	18.2	17.1
ADC2	75	21.2	21.4	20.4
C3	45	34.4	34.2	33.2
C4	50	34.5	33.3	32.2
FP	40	-1.7	-4.6	-5.7
Element	Tilt $\pm\mu\text{rad}$	Rot. around barrel axis		
		0°	40°	80°
C1	45	-39.1	-40.7	-40.7
C2	53	-39.2	-36.2	-35.8
ADC1	113	-21.3	-19.9	-19.9
ADC2	68	-22.1	-20.7	-20.7
C3	54	-10.1	-8.6	-8.7
C4	14	8.1	9.7	9.7
FP	25	10.6	12.1	12.1

3 Focal Plane System

The Focal Plane System (FPS) consists of three functional systems at optical focus:

1. Fiber Positioners each carry an individual science fiber to a unique target position for each observation.
2. Field Fiducials provide point light sources as references throughout the field for the fiber view camera.
3. Guide, Focus, and Alignment (GFA) sensors measure the telescope pointing as well as focus and tip/tilt of the focal surface.

These are supported mechanically in a Focal Plate Assembly, which attaches to the corrector barrel. The FPS also provides thermal insulation to block heat from escaping into dome air, thermal control to remove heat from the system, and service harnessing. An illustration of the focal plane system is shown in Figure 3.1.

The FPS also interfaces to several external systems:

1. Ferrulized fiber ends mechanically interface to the fiber positioners.
2. Fiber spool boxes mechanically interface to the focal plate assembly.
3. Corrector barrel mechanically interfaces to the focal plate assembly.
4. Cage assembly mechanically interfaces to the FPS thermal enclosure (FPE).

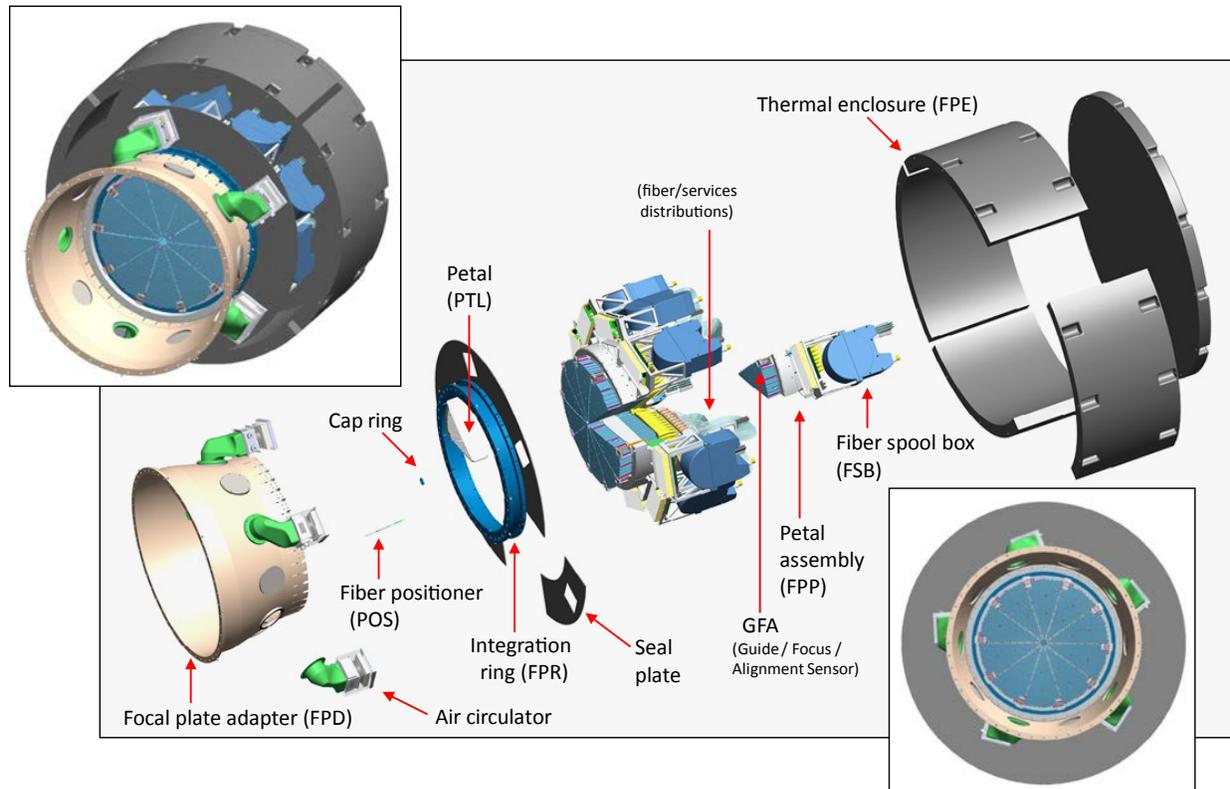


Figure 3.1: Illustration of the Focal Plane System. The Fiber View Camera, located at the primary mirror, is not shown.

Table 3.1: Focal plate key requirements.[†] Also see DESI-0455.

Item	Value	Rationale	Current Design
Number of fiber positioners supported within field of view	5,000	Science throughput.	5,000
Number of GFAs supported within field of view	10	Provides sufficient sensor area when using CCD 230-42 sensors.	10
Number of illuminated fiducials within field of view	≥ 60	Kinematics of fitting the field when viewed through fiber view camera.	120
Number of fiber management units supported	10	Logical distribution to 10 spectrographs.	10
GFA sensor radial position of active area	≤ 408 mm	Ensure sufficient bright guide stars and sufficient consistency of mode shapes.	407.2
Z deflection when at zenith	≤ 30 μm max (rel) ≤ 15 μm rms (rel) ≤ 100 μm max (abs)	Maintain figure of focal surface at worst-case gravity orientation. Do not unnecessarily consume hexapod focus range.	22.6 μm 9.8 μm 29.0 μm
Lateral deflection when oriented at 90°	≤ 10 μm max (rel) ≤ 5 μm rms (rel) ≤ 100 μm absolute	Maintain relative (x,y) positions of fiducials and fiber positioners. Do not unnecessarily consume hexapod lateral range.	2.0 μm 1.0 μm 12.2 μm
Radial deformation due to ΔT during an observation	≤ 10 $\mu\text{m}/^\circ\text{C}$ max	Maintain (x,y) positions during an observation.	2.5 $\mu\text{m}/^\circ\text{C}$
Normal deformation due to plate ΔT during an observation	≤ 5 $\mu\text{m}/^\circ\text{C}$	Maintain focus during momentary local heat loads.	0.5 $\mu\text{m}/^\circ\text{C}$
Plate ΔT during an observation	≤ 1 $^\circ\text{C}$	Thermal-mechanical stability.	0.7 $^\circ\text{C}$ max
Total focal plate assembly mass	≤ 870 kg	Ensure corrector barrel stiff and strong enough to support focal plane system.	674.5 kg
Heat load per observation	≤ 1000 kJ	Ensure practical sizing of cooling system (1 kW of cooling for a 1000 second observation).	516 kJ

[†]Positioner mounting requirements are handled separately within the positioner requirements table.

5. Instrument control system functionally interfaces to the fiber positioners, field fiducials, GFA, and thermal control system.
6. Fiber View Camera measures locations of the illuminated points provided by fiber positioners, field fiducials, and GFA.
7. Facility heat exchanger provides ambient temperature coolant to manifold on the FPE.

Requirements on the Focal Plate design are listed in Table 3.1.

3.1 Focal Plane Mechanical Design

The focal plate supports the fiber positioners, Guide-Focus-Alignment sensors (GFA), and field fiducials. The focal *surface* is a radially symmetric dome, defined by the corrector optical prescription; it is a definite geometric shape in space with respect to the corrector barrel. The focal surface is physically constructed of the science fiber tips and GFA active areas. The focal *plate* holds these items in position on the (virtual) focal *surface*.

The focal surface is 86.5 mm ahead of the front face of the focal plate. The “front face” is not a continuous smooth surface, but rather consists of 514 individual precision spot faces at which fiber positioners and fiducials mount (see Section 3.3.2.2). The focal plate itself is 82 mm thick at the edge, increasing to 103.5 mm at the apex of the dome. Behind the focal plate are supports for fibers and electrical services. Cooling service hardware attaches outside the perimeter.

The Focal Plate Assembly is built up of 10 radially symmetric sectors which are held in place by an Integration Ring around the perimeter. These sectors (or “petals”) are machined wedge-shaped objects, each supporting 500 fiber positioners, 10 field fiducials, and a GFA. On the rear side of each petal is attached a fiber guiding structure and a fiber spool box. These transmit the 500 individual fibers into a single cable, which is then routed down and off the telescope.

The integration ring attaches to the Focal Plate Adapter (FPD) via an FPD Ring. The FPD attaches to the rear-most flange of the corrector barrel.

The petals have precision mating faces to the integration ring, and are each bolted tightly to it. At the center of the assembly, two small Cap Rings transfer load between the petal tips.

The main support structures of the focal plate assembly are shown in Figure 3.2. To summarize, the Focal Plane System (FPS) consists of:

- Focal Plate Assembly
 - Focal Plate Adapter Assembly
 - * Focal Plate Adapter
 - * Focal Plate Adapter Ring
 - Focal Plate Integration Ring
 - 10x Focal Plate Petal Assembly
 - * Focal Plate Petal
 - * 500x Fiber Positioner
 - * 6-7x Field Illuminated Fiducial
 - * 1x Guide / Focus / Alignment sensor (GFA)
 - 3x GFA Illuminated Fiducial
 - * 500x Positioner Fiber Assembly **
 - * Fiber Spool Box **
 - * Fiber Focal Plane Guide **
- Focal Plane Enclosure
 - Focal Plane Thermal Shroud
 - Thermal control equipment, such as heat exchanger, etc.
 - Any electronics not on focal plane assembly, such as CPU, HV, etc.
- Fiber View Camera

Items marked ** above are elements of the Fiber System (Section 4), which are closely intertwined with the Focal Plane System.

Vibration is not expected to be a problem for the focal plate structure. The design is driven by achieving enough stiffness to control gravity-induced deflection, a body force. Therefore the modal stiffness is inherently high. For the flexured aluminum petals configuration, the finite element model had a first mode at 83.4 Hz. Differential motion between petals is also not expected to be a

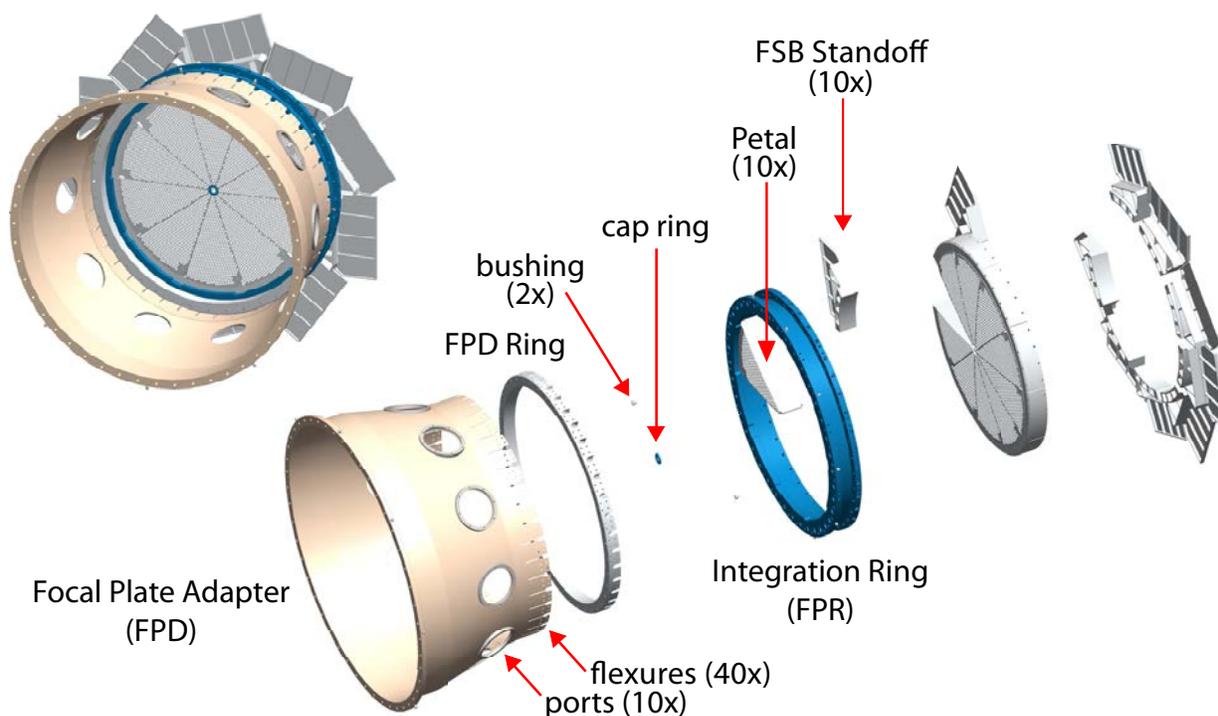


Figure 3.2: Focal plate assembly support structures. The focal plate adapter (FPD) and FPD Ring are permanently connected to one another. They form the FPD assembly, which is what connects the corrector barrel to the focal plate integration ring (FPR). Flexuring between FPD and FPD ring accommodates CTE mismatch between focal plate and barrel structure. The FPR supports the 10 petals. Each petal supports a standoff plate, where its fiber spool box (FSB) and control electronics are mounted.

problem. FEA results for petal-to-petal differentials due to thermal expansion were $< 1 \mu\text{m}$, and due to gravity orientation were $2 \mu\text{m}$. See DESI-0453.

Hexapod motions of the barrel impart reaction loads to the petals via the fiber cables. Measurements of fiber cable stiffness were made in summer 2014. From initial results, the magnitude of these loads will not contribute sensibly to the petal deflections. These loads will be included in the final FEA analysis.

3.2 Full-scale Demonstrator Petal

A full-scale, fully-detailed prototype petal was produced and surveyed. A photo of the petal is shown in Figure 3.3. This demonstrator petal was the culmination of several years of background work and development, including multiple iterations with vendors to understand manufacturing constraints and cost and performance drivers.

Additionally, subscale manufacturing samples to verify positioner mounting interfaces and per-hole machining costs / complexity were produced. These prototypes and tests are all very close to an expected final design.

Results from a metrology survey of the machined demonstrator petal are given in Table 3.2. Mounting hole angle is the most critical tolerance for throughput, and was held. The prototype did not meet the tolerances specified on hole diameter (worst case exceeded tolerance by $6 \mu\text{m}$) and hole location (worst case exceeded by $6 \mu\text{m}$). Additional test parts are being machined to assess

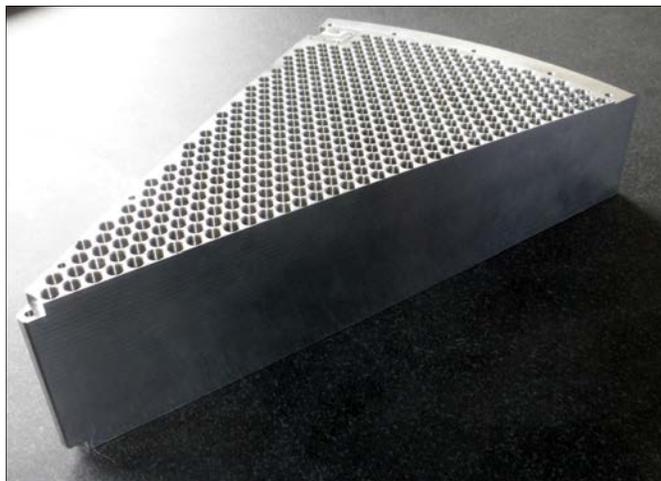


Figure 3.3: Full-scale, full-detail demonstrator petal.

whether these tolerances are fundamentally too tight to hold, or were just machined incorrectly in this one instance. Relaxing the tolerance on either hole diameter or location would consume some reserve margin on positioner close-packing. Relaxing the tolerance on the hole diameter would additionally affect positioner mounting angle error, and thus throughput. Neither is considered to be particularly problematic, as the errors here are relatively small. In either or both cases, a trade will be made to determine the best course.

Table 3.2: Hole machining accuracy on the demonstrator focal plate petal. 70 holes were surveyed.

Hole dimension	Tolerance	Max abs deviation	rms deviation
Angle (deg)	0.045	0.024	0.010
Diameter (μm)	15	21	16
XY location (μm)	60	66	34

3.3 Fiber Positioners

The focal surface is composed of 5,000 fiber tips. Each fiber is uniquely positioned by an individual robot, allowing rapid reconfiguration of the entire field for each observation.

3.3.1 Positioner Requirements

The basic requirement of the fiber positioner is that it consistently locate its fiber on target with accuracy $< 5 \mu\text{m}$. All 5000 fibers need to be in position in less than 120 seconds between exposures. In case this activity cannot be performed in parallel with other between-exposure activities, we require the positioner reconfiguration to be complete in 45 seconds. To close the loop on positioning, after each move the fibers are back illuminated and their actual positions are measured by the Fiber View Camera (see Section 3.6). Final accuracy may be achieved iteratively, so long as the time budget for the total number of iterations is not exceeded.

Positioners must be sufficiently robust to operate consistently for the lifetime of the project, have low mass, have low power consumption, and a sufficiently small mechanical envelope to fit 5,000 into the focal plane in non-vignetted light.

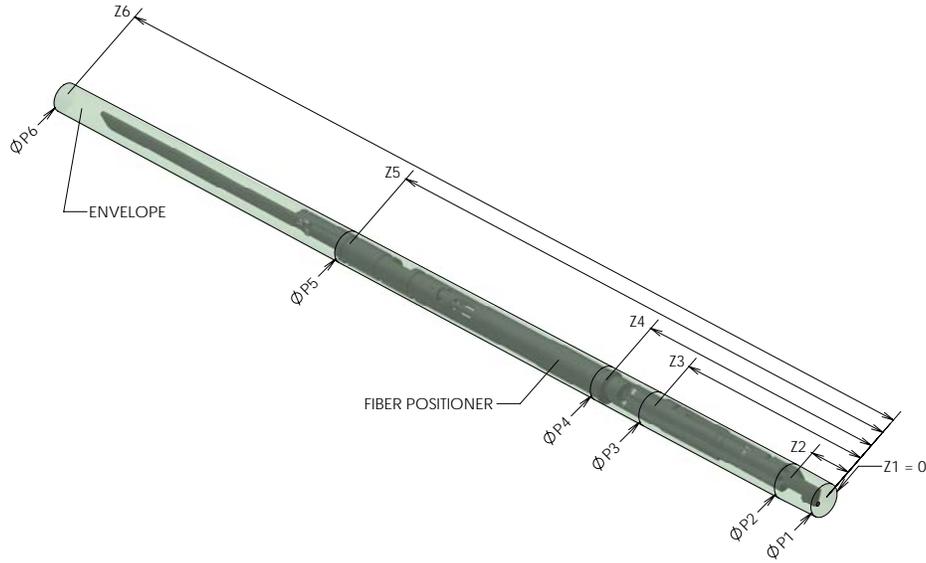


Figure 3.4: Mechanical envelope of fiber positioner, defined by several cones. Diameters p_k include dynamic and static tolerance stackups taken at axial positions z_k .

Table 3.3 lists fiber positioner requirements which have been developed to meet the science needs. These have been consistently met by multiple prototypes.

3.3.2 Positioner Interfaces

This section describes interfacing of fiber positioners to the focal plane system. This includes the subjects of mechanical envelopes and patterning of positioners, mounting, mass and materials, power and signal services, and thermal budget. Implementation of positioners is discussed separately, in Section 3.3.3.

3.3.2.1 Mechanical Envelopes and Patterning

The packing efficiency of fiber positioners on the focal surface must be sufficient to allow 5,000 within the unvignetted field. To pack positioners together as closely as possible without interferences, detailed knowledge of the positioner mechanical envelope is necessary.

We define the envelope as a rotationally symmetric volume, swept about the central axis of the positioner. This volume consists of a series of cones, which together form the total mechanical envelope for the positioner. This is illustrated in Figure 3.4.

At several key locations along the central axis, minimum pitch values (minimum center-to-center distance between neighboring positioners) are calculated. These define the diameters of the conic envelope. The minimum pitches are calculated as a Monte Carlo sum of nominal positioner dimensions, manufacturing tolerances, and the dynamic envelopes swept out during re-positioning.

Perfect hexagonal close packing of the fiber positioners is not possible on the curved focal surface. An algorithm for efficient packing was written to maximize the number of positioners within the unvignetted field, without neighbor collisions. The algorithm is:

1. Collect minimum allowed pitches p_k at several axial distances z_k from the focal surface.
2. Call the focal surface S_1 , and generate the several projected surfaces S_k below it at distances z_k .

Table 3.3: Fiber positioner requirements and key design points. Refer to DESI-0455 for the requirement rationales.

Item	Requirement	Value
gross moves (blind)	$\leq 100 \mu\text{m}$	25-30 μm max error
after correction move	$\leq 5 \mu\text{m}$	1-2 μm rms error (after a single correction)
lifetime moves	$\geq 372,000$	tested $> 400,000$ with no degradation
power peak	$\leq 1.2 \text{ W}$	1.38 W at 4 V, 2.84 W at 6 V (while moving, 250 μs sample)
power average	(secondary)	1.06 W at 4 V, 2.22 W at 6 V (while moving, 100 ms sample)
energy per observation	$< 30 \text{ J}$	3-11 J at 4 V, 5-21 J at 6 V
focal ratio degradation (rms)	0.2° rms	0.15° max Δ FWHM at f/3.75 over full patrol disk in repeated tests
focal ratio degradation (max)	0.4° max	0.14° additional offset after 400,000 moves of positioner
dynamic defocus error	$\leq 30 \mu\text{m}$	2.7 μm rms measured over full patrol disk
defocus mounting error	$\leq 20 \mu\text{m}$	15 μm anticipated (set by butting against one stop in tooling jig)
dynamic tilt error	$\leq 0.05^\circ$	0.011° rms measured over full patrol disk
max tilt error	$\leq 0.1^\circ$	0.047° max measured dynamic + 0.05° mounting (estimated)
operational temperature	-10°C to +30°C	tested -10°C to +42°C
survival temperature	-20°C to +60°C	$< -30^\circ\text{C}$ during operational test several times, not tested +60°C yet
total reconfiguration time	$\leq 45 \text{ sec}$	$< 20 \text{ sec}$ to reconfigure an array of 500 positioners
shaft speed	(secondary)	178 - 234°/sec (depends on motor vendor gear ratio)
mass	$\leq 50 \text{ g}$	30 g
fiber handling radius	$\geq 50 \text{ mm}$	$\geq 65 \text{ mm}$
fiber routing	(secondary)	68 mm free from ferrule to central axis, then gentle path through
hard travel limits	required	both directions, both axes, ok to ram at full speed/power
positive retention	required	M8.7 thread (like a sparkplug)
mating references	(secondary)	precision flange and cylinder on central bearing
thermal expansion	(secondary)	6061 aluminum; matches focal plate and GFA / fiducial supports
electrical connector	n/a	5 pin Samtec, mates one way
communication	n/a	standard CAN bus
power supply	n/a	+5 VDC nominal (4-6 V acceptable)

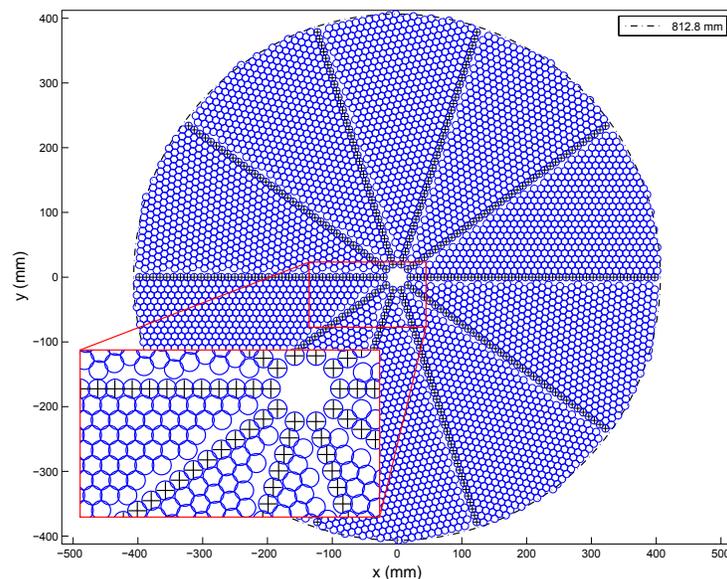


Figure 3.5: Typical output of fiber positioner patterning algorithm. Closeup view near center of the field is inset. “+” signs indicate locations where additional special constraints have been applied.

3. Project a flat hexagonal pattern (which is slightly too tight) onto S_1 .
4. Project the flat pattern to the surfaces S_k .
5. Iteratively:
 - (a) Select positioner i of the array.
 - (b) For positioner i , select the worst interfering neighbor j , considering all surfaces.
 - (c) Nudge i slightly away from j .
 - (d) Increment i .
6. Convergence is when for all surfaces S_k , all center-to-center pitches $\geq p_k$.

A top view plotting the typical output from the algorithm is shown in Figure 3.5. The field is composed of 10 identical wedge patterns, arrayed about the central axis. Additional constraints were simple to include in the algorithm. For instance, in Figure 3.5, locations marked with a “+” sign have additionally been constrained to lie along straight radial lines. This ensures a clean separation between wedges.

3.3.2.2 Mounting

Fiber positioners will be mounted in a hole plate, discussed in Section 3.1. At each hole the plate provides a precision bore for tip/tilt and lateral positioning, and a precision spotface for transverse (focus) positioning. Machining samples have been made and surveyed in multiple materials (6061-T6 aluminum, 4140 alloy steel, and CE Al-Si alloy) by multiple vendors to confirm tolerances. Two such samples are shown in Figure 3.6(left). Positioners are positively mechanically locked by a threaded “sparkplug” style feature shown in Figure 3.6(right), which has been tested and is attractive for its simplicity and machinability.



Figure 3.6: Left: Drill test blocks for positioner interface in 6061-T6 aluminum (rear) and 4140 alloy steel (front). Hole sizes, spacings, and tilts were machined at correct scales. Right: Section of a machining sample of the “sparkplug” style positioner retention feature. A typical precision bearing cartridge from an eccentric axis positioner is shown mated in the threads and registering below to the precision bore.

3.3.2.3 Mass and Materials

The focal plate can stably and accurately support significant loads, allowing some freedom in the mass of positioners. The plate is designed to support positioners up to 50 g each, totaling 250 kg for the system of 5,000. The plate mass inherently provides significant thermal capacity, such that the brief heat loads generated by moving positioners between observations are readily absorbed without significantly affecting plate geometry.

3.3.2.4 Fiber, Power and Signal Services

In addition to distribution of science fibers, power and signal must be routed to the individual positioners. These 5,000 sets of fibers and wires are of narrow gauge and thus take up little total volume; to avoid a nest of complexity, however, their routing requires a consistent and organized approach. The first level of this organization occurs naturally at the division into 10 petals, which immediately and logically reduces the complexity to 500 sets of services. From this point we dispatch fibers into 14 furcations of 36 each. Each furcation then divides into 3 smaller groups, where each group services 12 individual positioners (really 4 of these 42 groups will service only 11 positioners). This is illustrated in Figure 3.7.

The electrical services logically follow the fibers’ distribution. On each petal, the 42 groups (14 furcations x 3 groups) are serviced in 7 transverse rows. Each row has a printed circuit board with individual electrical connectors to the positioners in their groups of 12. These boards plug into a main service board by a robust connector with backup screws.

The PCB on each row is mechanically supported by a stiff transverse aluminum rail. The positioner connector groups are placed in alternation with fiber fanout hardware, also mounted to the rail.

In summary, this service organization scheme reduces the potential complexity of fiber and electrical distribution from 5000 to only 12 positioners at a time. Moreover, every group of 12 positioners is serviced in a standard and repeatable way, by identical electrical and fiber support hardware.

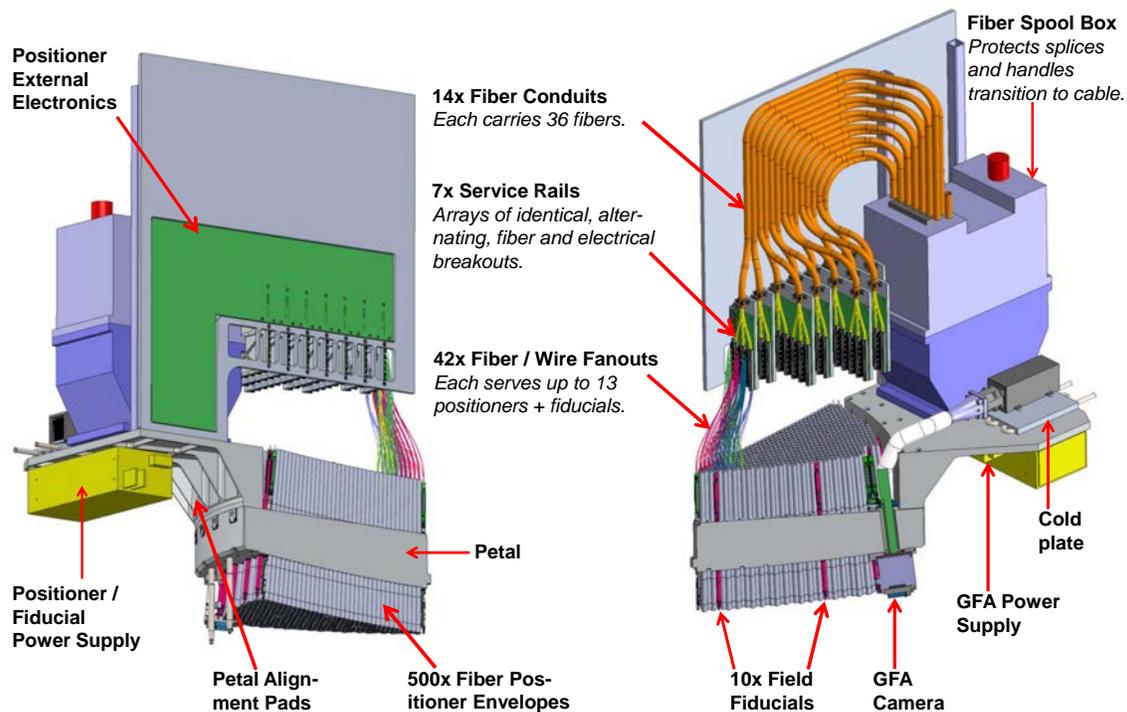


Figure 3.7: Illustration of completed petal assembly with fiber positioners, fiducials, GFA, and fiber spool box. This is a single unit ready for loading into the integration ring.

3.3.2.5 Thermal budget

Due to the heat capacitance of the focal plate structure, the system is insensitive to the particular step profile of the heat outputs of the fiber positioners. These are relatively momentary compared to the length of the observation. The momentary heat impulse during re-positioning is smoothed by the plate capacitance and gradually removed over the course of the observation. Control electronics are shut down during observation such that positioner power consumption is effectively zero when not moving. A total of 30 J each is allotted per observation cycle. The cooling system will be sized to these allotments, though it is noted that current positioner prototypes have total energy usage < 11 J per reconfiguration.

3.3.3 Positioner Mechanical Design

The DESI fiber positioner has eccentric axis kinematics and is sized for a 10.4 mm center-to-center pitch. Actuation is by two $\phi 4$ mm DC brushless gearmotors. Each positioner has one electronics board attached to the rear. This board accepts a DC voltage for power and CAN messages for communications and then drives the two motors. Power is shut off when the positioner is not operating. The positioner mounts to the focal plate petal by screwing it into a threaded hole like a sparkplug.

Prototypes are fast ($180^\circ/\text{sec}$), accurate (1st move error: 10-13 μm rms, 25-30 μm max; 1st correction error: 1-2 μm rms, 4-6 μm max), and robust (tested to 400k reconfigurations with no degradation in performance). One of the prototypes is shown in Figure 3.8 and the individual components are shown in Figure 3.9. Plots of positioning accuracy measured in a typical prototype are shown in Figure 3.10.



Figure 3.8: Prototype of the DESI 10.4 mm pitch fiber positioner.

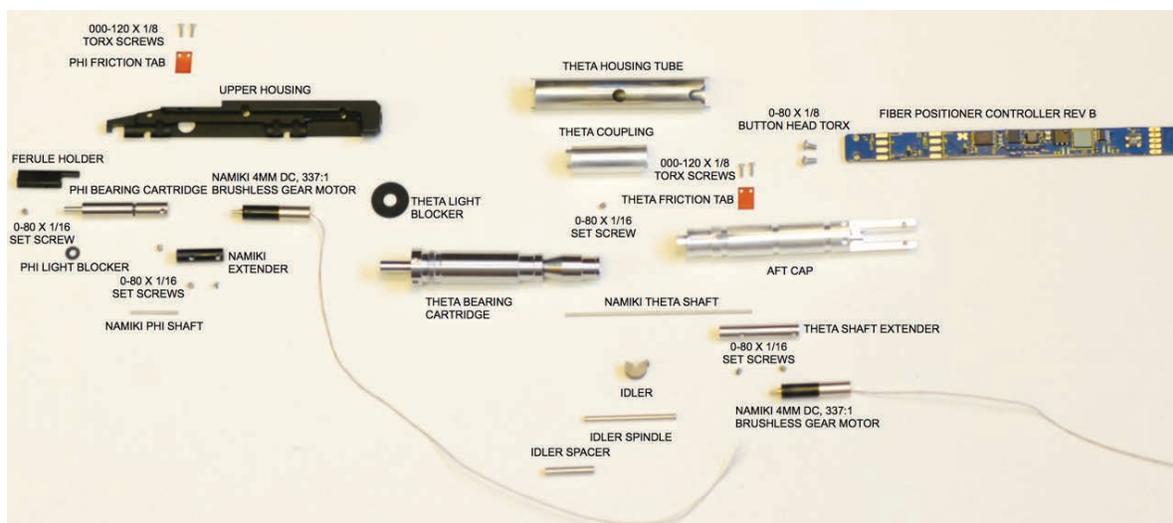


Figure 3.9: The components of the DESI 10.4 mm pitch fiber positioner. The design is based on commercial off the shelf $\phi 4$ mm DC brushless gearmotors.

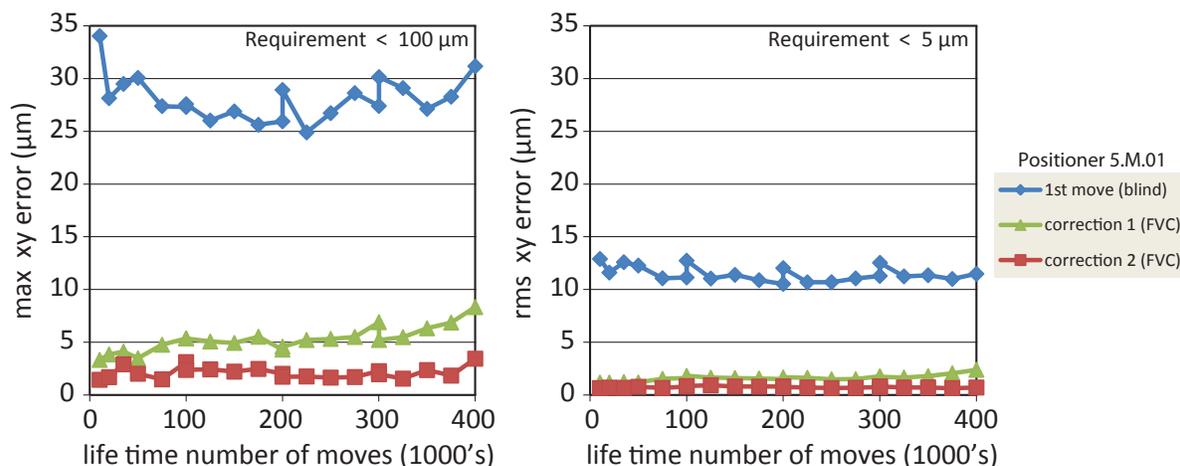


Figure 3.10: Positioning accuracy of prototype over a 400,000 move life time. The test is fully automated with a fiber view camera. The test takes place with continuous duty for over a month. The positioner met all requirements with comfortable margin throughout the life.

The positioner moves the fiber about a planar disk region. There are two rotational degrees of freedom, a central axis and an eccentric axis. These axes are parallel to each other. Often these axes are referred to as θ and ϕ . The kinematics and coverage are illustrated in Figure 3.11.

Each of the two motors directly drives an axis. There are no custom gears or off-axis transmis-

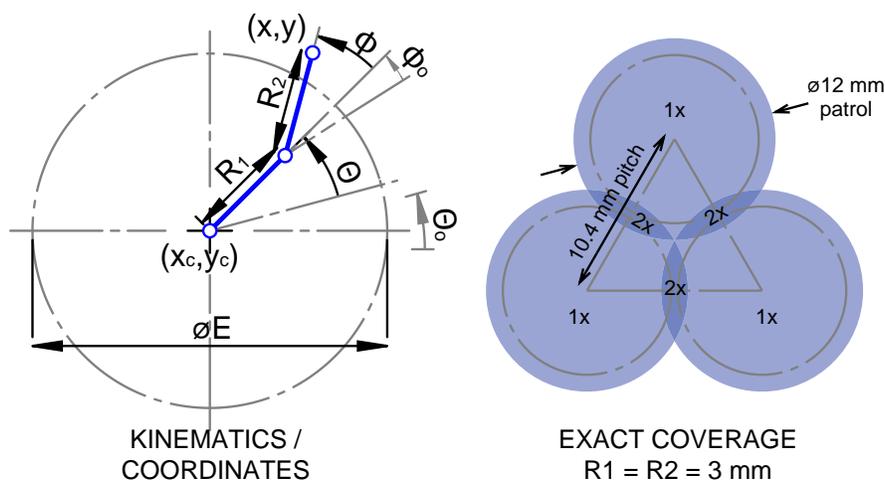


Figure 3.11: Left: Eccentric axis (“ θ - ϕ ”) kinematics and coordinate systems. Whenever R_2 is retracted within the dashed circle E , the positioner is guaranteed free rotation about θ without obstruction from its neighbors. Right: Patrol coverage regions for neighboring positioners. Regions labeled “1x” indicate coverage by a single positioner, “2x” by two positioners, and “3x” indicates three positioner coverage.

sions needed. The motors can be purchased from any of several vendors. Motors come from the factory with an integral gear head that has a reduction ratio of 256:1 to 337:1, depending on the particular vendor.

We control stiffness, run-out, and parallelism of the two rotational axes by two bearing cartridges (one for the θ -axis and one for the ϕ -axis). Each cartridge is a hollow cylindrical assembly containing two ball bearings and an internal shaft. The cartridges are mounted in-line with their respective motors’ output shafts. The cartridges are purchased as integrated units from a bearing manufacturer.

The positioner has mechanical hard stops in both directions of both axes. Either axis can be driven at full speed and power into either hard stop repeatedly and without damage. We have failed to produce any test in which repeated hard stop ramming caused any discernible damage.

The fiber ferrule is held by a ferrule holder arm. The arm secures the 1.25 mm DESI ferrule against a precise cylindrical mating surface. The ferrule is contacted by a nylon-tipped set screw under controlled preload, with a small quantity of adhesive at the threads and tip to lubricate the contact point during insertion and then to guarantee it cannot later loosen.

All the mating features for precision mounting and retention in the focal plate petal are machined into the central axis bearing cartridge. A cylindrical datum constrains tip / tilt and xy position. A flat flange datum defines focus. A thread provides positive and firm mechanical retention. These identical features are used on the assembly jigs that locate the eccentric axis bearing and the ferrule holder for each positioner. The features are illustrated in Figure 3.12.

3.3.4 Positioner Electrical Design

The two motors are driven by one electronics driver board attached to the aft end of the positioner. There is no encoder on either motor. The motors each have 3 coils and are driven by pulse width modulation of the current applied to its coils. The shaft position is controlled open-loop by rotating the sum magnetic field of the 3 coils.

For large motions, the magnetic field, and thus the motor shaft, is ramped up rapidly to a

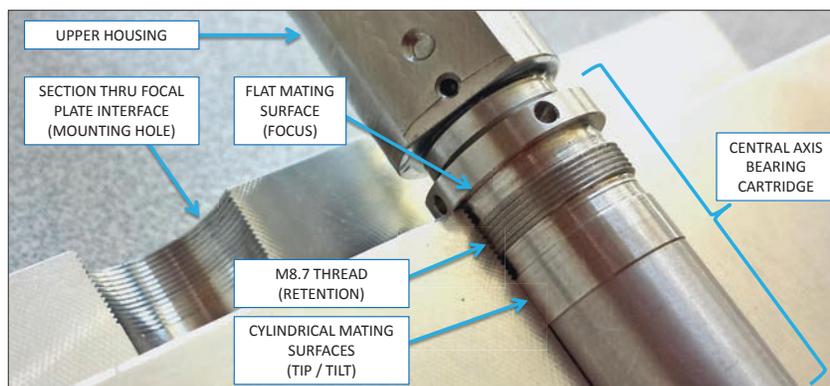


Figure 3.12: Positioner mechanical interface to focal plate. During insertion, the precision cylinder (g6 tolerance) of the bearing cartridge engages the precision hole (H7 tolerance) in advance of the threads. This keeps the threads well-aligned so that they engage smoothly every time.

rotation rate of 10,000 rpm. This is very fast in practical terms: $\sim 180^\circ/\text{sec}$ at the output shaft, depending on exact gear ratio. When re-positioning, the final $\sim 50 \mu\text{m}$ of the move is done at low speed (15 rpm) and very fine resolution (0.1° at the motor shaft, $\sim 0.0003^\circ$ at the output shaft). After positioning a shaft, the coils are completely de-energized and the position remains stable.

Electrical connection to each positioner is by a single connector with 5 wires. The connector is mechanically robust and is keyed so it can only be mated the correct way. Two lines of the five are for +DC power and ground. Two lines are for the CAN bus. The fifth line is for a sync signal so that multiple positioners' motions can be easily coordinated.

Each positioner is uniquely addressed by ID number, and can be physically placed anywhere on the CAN bus. Groups of positioners are connected in parallel, and in any order, to simple 2-line power and signal rails. This decoupling is advantageous at all levels of testing, integration, and maintenance.

The PCB is a 0.8 mm thick 6-layer board, with commercial components, to achieve the necessary small size. The low-level firmware is compiled C code. The firmware is compact ($< 6\text{K}$ bytes exclusive of tables) and has been thoroughly debugged and tested, including motor control and CAN communication. Figure 3.13 shows the prototype board.




Figure 3.13: Electronics driver board for the fiber positioner, which was laid out at University of Michigan. On the left side is the spring clip which retains the fiber. On the right the two holes are where the board screws to the aft end of the positioner. The board is 8 mm wide and has been carefully designed so that all components, connectors, and fiber pass easily through the focal plate interface.

3.3.5 Positioner Software

The array of positioners is controlled by a Linux computer, which communicates with each positioner by ID number over the CAN bus. The controller has software which keeps track of each positioner's status and shaft angles, and sends out move commands. The software to run a single positioner has been thoroughly debugged and tested. The external software interface is a single

object written in the Matlab language, with a complete set of external methods provided. All calibrations and parameters are set by a simple key/value list. The parameter values can be granularly set uniquely for each positioner, can be updated in real-time, and generally are typed and structured for ease of logging and simplicity of database configuration control. Control of an array of multiple positioners is established by making multiple instances of the object with the appropriate ID numbers.

One level of abstraction higher, there is software to coordinate the array of positioners. In particular, this software includes an anti-collision algorithm, since positioners can reach into their neighbors' patrol envelopes. This algorithm has been coded and debugged in simulation, but it has not been tested on a physical array. The simulation was run for 10^5 random configurations. Because of the $180^\circ/\text{sec}$ shaft speed, the maximum time to reconfigure the array including all anti-collision moves is 4 seconds, and the average is 3.6 seconds.

3.3.6 Fiber Interface

The positioner accepts the ferrulized and polished science fiber and provides a mechanically safe path through its internal mechanism. The fiber path is illustrated in Figure 3.14. The fiber is installed in the positioner, and the positioner is then inserted into the focal plate from the corrector side. A precision jig sets the placement of the ferrule tip with respect to those mechanical datums which contact the focal plate.

The integration of fibers into positioners is discussed further in Section 4.



Figure 3.14: Fiber route through the fiber positioner is illustrated by a thick red line. Ferrule holder is at the right, exit at electronics board is on the left.

3.4 Guide-Focus-Alignment

The guide, focus and alignment (GFA) system meets the following DESI requirements (see DESI-0526):

1. Provide guide signals to the telescope at 1 Hz to a precision of < 0.03 arcsecond and latency of < 0.5 second.
2. Monitor camera focus and alignment from at least three locations with approximately azimuthal symmetry.
3. Process and produce results from at least 50 defocused star images within 5 seconds.
4. Meet system environmental requirements from DESI-0583.
5. Determine accurate telescope pointing after slew within 20 seconds.
6. Determine camera defocus relative to M1 with better than $30 \mu\text{m}$ accuracy.
7. Determine camera tip/tilt relative to M1 with better than $10 \mu\text{m}$ accuracy.
8. Camera must operate in both full frame and region of interest (ROI) mode.
9. Determine the current telescope pointing within 20 seconds after telescope slew.
10. Guide cameras will deliver empty sky images for seeing and transparency determination.
11. GFA system must operate during all conditions in which the telescope can operate.
12. GFA system can operate in event that an overly bright star is in the field of view.
13. The guide cameras can be requested to deliver full frame images at any time.

Additionally, two design guidelines constrain the GFA design. These are

1. The GFA cameras will operate at ambient temperature to minimize local heating near the focal surface.
2. The GFA camera footprint will be approximately the footprint of the e2v CCD230-42 to minimize the number of science fibers displaced.

The GFA system contains ten nearly identical cameras divided into two groups: focus and alignment cameras and guide cameras. Each camera contains a single CCD sensor and is mounted and operated as a standalone instrument. Each camera provides all readout modes used in any GFA camera. The cameras vary only in optical filter mounted above the CCD. An essentially single development stream minimizes risk, development time and cost. Each camera operates without a shutter in frame transfer mode and is sealed with a broad range (red) optical filter. Each camera contains all CCD readout electronics and all camera control and requires only DC power and a gigabit Ethernet connection. USB connectors may also be provided for in lab testing.

3.4.1 Sensor Selection

The GFA system is required to operate at ambient temperature to minimize the heat load in and near the DESI optical path. This leads to a sensor requirement of excellent dark current performance. This, combined with the required sensor area, reduces the number of candidate sensors. The e2v CCD230-42 is baselined since it has excellent ambient temperature dark current performance and read noise. This sensor has excellent manufacturer support and several commercial astronomical cameras have incorporated it (e.g., Apogee Alta F and FLI Proline). The sensor provides four channel readout and can operate in frame transfer mode removing the need for an optical shutter. The frame transfer operation uses 50% of the sensor area leaving 9.4 cm² active area. The DESI plate scale varies with radius so that radial and azimuthal plate scales are slightly different. At the edge of the focal plane where the GFA camera is located the plate scale is $\sim 70 \mu\text{m}/\text{arcsec}$. The active area of each sensor provides $\sim 29 \text{ arcmin}^2$ of area on the sky.

The GFA system carries a risk that operating the sensor at ambient temperatures falls outside of the “normal” operating procedures for a CCD. In order to mitigate this risk, an FLI Proline ML23042 camera was obtained and tested. While the dark current proved stable and repeatable it was found to be significantly higher than predicted in the datasheet. e2v confirmed a mistaken scaling equation. Eventually e2v replied that the given data sheet formula of At 20 °C the dark current was found to be 140 e⁻/s/pixel ($\sigma = 11.8 e^-$). This is to be compared to a read noise of 20 e⁻/pixel in the FLI camera. Only on a rare summer night would we expect the sensor to approach 28(82) °C (F) producing a dark current of 400 e⁻/pixel.

3.4.2 Packaging

The ten GFA cameras distributed around the focal surface with one camera per focal plane petal can be seen in the bottom right hand side of Figure 3.1. A detailed concept design for the camera has been produced and is illustrated in Figure 3.15. In order to minimize the footprint of the GFA camera, all readout electronics are located on boards running perpendicular to the sensor surface. Figure 3.16 shows a single petal and the location of the GFA camera on that petal. In-focus sensors distributed evenly around the perimeter of the focal surface provide a cross check for any atmospheric or thermally induced changes in the magnification of the system. Having defocused sensors distributed evenly around the perimeter of the focal plane is required to fully sample the wavefront.

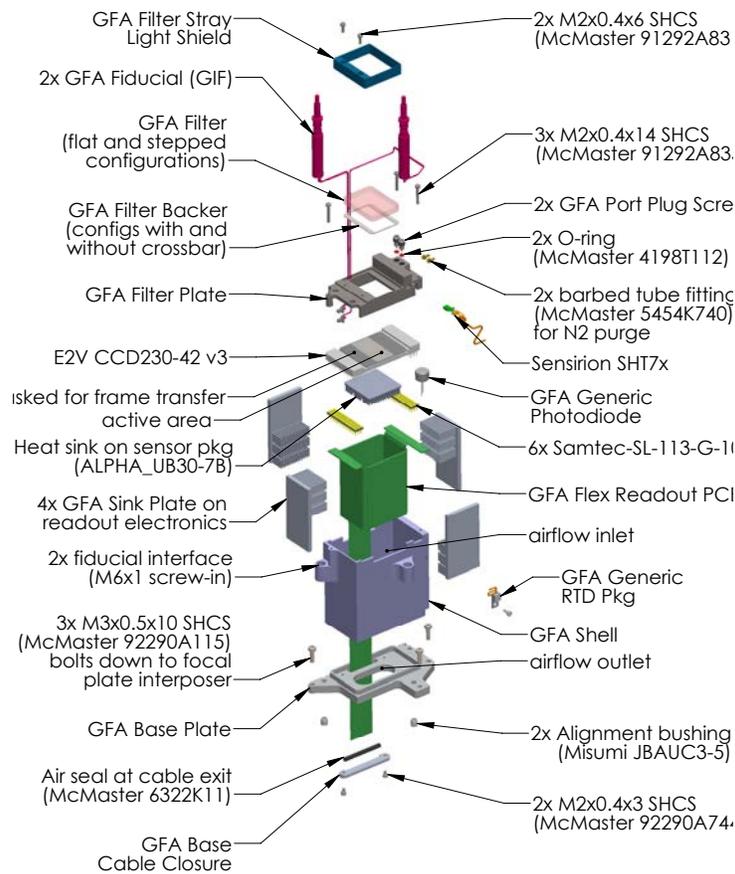


Figure 3.15: Detailed concept design for the GFA camera.

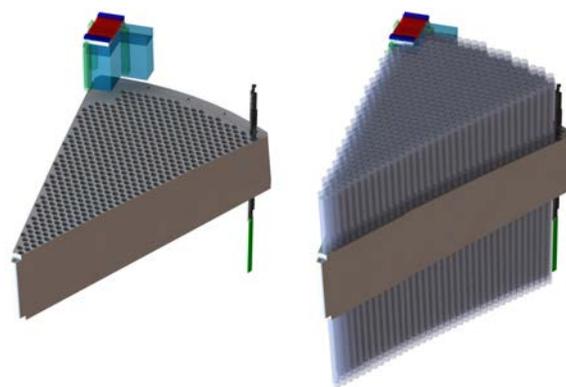


Figure 3.16: GFA mechanical envelope is shown in relation to a focal plate petal. The envelope includes an e2v CCD230-42 package, masked for frame transfer, with the unmasked active area in unvignetted light. The GFA envelope includes generous packaging room for illuminated fiducials (transparent green) and electronics (transparent blue). A fiber positioner is shown at one corner of the petal, and in the right view positioner envelopes illustrate the full packing.

3.4.3 Electronics

Readout of the CCD will be fully digital. This means that the output signal from each CCD amplifier will be digitized at a high rate (100 Msps) and then a digital correlated double sampling

applied. The electronics is in charge of generating the clocks to shift the charge on the CCD synchronously to the ADC and the firmware which implements the correlated double sampling. The voltage bias and clock values will be fixed on CCD characterization to a value, allowing a reduction of the required space to implement it. Each CCD controller will have an Ethernet interface, a power module, a telemetry module and 4 modules to operate with each of the CCD channels as shown in Figures 3.17. The main idea is that the system will only require 2 cables: Ethernet and power. Main power supply will be external to the system.

3.4.4 Illuminated Fiducials

The science fiber tips are mapped to sky positions by the Fiber View Camera and the GFA system. The acquisition step will determine the absolute pointing of the GFA sensors on the sky. Illuminated fiducials mounted near these sensors will be correlated to the position of all of the other illuminated fiducials and then the fibers located within the fiber actuators. Mechanical survey and on sky calibrations will be required to complete the guide sensor to science fiber calibration.

3.4.5 Acquisition and Guiding

DESI requires absolute pointing on the sky in order to deliver light into the science fibers. For each spectrographic exposure, the telescope will slew to a new location and all guide sensors will be read out in full frame mode and an astrometric solution computed. Stars found in these images will be compared to a star catalog to determine the absolute pointing of the telescope. This catalog needs to be matched absolutely to the target lists and should be created from the same data set as the targets or from an extremely good astrometry catalog such as *GAIA*.

Once the absolute pointing is determined the guide sensors will switch to region-of-interest (ROI) mode and start guiding the telescope to the correct absolute position on the sky and maintain that pointing during the observation. Photometric and image quality information from stars will also be used to determine observing conditions to be used in a dynamic exposure time calculation. To provide consistent guiding on all parts of the sky the system contains “in focus” optical sensors covering a total of ~ 180 arcmin². Six of ten GFA cameras will be used for this purpose with each camera covering ~ 29.3 arcmin². In the guiding configuration, the camera is equipped with a flat optical (R-band) filter (Figure 3.18a). With this area, at least 10 guide stars ($15 < R < 19$) will be available for more than 99% of the survey footprint. Additionally, this area is sufficient for

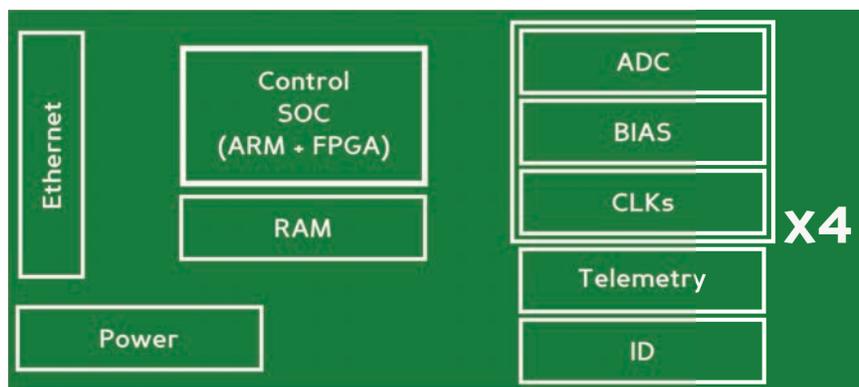


Figure 3.17: All systems will be coordinated by a Xilinx System on Chip (Zynq) which will host both the low level firmware in vhdl and also a Linux embedded system.

determining the current telescope pointing within ~ 20 seconds assuming that the Mayall provides ± 10 arcminute pointing accuracy after a large slew.

The delivered optical PSF are determined from the guide signals and provided to the focus and alignment system as well as the telescope telemetry. This information will be used to help adjust the exposure times for the science fibers.

Additionally, the 4 channel ROI readout mode of the cameras provide 1 star/object and 3 empty ROIs. These empty ROI frames are also delivered to any interested client for determining changes in total atmospheric and instrumental transmission.

3.4.6 Focus and Alignment

Four of the ten identical cameras will be used for focus and alignment. In this configuration the cameras have a dual thickness optical filter (Figure 3.18b). They are otherwise identical to guide cameras. This dual thickness filter provides intra and extra focal images of stars. One half of the acquired image contains stars nominally ~ 1.5 mm below focus and the other half is ~ 1.5 mm above focus. These combined images provide all needed information to correct focus, tip/tilt and decenters with the corrector hexapod.

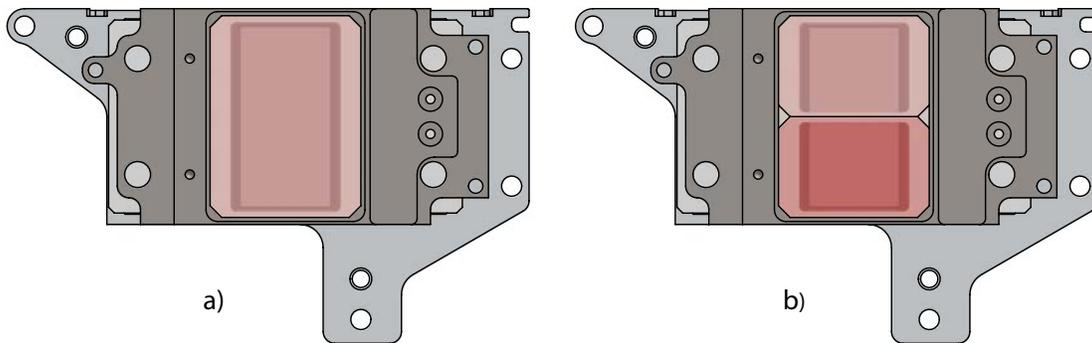


Figure 3.18: Top views of a GFA camera showing different filter configurations for a) guide/acquisition and b) focus/alignment.

The design of this system is based on the very successful system used in the Dark Energy Camera (DECam). Out of focus stars will appear like the pupil plane, which in the case of a prime focus instrument is an annulus or “donut”. An example donut image taken from DECam is shown in Figure 3.19 left. Simulations of the optical system can generate wavefront error maps so that any observed collection of donuts can be used to determine the misalignments of the DESI focal surface. It is important to have donut samples at various locations all around the focal surface. Intra and extra focal donut images for DESI from a Zemax simulation and shown in 3.19 right.

The focus and alignment algorithms are based on the proven techniques used in the DECam [7] active optics system (AOS). The AOS currently fits one donut per CPU core in less than 2 seconds. A forward modeled χ^2 fit is performed comparing the observed out of focus images (64×64 pixel stamps) to a modeled expected image by varying leading order aberrations. The model includes a uniform sky background, pixelization, and a Kolmogorov kernel to model atmospheric seeing. The derivative of the χ^2 with respect to the Zernike coefficients is calculated in closed form using the method described in Fienup [8]. The χ^2 is minimized using the MIGRAD algorithm in the MINUIT [9] package, which implements a Davidon-Fletcher-Powell variable-metric method. Figure 3.20 shows a sample of fitted donuts from DECam showing the observed image, fitted model and model predicted image.

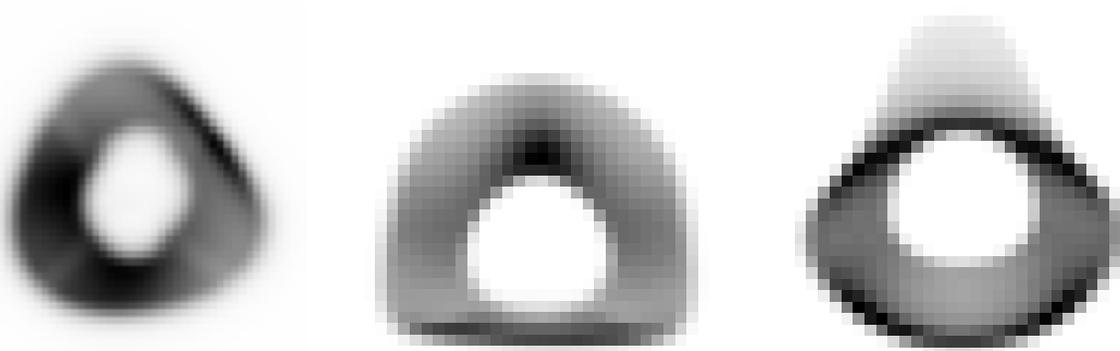


Figure 3.19: Left: Image of an “out of focus” star taken by the Dark Energy Camera. Center and right: simulated DESI intra and extra focal donuts, respectively.

Figure 3.21 shows the performance of the DECam AOS for all available exposures for September 2013. Performance of $300 \mu\text{m}$ rms in decenter and $30 \mu\text{m}$ rms in defocus is shown. Exposures where AOS could not accurately determine the wavefront are omitted.

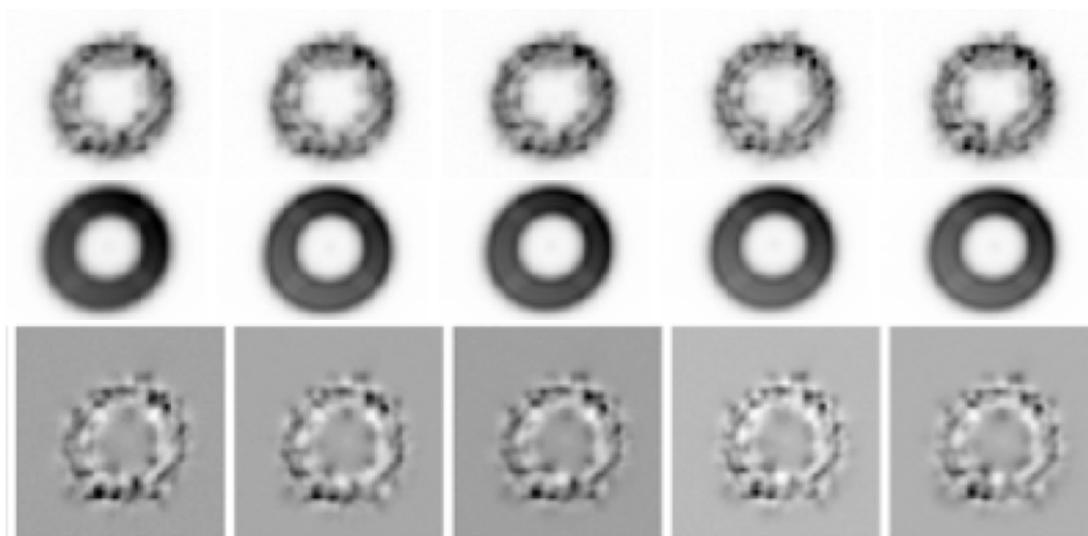


Figure 3.20: Sample donuts (top), fitted model (center), and image minus model (bottom).

3.4.7 Stellar Density

The GFA sensors will use stars to provide the guide signal and to measure focus and alignment of the DESI instrument. In order to determine the required area of sensors, simulations were run using both the NOMAD catalog [10] and tabular information from [11, 12]. Figure 3.22 shows the total and average number of stars found vs galactic latitude using the NOMAD catalog. To account for sensor dynamic range, stars were grouped into bins covering 2 magnitude bins and counted in random one degree regions of the sky. Signal-to-noise studies indicate that using magnitudes of $15 < R < 17$ and ten stars slightly exceeds our required pointing accuracy [13]. The legend in figure also shows the percentage of fields that had a total of ten guide stars available. It is important to note that this simulation did not include rejection of stars with a nearby neighbor. Additionally,

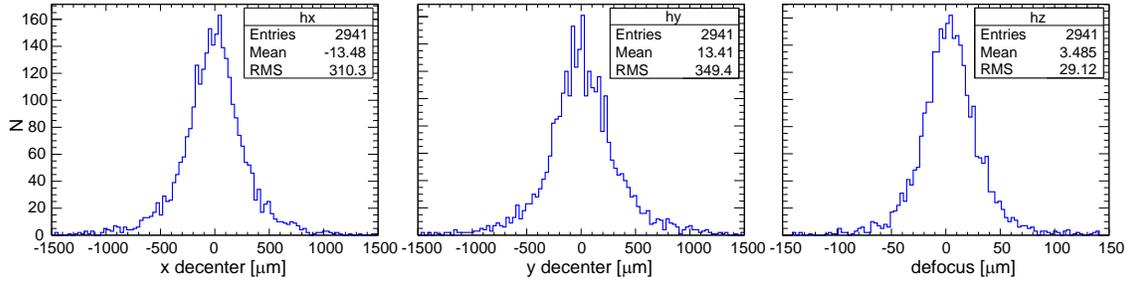


Figure 3.21: Performance of DECam $x - y$ decentering and defocus from September 2013.

while the simulation used the correct sensor locations and sky area, the sensor was simulated as a circle on the sky (DESI-0341).

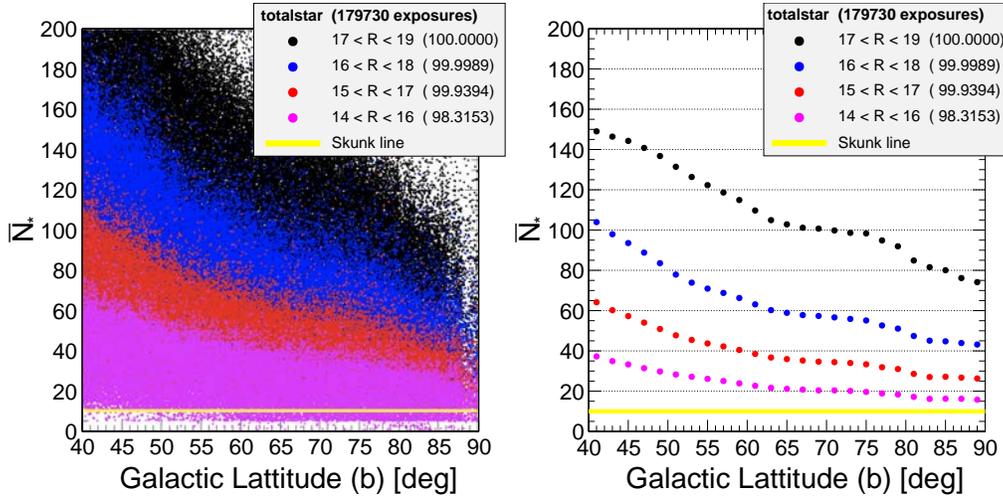


Figure 3.22: Total number of stars seen in six DESI GFA sensors using random pointings and the NOMAD catalog.

3.4.8 Signal-to-Noise Studies via Simulation

In order to better understand the effects of higher dark current and potentially higher read noise, a full simulation of guiding signal-to-noise was developed. The contents of this simulation are as follows:

- A random night over the coming two years was selected. Worst case: summer and winter nights had same length.
- A random telescope zenith and azimuth angle were selected: zenith $>45^\circ$.
- Sky brightness of the full moon always used. Worst case.
- Temperate selected from Mayall historical record using full temperature range including daytime highs. Worst case. Sensor assumed to be 5°C above ambient.
- Delivered PSF with mean of 1.0 arcseconds and a range from 0.8 to 2.0 arcseconds was selected randomly.

- For each of the 4 channels on each of 6 guide GFA cameras the brightest star in the range $15 < R < 19$ was selected. Used Bachall 1986 formulation for speed.
- The SNR of each of the (up to 24) stars was calculated.

Figure 3.23 left shows the sky coverage of the simulation. Figure 3.23 right shows the median signal-to-noise (here the 12th best of the up to 24 available guide stars). The mean SNR of the median guide star is more than 40 and only rarely does SNR fall below 20. Using

$$\sigma_{\text{centroid}} = \frac{\sigma_{\text{seeing}}}{\text{SNR}} \quad (3.1)$$

we can expect to easily meet the required guide accuracy using even a single median guide star. Multiple guide stars are required, however, to account for systematic changes in focal plate change, atmospheric dispersion, etc. Nominally 10 guide stars will be used, increasing centroid accuracy by ~ 3 .

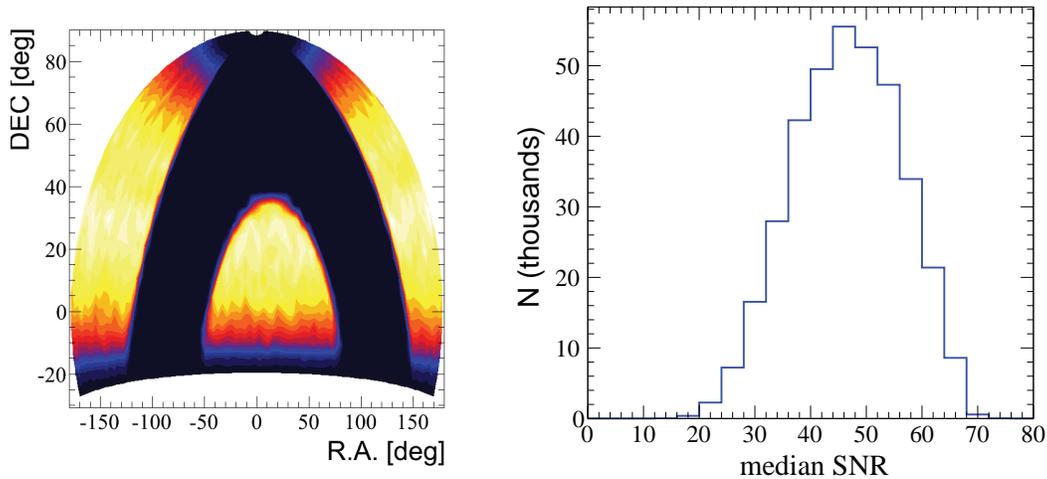


Figure 3.23: Left: Sky coverage for guiding SNR study. Right: Simulated median signal-to-noise for guide stars over a wide range of conditions.

3.4.9 Commissioning

The GFA sensor is the only imaging system in DESI and will be vital during commissioning and engineering time for DESI.

A new pointing map will need to be created for the Mayall telescope. This is done by scanning the sky (15 degree steps in azimuth and zenith angles) and determining flexing of the telescope so that corrections for this can be made automatically by the telescope control system from the produced lookup table. Additionally, at each location the nominal hexapod settings required to maintain mechanical alignment are determined and stored in a separate lookup table.

3.5 Fiducial Illuminators

Illuminated fiducials are point sources distributed throughout the focal plate field. These fiducials are illuminated during Fiber View Camera (FVC) measurements (see Section 3.6). Field fiducials are attached to the focal plate petals in place of positioners. Similar fiducials are affixed to each GFA mechanical assembly (see Section 3.4). Each fiducial has precision features for mechanical

survey. The mechanical datums are each measured carefully with respect to the optical source points, and with respect to focal plate datums. These are surveyed with respect to the GFA sensor active area and with respect to focal plate datums.

Once the installed field fiducials have been surveyed with respect to the focal plate datums, we have a complete set of survey data. These data are completely constrained for all the functional items on the focal surface, as measured at the survey temperature and orientation. With this set of known relations, FVC measurements of the illuminated focal plate fiducials, GFA fiducials, and back-illuminated science fibers can map accurately to physical locations, establishing the focal plate scale.

A study (DESI-0485) assessed kinematics of the field as viewed by the FVC through the corrector. The study finds that accurate and robust interpolations are made with 4 field fiducials distributed radially through roughly the center of each petal, and 6 more field fiducials at the perimeter of each petal, a total of 100 field fiducials. Each GFA has 2 fiducials to track the guide sensor coordinates relative to the field fiducials. Thus a total of 100 focal plane fiducials and 20 GFA fiducials will be measured on each FVC exposure. The location of these fiducials are shown as red dots on Figure 3.24. The fiducial fibers will of course be illuminated only when the positioner fibers are back illuminated during an FVC exposure, and not during science exposures.

The focal plane fiducials have the shape of long cylinders (Figure 3.25) the same diameter and length as the fiber positioners and they are threaded into holes on the focal plane just like the fiber positioners, with their tips coplanar with the tips of the positioners (Figure 3.26). Each fiducial contains a ~ 40 mm long single mode fiber, $5 \mu\text{m}$ in diameter, illuminated by an LED of 470 nm wavelength. The tip of the fiber is in a ceramic ferrule with the fiber positioned in the center with a $1 \mu\text{m}$ precision. After installation in the fiber plane the position of the fiducial fibers will be measured to a few μm accuracy by a measuring machine contacting the outside diameter of the ceramic ferrules.

The GFA fiducials will be mounted on two sides of the GFA enclosure as shown in Figure 3.27. The tips of these fiducials will be identical to the tips of the focal plane fiducials with a single mode fiber illuminated by an LED and centered in a ceramic ferrule to facilitate precise location measurement.

3.6 Fiber View Camera

The purpose of the Fiber View Camera (FVC) is to take an image of the fiber plane after the robotic mechanism has positioned them and calculate the offset of the actual position of the fiber

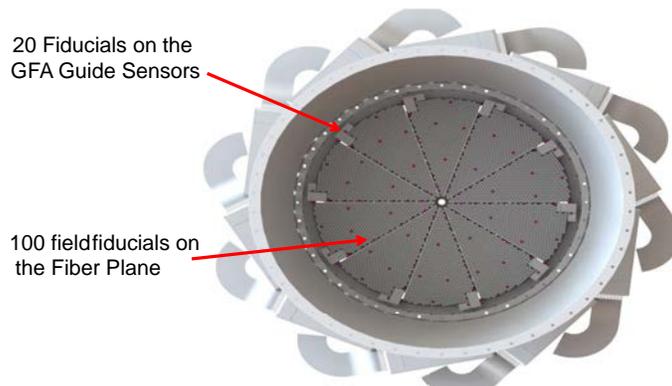


Figure 3.24: Illuminated Fiducials on the Focal plane (red dots).

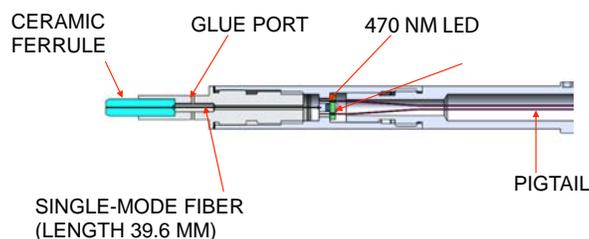


Figure 3.25: Illuminates fiducial cross section.

Table 3.4: Fiber View Camera requirements.

Item	Requirement	Rationale
Measurement accuracy	$< 3 \mu\text{m rms}$	FVC is used to position fibers, and must be able to locate the illuminated fibers to this level of accuracy.
Nearest neighbor resolution	1 mm	Minimizes planning restrictions on fiber location.
Integrate, read out, compute centroids	≤ 5 seconds	FVC must image and centroid fiber tips quickly for multiple fiber positioning commands.

from its desired position to better than the $5 \mu\text{m}$ precision. These offsets are fed to the computer controlling the fiber positioners so that the positions of the fibers can be corrected. The estimate from simulations of this process is that several iterations will suffice to get all of the fibers positioned to the required positions. The performance requirements on the camera are listed in Table 3.4 (DESI-0589).

The FVC measures the locations of the 5000 fiber positioners, the 100 field fiducial fibers, and the 20 GFA fiducials. These items are back-illuminated between observations (when the spectrograph shutters are closed), and the FVC surveys them all simultaneously in one field, looking at them through the corrector. This closes the loop unambiguously for positioning of fibers on every observation, as well as providing continuous feedback of variations in plate scale.

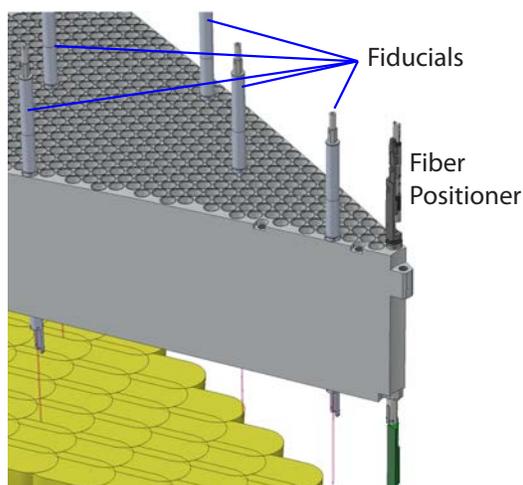


Figure 3.26: One fiber positioner and several illuminated field fiducial on a focal plate petal.

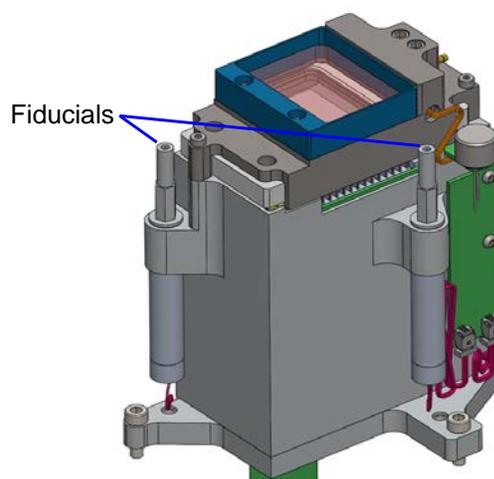


Figure 3.27: Location of the fiducials on the GFA enclosure.

3.6.1 Fiber View Camera Design

In the design of the FVC a fiber plane of ~ 1 m diameter was assumed. The camera is to be located on the axis of the telescope below the center of the primary mirror, looking up at the fiber plane through the hole in the primary mirror, about 12.25 m below the fiber plane, as shown in Figure 3.28. To fit the image of the fiber plane on a ~ 40 mm CCD requires a demagnification of ~ 25 , which can be accomplished by a 600 mm focal length camera lens. At this demagnification the $5 \mu\text{m}$ precision on the fiber plane translates to a $0.2 \mu\text{m}$ precision on the CCD. With a pixel size of $6 \mu\text{m}$ by $6 \mu\text{m}$ this means a centroid precision of $1/30$ of a pixel or 33 millipixels. To satisfy these design requirements the following camera components have been chosen:

1. A Kodak KAF50100 CCD with 6132×8176 pixels $6 \mu\text{m}$ by $6 \mu\text{m}$ each. This is a monochrome CCD with a 1 second readout time, with a read noise of 10 electrons. The dark current is 15 e/pixel/sec at 25°C , so the camera can be operated at room temperature.
2. A Canon EF 600 mm f/4 lens. With a Canon lens mount the lens focusing and f stop selection can be done under remote computer control.
3. CCD control and readout electronics suitable for operating this CCD, utilizing a Proline PL50100 controller available from Finger Lake Instruments.

The fibers will be back illuminated by monochromatic LEDs in the spectrometer enclosures at a level that will provide 25,000 electrons per fiber image on the CCD. At this level of illumination the dark current and the read noise are negligible.

Another important consideration to be taken into account in the design is the fact that the images with the camera will have to be taken through the telescope corrector optics. This configuration has been carefully simulated with the detailed design of the corrector optics and the FVC camera using the BEAM4 ray tracing program. The conclusion of this study was that the distortions introduced by the optics can be adequately corrected for by a third order polynomial transformation. There will be 100 fixed fiducial fibers on the focal plane with precisely measured positions that will be used to calculate the coefficients of the transformation with every image taken, tracking thermal effects, position drifts and other possible perturbations. An additional 20 fiducials (2 per GFA) locate the guide/focus cameras.

3.6.2 Development Program

A development program has been carried out to demonstrate the precision that can be obtained with the camera. A prototype camera has been constructed with the design described above, as shown in Figure 3.29. A prototype of a 450 mm by 600 mm section of the fiber plane has been constructed with 64 $120\text{-}\mu\text{m}$ -diameter fibers embedded in it. The fibers were back illuminated by monochromatic LEDs. The positions of the fibers were measured with an OGP (Optical Gauging Products, Rochester, N.Y.) Model Avant ZIP400 measuring machine with $1.5 \mu\text{m}$ precision. The fiber plane was then placed 8.9 meters from the prototype camera. Images with a variety of illumination levels, camera lens f-stops and exposure times were taken. The reconstructed images on the CCD were transformed to the fiber plane using a third order polynomial transformation and compared with the true positions of the fibers from the OGP measuring machine. The rms of the deviations of the reconstructed positions and the OGP measured positions is shown in Figure 3.30. The precision achieved is better than the $3 \mu\text{m}$ rms requirement.

A number of studies have been carried out to investigate the relevant parameters of the camera, with the following results:

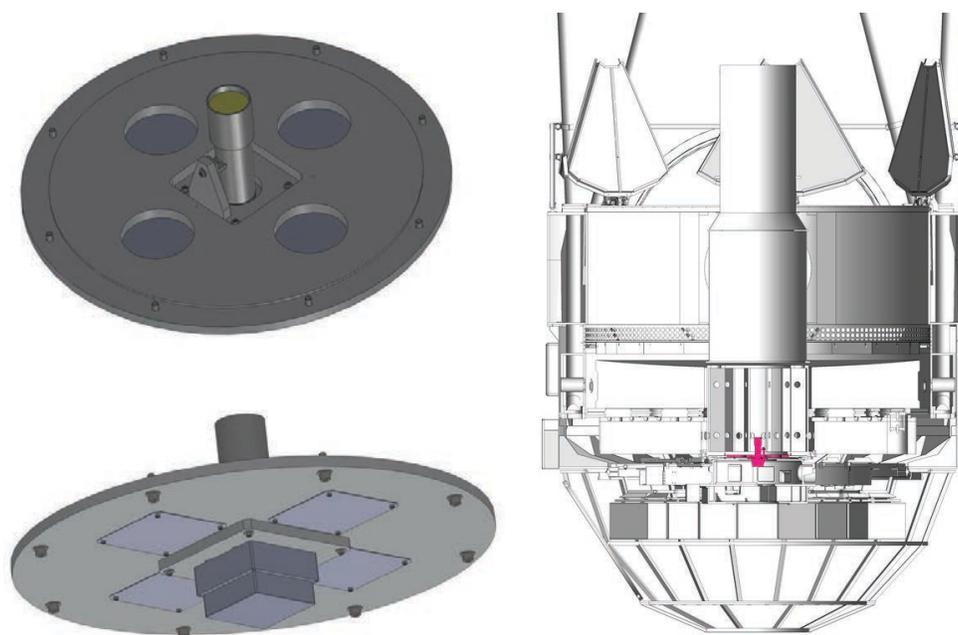


Figure 3.28: Location of the Fiber View Camera in the Mayall Telescope.

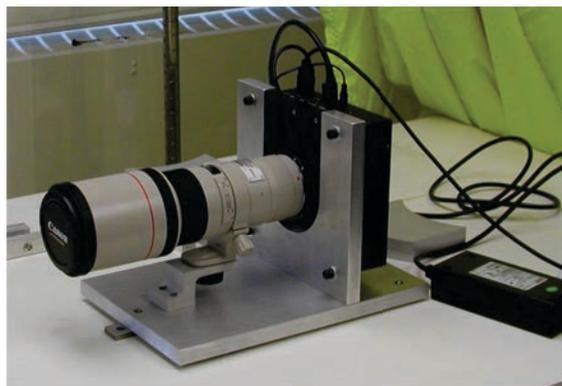


Figure 3.29: The prototype Fiber View Camera.

1. The best resolution was obtained when the camera was slightly defocused to produce an image on the CCD between 1.5 and 2.0 pixels wide. Narrower images did not have sufficient flux in pixels neighboring the central pixel to allow for precise interpolation to obtain the centroid position.
2. The most reliable good resolution was obtained with the lens f-stop set at $f/16$. At this aperture the image was diffraction limited with a diffraction peak 1.6 pixels wide, which gives the best resolution in a robust way. At this f-stop the camera has a large depth of field, making it insensitive to slight shifts in camera or fiber plane motions due to flexing of the telescope support structure or thermal effects.
3. The best resolution was obtained with between 10,000 and 40,000 electrons per image on the CCD. Below 10,000 electrons statistics started to limit the resolution, and above 40,000 saturation effects started to set in. The design therefore calls for an illumination to produce

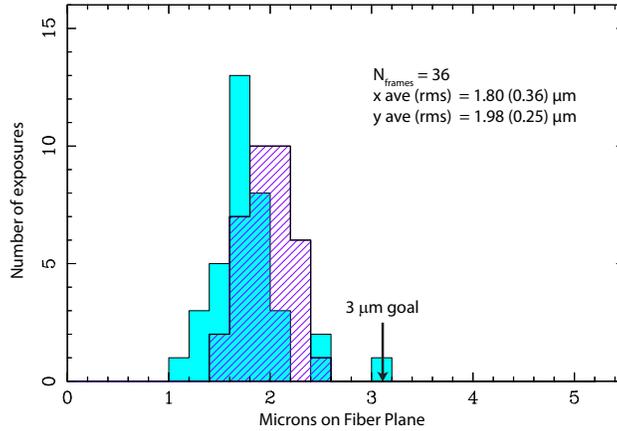


Figure 3.30: Distribution of the rms deviations of the FVC reconstructed fiber positions relative to their OGP measured positions. Blue is x distribution; red hash is y distribution.

25,000 electrons per image, in the middle of this range.

3.6.3 Camera Control System

Ethernet communication will be used to control and read out the camera and the control software has been developed in the R&D program. Software has also been developed and tested in the R&D phase to generate centroids from the FVC images. This software has been carefully optimized to carry out the analysis required to centroid the 5000 positioner fibers in somewhat under 1 second. The time for one iteration with the Fiber View Camera, consisting of 1 second exposure time, 1 second readout, and 1 second centroiding software time, satisfies the 5 sec requirement.

3.7 Thermal Management

The primary purposes of the FPS thermal management system are:

- Prevent significant temperature changes of the focal plate during an observation. This ensures stability of the fiber and GFA locations.
- Insulate the dome air from FPS heat, sufficiently evacuating FPS heat throughout the night.

Additionally the system will provide local cooling to GFA that operates at ambient temperature. Also, the thermal management system includes small circulation fans to ensure no significant density gradients in the air volume between the C4 corrector lens and the focal plate.

It is estimated that the focal plane system will consume ~ 516 kJ per observation cycle (DESI-0995). The thermal enclosure is a 75 mm thick insulator ($< 1 \frac{W}{m \cdot K}$). Heat exchanger plates are located within the thermal enclosure, mounted with flush thermal contact to the petal structures. The exchangers will remove the generated heat at a sufficient rate to prevent $\Delta T > 1^\circ\text{C}$, which could contaminate telescope seeing. A coolant line will carry the heat from the exchanger and off the telescope. The coolant will track ambient dome temperature. The thermal management system is illustrated in Figure 3.31.

Neglecting entirely the heat removal by natural convection and conduction, it is still expected that the thermal capacitance of the support plate and positioners themselves will be sufficient to keep the plate temperature change well under $\Delta T < 0.5$ K during the course of an observation. Over

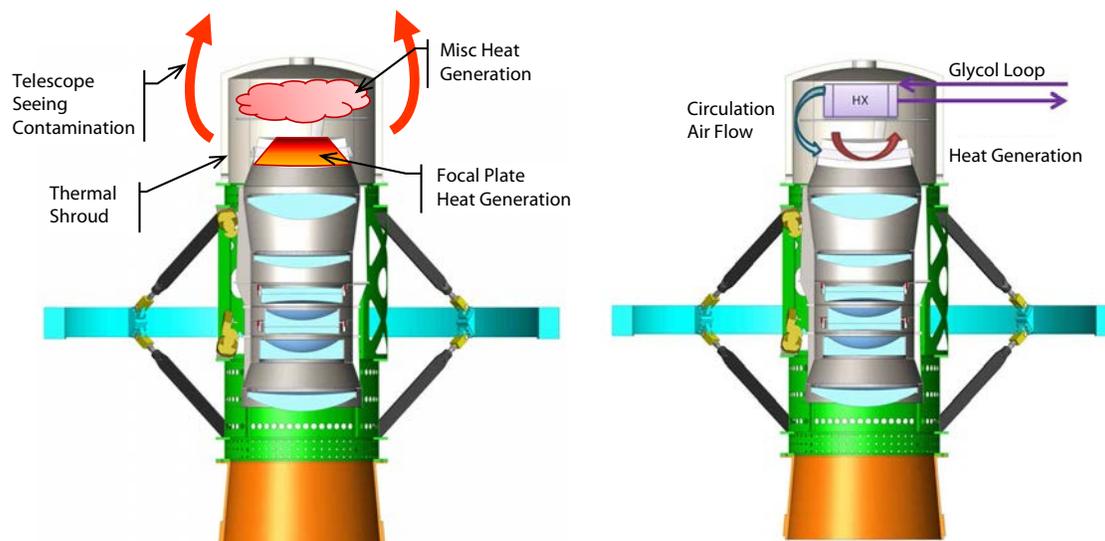


Figure 3.31: Left: heat production in the focal plane system. Right: thermal management.

a $\phi 0.82$ m aluminum focal plate, $\Delta T = 0.5$ K corresponds to a worst case radial motion $< 5 \mu\text{m}$ of the outermost fibers and GFAs with respect to the optical axis.

We additionally anticipate between observations circulating some air from the space between C4 and the focal plate to the rear, to ensure achieving good mixing and getting warmer air to the heat exchangers. In summary thermal management is expected to be fairly straightforward. A full-scale breadboard test is planned early on to ensure all the thermal management components have been well-sized.

3.8 Alignment, Integration, and Test

The key alignment step for the focal plate assembly is bolting the petals to the integration ring. A schematic of this is illustrated in Figure 3.32. Each petal references along its outer radius and front face to the integration ring. Radial and 45° bolts ensure tight mating of these surfaces.

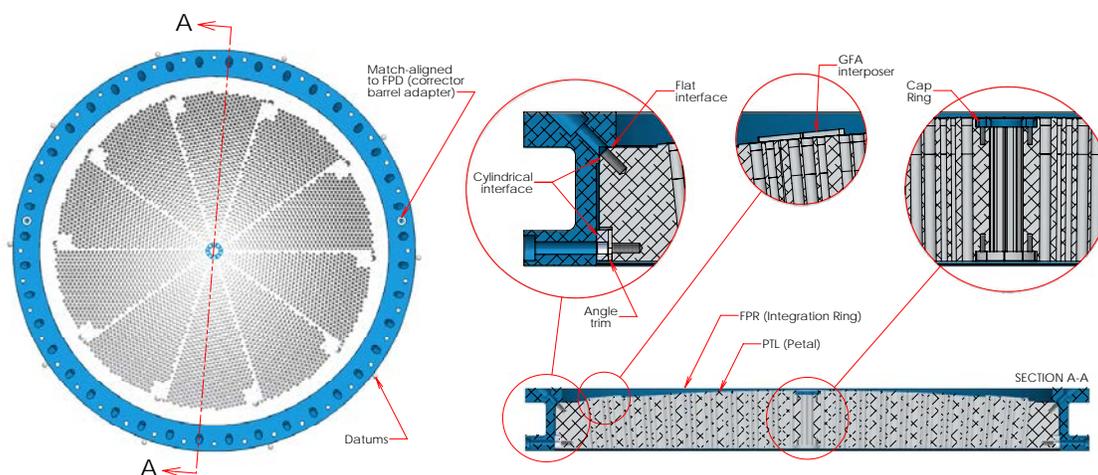


Figure 3.32: Schematic of focal plate petal alignment to integration ring.

Before integration of positioners, the petals are introduced to the ring for a dry fit. Standard machining tolerances will get the petal tilt within 0.05° of nominal. Petal datum balls are surveyed with respect to integration ring datums. As necessary, each petal is then trimmed in place to an angular resolution of 0.002° , by replacement of gauge spacers at the radial bolts. The small center cap ring (attaches to wedge tips on the front surface) is face machined appropriately at each of the 10 pads where it bolts to the wedges. After it has been attached, the compliant rear cap is attached, and the assembly is re-surveyed.

With the 10 petals aligned, the GFA interposer plates are aligned. One GFA interposer is bolted to each petal. Each interposer has two pin bushings which have been located on the same fixture, so that all 10 interposers present an identical mounting interface to the 10 GFA assemblies. Standard machining tolerances will put the interposers within $100\ \mu\text{m}$ of nominal. The interposers are surveyed in place on each petal; then they are trimmed in place to a resolution of $2.5\ \mu\text{m}$ and re-surveyed to confirm.

Subsequently, the petals are disassembled from the ring and integration of positioners commences. A key benefit of having the focal plate sectored in 10 petals is factorizing positioner loading. Each petal may independently have all its positioners loaded at one station (a process which may take some 2–3 weeks per petal), and then be taken to a completely separate station(s) for fiber dressing and splicing (another 2–3 weeks). Petal field fiducials are also installed. Meanwhile the positioner loading station is free for repeating the process with a fresh petal. Subsequently the latest fully-loaded petal can go to survey.

A fully loaded petal assembly is illustrated in Figure 3.7. When all the petals are fully loaded, they are re-introduced to the integration ring for final bolt-up and survey check.

There is an option to mount the GFAs to their respective petals at yet another independent station, prior to integration ring bolt-up; or after having bolted in the 10 loaded petals, to mount and survey all 10 GFAs at the same time. The second option is likely preferable, as it maximizes the decoupling in schedule of GFA production from positioner loading.

The assembled focal plate with positioners, their optical fibers and electronics, GFAs, fiber spool boxes, and coils of fiber optic cables are shipped as a unit to the telescope; the focal plane enclosure is shipped separately.

3.9 ProtoDESI

3.9.1 Introduction

ProtoDESI is the planned small-scale installation of prototype DESI elements at the Mayall scheduled for installation and commissioning at the Mayall telescope during summer 2016. ProtoDESI is a risk reduction tool for the full-scale DESI project (hereafter referred to as ‘DESI’). This document defines goals and technical specifics for ProtoDESI.

ProtoDESI will include a focal plane populated with prototype DESI fiber positioners, Field Illuminated Fiducials (FIF), and a Guide Focus Alignment (GFA) sensor module. The GFA has two more fiducials (GIF) mounted directly to it. The focal plane will be mounted to the existing 0.8 degree FOV, $f/3.2$ refractive corrector at the prime focus (PF) of the Mayall telescope. Short optical fibers will be routed from the positioners to the Fiber Photometry Camera (FPC), a commercial camera that will image the fiber tips. It will also be located in the PF cage. A fiber back-illumination system will be included in the FPC. The Fiber View Camera (FVC) will be mounted to the lower surface of the primary mirror cell. A subset of the DESI Instrument Control System (ICS) will control the ProtoDESI subsystems, communicate with the Telescope Control System (TCS), and collect instrument monitoring data.

3.9.2 Purpose

There are two primary goals for ProtoDESI; both to reduce the risk related to the technical challenge of placing the fiber tips on targets and keeping them there with sufficient accuracy for the duration of a DESI exposure. First, the GFA-ICS-TCS control loop will be tested to see if the system can place guide stars on requested GFA pixels and that they then remain stable in position over the period of an exposure. Once this is established, the second goal is to test the GFA-positioner-FVC control loop. Target objects will be identified relative to guide stars. The positioners will be placed on the targets relative to assumed guide star pixel locations on the GFA by iteratively using the FVC, fiducial illuminators and fiber back-illuminator to generate corrective delta motions. The GFA-TCS will then place the guide stars on those pixels' locations. The FVC will then measure the intensities of the positioners' fibers; the positioners can be dithered to look for intensity changes indicating how well the fibers were initially positioned on target centers.

3.9.3 Additional Benefits

In order to effectively use the field fiducials to account for system variations for accurate fiber positioning, metrology will be done on the assembled focal plane system. This effort will relate the field fiducials (FIFs) to the fiducials on the GFA (GIFs), and therefore to the pixels of the GFA. This will provide early validation of the metrology method required for the more complex DESI focal plate.

3.9.4 Performance Goal

The goal for the performance of ProtoDESI is to operate on the Mayall telescope for a 6 hour period per night, successfully placing celestial targets on >75% of its targeted fibers. Exposures will be 20-30 minutes and there will be <15 minutes between exposures. Completely automated observation is not required; manual interactions and inputs are allowed. The long inter-exposure time allows for the sequence to be less parallelized than required for DESI and allows for less maturity of the software and hardware. There is no specific throughput or signal-to-noise goal or requirement.

3.9.5 ProtoDESI Elements

Figure 3.33 illustrates the layout of the elements installed on the ProtoDESI focal plate.

3.9.5.1 Focal plate

The focal plate will be an aluminum part with provisions to mount two GFAs (though only one is needed for ProtoDESI). Adjacent to the GFA there will be approximately 30 standard, threaded, DESI positioner-interface holes, not all of which are planned to be populated. The front of the focal plate will be flat, with the positioner holes perpendicular to that surface. Positioner focal position is set by having all the positioner flanges contact directly to the flat surface (unlike full DESI, where each positioner flange contacts a uniquely-oriented spot face on each hole). The positioner holes will be on a hex pattern, spaced 10.5 mm apart, similar to the spacing on DESI.

3.9.5.2 Positioners

Approximately 8-10 prototype positioners will be installed in the focal plate, clustered near the center of the focal plane. Each positioner will have a short length of fiber with a ferrule at both

ends installed. After integrating positioners into the focal plate, all the free-end ferrules will be integrated in an array block so they all face the Fiber Photometry Camera.

3.9.5.3 Positioner Collision Avoidance

Positioner collision avoidance is beyond the baseline scope of ProtoDESI. The focal plate will be populated with positioners such that no positioners are adjacent. The densest positioner packing would be a hex pattern where each positioner is surrounded by six holes that are either unoccupied or have a fiducial illuminator. We note that the focal plane can be used later for lab testing of collision avoidance.

3.9.5.4 Fiber Photometry Camera

A commercial camera behind the focal plate will simultaneously image all fiber ends to roughly measure target fluxes, to determine positioner placement accuracy. It is possible this camera can be read out in real time for feedback as to how light throughput (and therefore fiber position accuracy) is being maintained. Small dithers of the positioners or the telescope can be used to explore how well fibers are placed on target centers. This camera is to be present for ProtoDESI but not for DESI.

3.9.5.5 Fiber Back-Illumination System

A system to back-illuminate the fibers will be installed with the FPC. The FVC can then survey fiber positions simultaneously with the FIFs and GIFs, to iterate and confirm fiber positioner placement.

3.9.5.6 Field Illuminated Fiducials

Approximately six prototype FIFs will be installed in positioner mounting holes, in a pattern to be determined by field distortion analysis of the prime focus optics. FIFs are sized such that they

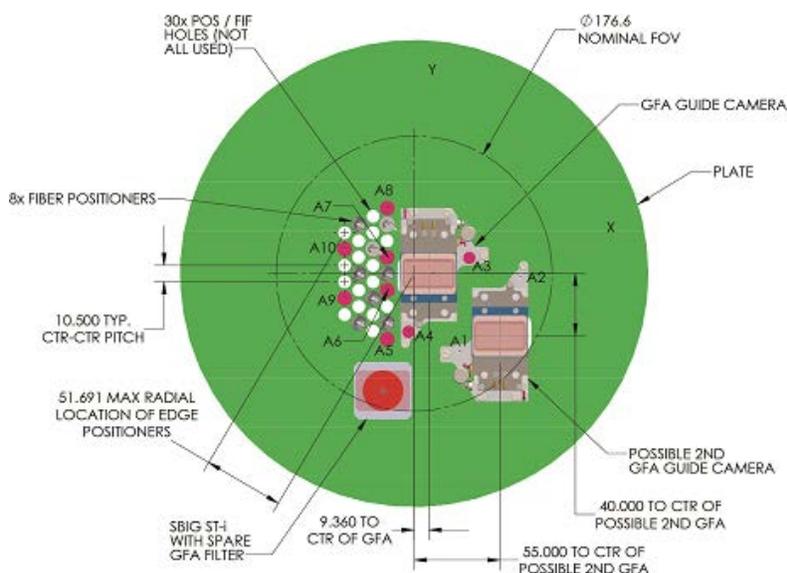


Figure 3.33: ProtoDESI focal plate layout.

cannot be contacted by an adjacent fiber positioner, so there is no need for anti-collision software for this case.

3.9.5.7 Guide/Focus/Alignment Sensor Module

Precision, repeatable mounting features will be provided for two GFAs with the active areas within the 176 mm diameter field of view. ProtoDESI is baselined to use only one GFA, but the other position offers the option to install another one if available, or is a backup mounting position in case of damage to the other. The primary GFA will be located to provide significant sensor coverage at the boresight. The GFA will be mounted outside the patrol range of any adjacent fiber positioners, so there is no need for anti-collision software for this case.

3.9.5.8 Metrology

In order to effectively use the field fiducials to account for system variations for accurate fiber positioning, metrology will be done on the assembled focal plane system. This effort will relate the field fiducials to the fiducials on the GFA, and therefore to the pixels of the GFA before shipment.

3.9.5.9 Ancillary Hardware

Attached to the focal plate will be any required fiber and wiring management hardware. We anticipate CAN signals will be distributed to positioners and fiducials via either 1 or 2 small breakout boards. The breakout boards would have the same connectors and electrical features as we anticipate for the petals in full DESI. The breakout boards then connect to a master board. The master board supplies DC power and is what communicates to the Ethernet network. These local control electronics and power supplies or other ancillary focal plane systems will all be located inside the PF cage.

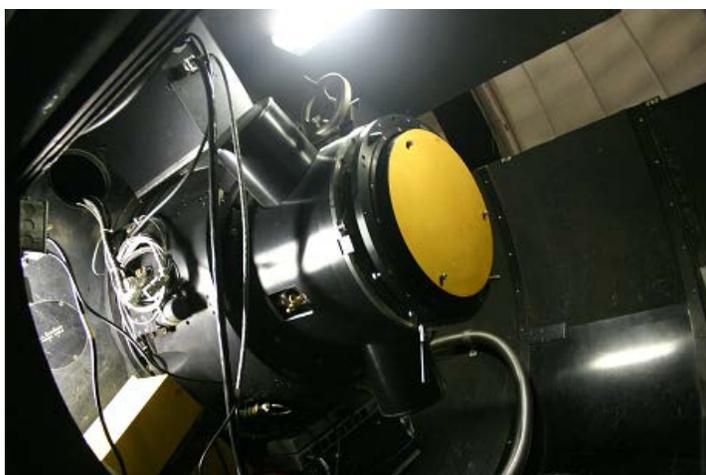


Figure 3.34: PF cage viewed from below with telescope oriented for MOSAIC install. Photo taken through hole that MOSAIC comes up through. Yellow protective cover over 4th lens of corrector. Interface plane & alignment pins surround that. Power strip and Ethernet switch visible below corrector. Craning cutout in cage visible in upper right.

3.9.5.10 Integration

The ProtoDESI focal plate system will be integrated to the PF cage with the telescope pointed south at low elevation, in generally the same way MOSAIC installation and removal are currently done. The MOSAIC installation and removal procedures are described in detail in DESI-0647. In short, with the telescope pointed south as shown in Figure 3.34, the dome jib crane will lower its hook through the slot on top of the PF cage and lift the ProtoDESI focal plane system from its cart to a height a little greater than the lowest position of the scissor lift. Then the scissor lift will be moved into place below ProtoDESI, and the installation personnel will get on the lift (with safety harnesses).

The scissor lift and crane will be raised together, so the personnel can guide the focal plane assembly. Then the focal plane assembly will be moved into its position and fastened to the interface ring.

Finally, the Ethernet and 120 V power cables will be plugged into the PF cage outlets.

3.9.5.11 Fiber View Camera

The ProtoDESI fiber view camera hardware, identical to the DESI FVC hardware (with the possible exception of the use of a 400 mm focal length lens rather 600 mm), will be mounted to the lower surface of the primary mirror cell in place of the Mayall Guider and Cassegrain Instrument Rotator assemblies.

The computing and software needs for the ProtoDESI FVC installation are less than for DESI since there is no requirement on inter-exposure timing.

Power, data, and ambient cooling are all expected to be more than sufficient in the Cassegrain cage for the FVC.

3.9.5.12 Instrument Control System

The ICS will be an early release of the DESI ICS supporting only those elements needed to operate ProtoDESI and communicate with the TCS. It also will not have the fully-developed user interfaces DESI will have. It will have interfaces with the TCS, FVC, FPC, and positioner controller.

The ICS will require computers located in the existing Mayall computer room, but will be substantially smaller in the number of cores and amount of storage planned for DESI. Power and cooling resources in the computer room are expected to be sufficient for ProtoDESI needs.

3.9.6 Mayall

3.9.6.1 Telescope Control System

The TCS modernization will be completed in 2015 and will have been tested both with the MOSAIC instrument and with the ProtoDESI ICS at least several months before the complete delivery of the ProtoDESI elements.

3.9.6.2 Electrical Power

As described elsewhere in this document, existing electrical capacity is expected to be sufficient for ProtoDESI.

3.9.6.3 Control Room Annex

The commissioning and operation of ProtoDESI will require more control room space than is currently available at the Mayall. A lounge area on the U floor of the Mayall will be converted to a Control Room Annex to accommodate 10 or more people.

3.9.6.4 Data

Data bandwidth is not expected to require expansion for ProtoDESI.

3.9.6.5 Mechanical/Architectural

Aside from the modifications required to implement the Control Room Annex, it is expected that ProtoDESI will require minimal mechanical alterations to the Mayall facility. The focal plane system will be designed compatible with the existing envelope and cutout in the PF cage, and it should be readily balanced using existing hardware.

3.9.7 Targeting and Observing Plan

An observing plan will be developed for ProtoDESI based on available targets and final installation schedule. ProtoDESI will require target locations to be identified and translated into coordinates for the fiber positioners. Guide stars and guiding analysis code will be required for all fields to be observed. The fiber targets will likely be a mix of galaxies and stars.

4 Fiber System

4.1 Overview

The function of the fiber system is to transmit the light from 5,000 science-targets imaged at the telescope prime focus to the spectrograph optical input. Figure 4.1 shows a schematic diagram of the fiber system. Each optical fiber, with a $107\ \mu\text{m}$ diameter core, is terminated in a ferrule that is then mounted in a positioner arm (Section 4.3). The fibers are collected behind the focal plane into ten groups of 500. Each group spans $\sim 38\ \text{m}$ from the focal plane to the spectrograph room via guides, supports, strain-relieving spool boxes, and ruggedized cables (Section 4.4). Each group of 500 fibers is then precisely arranged and terminated into a linear arc that provides the optical entrance-slit illumination (Section 4.5) to an associated spectrograph. The fiber run includes a fusion-splice connection near the focal plane to allow for positioner installation and to facilitate fabrication, integration and testing flow. The major deliverables for the fiber system are the 10 ruggedized fiber cables, each with a 500-fiber slit assembly on one end and 500 individual ferrules on the other. Declination and polar bearing cable wraps and cable and fiber routing support elements are other key deliverables.

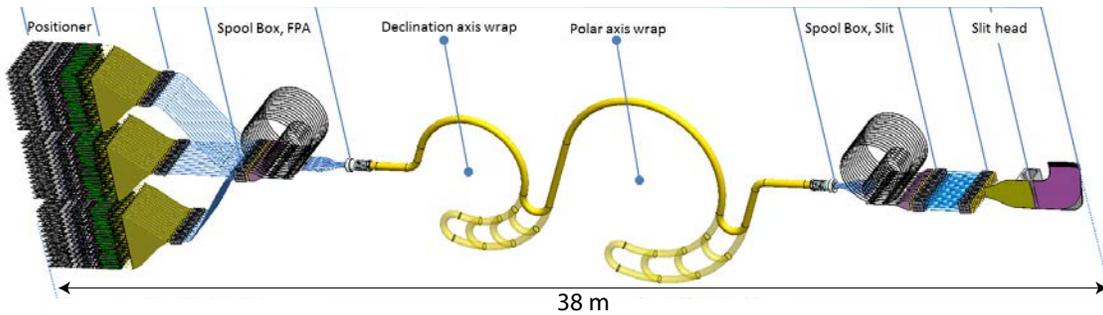


Figure 4.1: The fiber system schematic.

The performance requirements for the Fiber System are summarized in Table 4.1. Further discussion of the parameters is included with the relevant sub-system description below.

4.2 Optical Fibers

Throughput losses cause increased exposure times, limiting the survey rate. Therefore, control of fiber losses is a critical issue in the DESI design. The fiber system throughput to the spectrograph is mainly affected by bulk transmission losses in the glass, by losses at the fiber ends due to termination imperfections and surface reflections, by geometric misalignments at the fiber entrance and exit, and by angular diffusion caused by focal ratio degradation (FRD). Figure 4.2 shows the budgeted total fiber throughput as well as its constituent parts, which are a combination of both measurements and predictions, as described in more detail in the following sections.

It is convenient to consider the bulk properties of the fibers separately from the issue of FRD.

4.2.1 Bulk Fiber Losses

Fiber bulk attenuation is dictated by the fiber glass type and its spectral transmittance, the fiber length, and the ability of the fiber's limiting numerical aperture (NA) to fully accept the input $f/\#$ from the corrector. We plan to use Polymicro FBP, a low-OH step-index fused silica fiber, $\text{NA} =$

Table 4.1: Fiber System Requirements. Refer to DESI-0581 for the requirement rationales.

Title	Value	Statement
Fiber core diameter	107 $\mu\text{m} \pm$ TBD	Fiber average core diameter
Fiber System Bulk Throughput ¹	λ (μm)	Efficiency
	0.360	0.555
	0.375	0.655
	0.400	0.705
	0.500	0.848
	0.600	0.891
	0.700	0.903
	0.800	0.914
	0.900	0.929
	0.980	0.937
Fiber System Throughput due to FRD loss.	≥ 90 % from 360nm - 980 nm	Main contributors: fiber end polishing/cleaving/bonding, fiber splice, positioner motion, cable and cable guide bending
Single Fiber System Lifetime Throughput Loss	No more than 100 fibers per year (TBC) to suffer a loss of $\geq 20\%$ (TBC)	The total throughput of any single fiber, including both bulk throughput and FRD losses, shall not degrade from the nominal average value by more than 20% (TBC) over a 5 year lifetime of use
Number of Science fibers	≥ 5000	There shall be at least 5000 science fibers at the focal plane
Fiber positioner flexure lifetime	376,000 positioner moves	The fiber shall maintain performance after 376K positioner moves
PFA traceability	PFA to slit	It shall be known which position in the slit corresponds to which positioner
Fiber Cable flexure lifetime performance	169K cycles	Fiber System performance shall be maintained over 169K cable pivot bends
Number of fibers per slit	≥ 500	There shall be at least 500 fibers per slit
Near field stability / homogeneity ²	TBD	The near field pattern of the fiber shall be uniform and stable to TBD
	Facilitate the calibration strategy	

¹Neglecting FRD losses and averaged over 5000 fibers for uniform f/3.57 input (telescope obscured) at beginning of mission life.

²Conditions: observation, night-time, telescope slew.

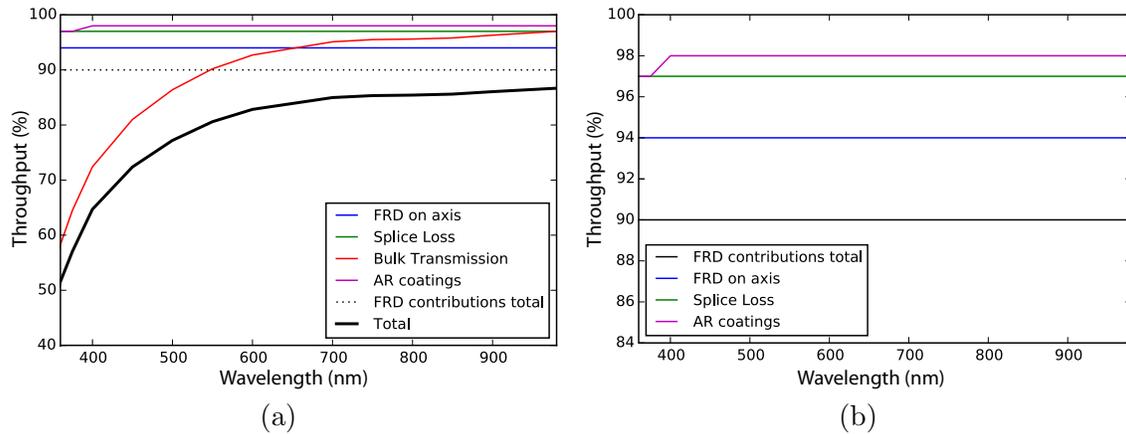


Figure 4.2: The predicted fiber throughput from 360 nm to 980 nm for 38 m of FBP fiber is shown in panel (a) and panel (b) shows the contributions that can be controlled. FRD, splice connection, and AR losses have been presumed constant with wavelength.

0.22, that has been well characterized to have excellent band transmittance without the complex and potentially confusing spectral absorption features found in high-OH, UV enhanced type fibers. The fiber core size (107 μm diameter) is selected to optimize science target flux collection versus background. The fiber cladding size (150 μm diameter) is chosen to eliminate significant evanescent surface loss. The fiber size is bracketed by and scaled from existing commercial products so it can be purchased as a custom draw lot under the same fabrication process.

Fiber routing options have been studied to minimize the total fiber length while maintaining a plausible method of integration with the telescope tube and pivot wraps. The length of the fiber is estimated to be 38 m, so the fiber system will use about 200 km of optical fiber. The predicted bulk fiber throughput for 38 m FBP fiber is shown by the red line in panel (a) of Figure 4.2. The black line corresponds to the total throughput when including the contributions from FRD, splice loss, and antireflection coatings.

4.2.2 Focal Ratio Degradation

Light incident on a fiber at a single angle exits the fiber in a cone with finite angular width. Consequently, an incident cone of radiation exits the fiber over a larger included angle (or smaller focal ratio) that could distribute light beyond the spectrograph entrance pupil. This focal ratio degradation (FRD) can be due to modal diffusion within the fiber caused by manufacturing imperfection and mechanical stress induced by termination, bonding, or mechanical force. FRD may be characterized in two ways:

Cone (or solid angle) test measure a fiber's angular diffusion by illuminating the fiber with a filled cone of light with constant surface brightness within a specified angle. To better simulate the illumination from the telescope, a scaled obscuration is added to simulate obstruction by the telescope's secondary mirror. This test directly describes how the fibers will behave in an instrument, specifically how much energy will be enclosed within some $f/\#$ for this illumination geometry.

Ring (or collimated) test measures FRD by injecting a collimated beam (from a low-power laser) into the fiber. The beam is azimuthally-scrambled to form a ring which is recorded by an imaging detector. The FRD is characterized by the thickness of the ring in the radial direction. Although, less direct than the cone test, it is very simple to do and interpret the results.

It has been shown, that these methods are equivalent (i.e., give the same result) except at very

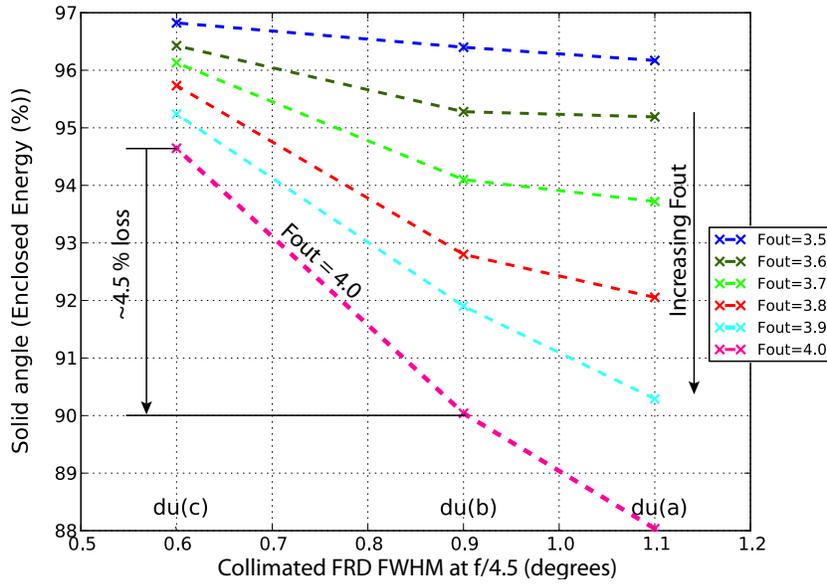


Figure 4.3: The effect of fiber collimated FRD on encircled energy measured for three different ~ 40 m cables, denoted by du(a) du(b) and du(c), with polished ceramic ferrules on each end.

small injection angles [14]. Determining collimated FRD is straightforward because the injection angle is obtained from the same image from which the ring thickness is measured. The relationship between the collimated FRD and the solid angle FRD is established by measurement and modeling as is shown in Figure 4.3. The horizontal axis shows the FRD (FWHM) of each fiber from a collimated FRD test at an angle corresponding to $f/4.5$. The vertical axis shows the enclosed energy within different output focal ratios from a solid angle FRD test using an input focal ratio of $f/4.5$ with a scaled obscuration. These data establish a relationship between the collimated and solid-angle FRD and establish the throughput tolerance to fiber collimated FRD. For example, there will be a throughput loss due to FRD of 4.5% if the fiber collimated FRD is increased by 0.3 degrees FWHM (for an $f/4.5$ input, an $f/4.0$ output, and a starting FWHM of 0.6 degrees

The FBP fiber selected for DESI has excellent FRD performance due to its extremely uniform cladding thickness and a thermally stress-relieved polyimide jacket. Low OH fibers from alternate vendors exist (e.g., CeramOptec Optran[®]) although studies show that the FBP fiber offers the best performance overall in terms of transmission and FRD performance [15].

In order to determine the actual fiber FRD performance, we have measured solid angle FRD as a function of input $f/\#$ for multiple fibers. The illumination geometry, and fiber termination method were found to have significant impact on the results. We have 38 m lengths of $120 \mu\text{m}$ core FBP fiber that were terminated both with polished ceramic ferrules and cleaved fibers bonded into glass ferrules. The results of these measurements (see Figure 4.4) were used together with corrector, positioner and ferrule injection angle values to establish that the FRD throughput loss due to angular misalignment between the input beam and the optical axis of the fiber will not exceed 10 % given the corrector injection $f/\#$'s and the spectrograph's acceptance $f/\#$. The contribution to the throughput budget from FRD is shown in Figure 4.2.

In addition to FRD increases due to injection angle offset, we have also tested the potential for FRD changes due to flexure of the fiber both in positioners and in the fiber cable as the telescope tracks over the observation lifetime. Significant fiber motions are caused by rotational type actuators and primarily constitute bending. Our tests showed no significant changes in fiber angular output distribution over 90,000 bends of 50 mm radius, although measurable throughput

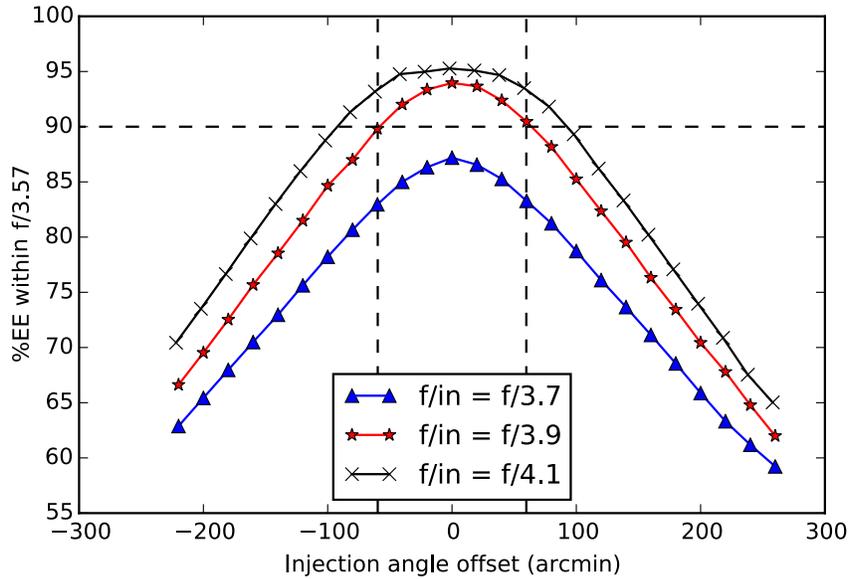


Figure 4.4: The effect of FRD and flux injection angle on throughput is derived from these measurements of the percentage of the energy contained within $f/3.57$ which is the spectrograph acceptance speed. The figure shows results for a test fiber illuminated with a telescope simulator at different focal speeds of $f/3.7$, $f/3.9$, $f/4.1$ (colored lines) and with chief-ray injection angle tilts of ± 240 arcmin. The relevant specification is as follows. The 90% efficiency requirement will be captured for the average DESI injection cone of $f/3.9$ (red line) at the DESI collimator acceptance speed of $f/3.57$ if the injection angles are kept below $\sim \pm 60$ arcmin (vertical dashed lines). Chief ray deviation shall not exceed 1.0° max, 0.5° field-weighted average (DESI-0478). The test fiber was a 38 m, $120 \mu\text{m}$ diameter core FBP fiber with ceramic polished ferrules and a collimated beam FRD of 1 deg FWHM at $f/3.7$.

losses were seen at bend radii less than 50 mm.

Tests were conducted to see if actuation over the positioner patrol disk impacted FRD. Ceramic ferrule terminated fibers were attached to development versions of rotational and spine type positioners. Initial tests with optically terminated bare fiber indicated that the FRD performance is affected in some extreme actuation geometries for rotational positioners. Although the fraction of the patrol disk impacted was small, modifications were made to the PFA in order to minimize stress to the fiber. These modifications, which included a polyimide strain relief tube that prevents the fiber from directly touching the actuator, greatly improved the FRD performance of the fiber in the actuator over extreme actuation positions. These results in addition to lifetime tests are shown in Figure 4.5.

The fibers will also be flexed in their bundled run assemblies as the telescope slews over the sky. Bending will be constrained to radii ≥ 50 mm using guides belts, rails and soft clamps. Stress propagation to the fiber ends caused by friction-induced winding over many motion cycles will be mitigated by using a cable with spiral wind construction and low friction sleeves over the sub-bundles. A fiber cable assembly mock-up has been exercised to ensure that the telescope motion will not be affected due to the stiffness of the fiber cables.

4.2.3 Near Field Stability

During the course of measuring the FRD performance of the test fibers in the positioners, it was discovered that the near field intensity distribution is affected in addition to the far field

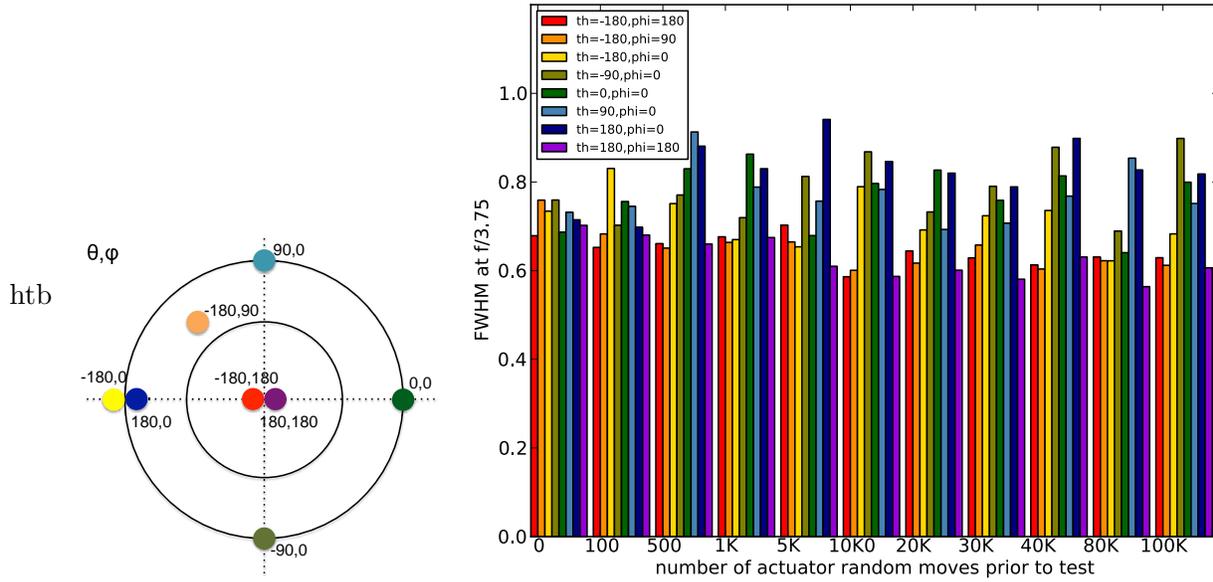


Figure 4.5: Each bar in the right panel shows the range of FRD over various actuator positions ($\theta = -180^\circ$ to $+180^\circ$, $\phi = 0^\circ$ (most amount of bending) to 180° (no bending)), see left sketch, as a function of lifetime (i.e., number of actuator random moves prior to test). Initial tests with a bare fiber showed that in some extreme rotational actuator geometries FRD was increased. However, using the PFAs described in section 4.3, the polyimide sleeve protects the bare fiber and the average FRD over the range of motion meets all requirements. To date, this performance is maintained to 100k cycles with continued testing underway.

performance. The near field intensity distribution is the the distribution of flux at the exit face of an optical fiber and represents a combined intensity distribution of optical propagation modes. The near field intensity distribution is subject to variations due to many factors such as fiber run geometry, illumination angle, optical wavelength, and bandwidth. In contrast, the “far field” pattern, an expression of the FRD, is the flux distribution at large distances from the fiber face caused by the angular distribution of the output. Because the fiber end is directly imaged to the spectrograph sensor, the final point spread function is a combination of the near field pattern, spectrograph optical aberrations, and sensor pixelization. If the near field pattern varies at some significant level, the instrument’s spectral response can be altered. Therefore, the form and stability of the near field pattern averaged over the data integration time is important for data comparisons such as calibrations.

Our measurements of the near field for a representative fiber show that the near field pattern does indeed vary with illumination geometry and fiber end finishing. Figure 4.6 shows how the near field intensity changes as a result of input injection angle as the fiber was held in a tilting spine actuator. Similar tests were performed for a rotating axis positioner and it was determined that if the fiber had suitable strain relief, the near field intensity remained stable. We believe that the bimodal pattern observed in the near field is a result of stress due to the hard epoxy that is required to hold the fiber during polishing. Preliminary data shows that this problem is reduced if the fiber is cleaved and bonded into a glass ferrule with a relatively soft glue.

The ultimate spectrograph response has been predicted using an end-to-end model that involves these measured near-field patterns, ray-traced aberration functions, modeled aperture diffraction, and sensor pixelization. Although in extreme cases, near-field inhomogeneity could cause significant departures in spectral response that would impact science investigations, the actual con-

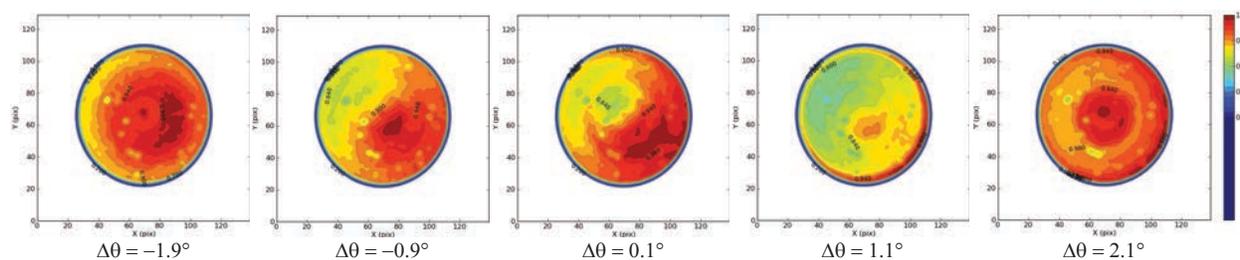


Figure 4.6: Near field intensity distribution as the input angle is offset from on-axis.

sequence depends on dynamical issues such as the exposure time, tracking geometry and calibration strategy, which are still under investigation. We are continuing with the near-field measurements and instrument simulations to establish the magnitude of the effect, and its mitigation.

4.3 Positioner Fiber Assembly

A 3 m long Positioner Fiber Assembly originates at the focal plane with an optically-terminated fiber connected to the positioner arm (Figure 4.7). The assembly begins at the focal plane area and terminates in a Fiber Spool Box where it will be connected to the long run of fiber bound for a spectrograph. As stated in previous sections, the fiber input termination will be made either by bonding the fiber into a close-fitting ceramic ferrule and then polishing the end face or by cleaving the fiber and bonding it into a glass ferrule. A supplementary strain-relief sleeve of polyimide protects the fiber starting at the ferrule and passing through the positioner.

This sleeve must allow unimpeded movement of the actuator and have adequate wear resistance to the repeated movement within the actuator's fiber guide channel. The strain relief tube transitions to fluoro-polymer (Hytrel[®]) furcation tubing (jacketing) at a steel adapter, also used as a tubing anchor point at the positioner's terminus.

The fiber termination process has been subject to a substantial development effort. Two main methods of fiber termination were explored: polished fibers and cleaved fibers. The polishing development effort involved combinations of the ferrule and strain relief tube's material, geometry, and adhesive type, application and curing together with polishing conditions to optimize the FRD,

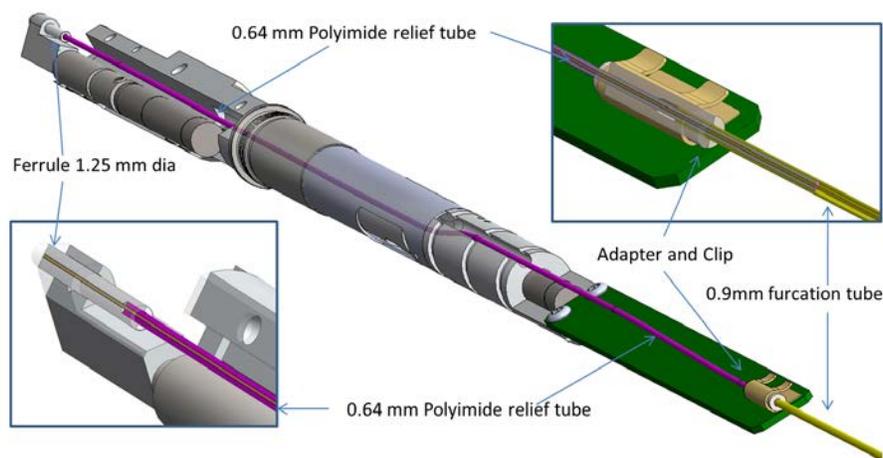


Figure 4.7: Positioner Fiber Assembly.

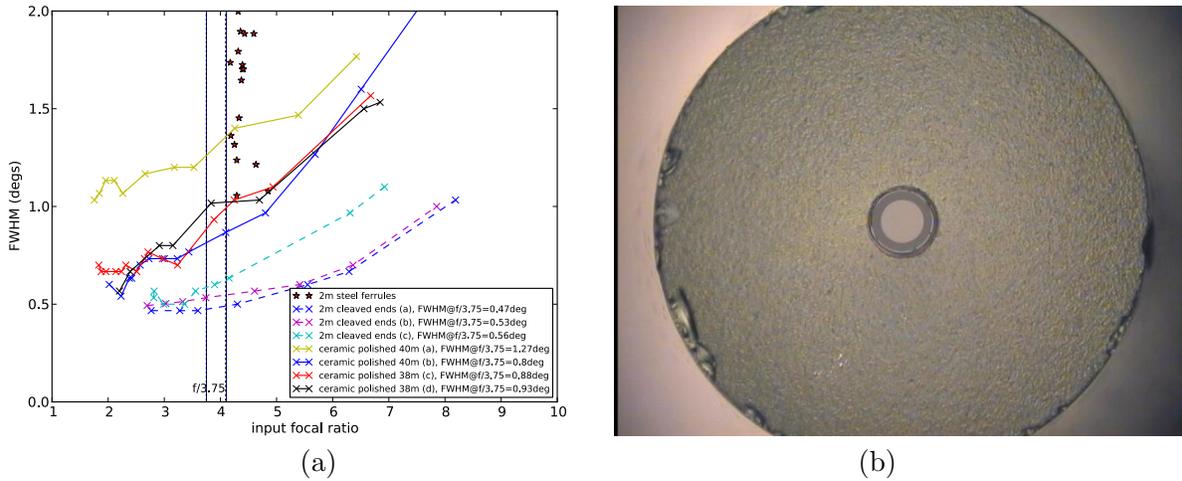


Figure 4.8: Collimated FRD for different methods of fiber termination. The horizontal axis shows the input focal ratio and the vertical axis shows the collimated FRD (FWHM, deg). Fibers finished with steel ferrules are shown as stars, fibers with ceramic ferrules are shown with a solid line, fibers that have been cleaved are shown with a dashed line. The vertical lines bound the $f/\#$ input range, $f/3.75$ to $f/4.25$, found at the DESI focal plane.

end polish quality, optical axial alignment and process yield. The best results have been obtained with flat-surface polishing of hard-epoxy bonded ceramic ferrules using a minimum application of glue.

The cleaving effort was divided into a number of stages. First, it was demonstrated that fibers could be cleaved provide excellent FRD performance. Next a glue and ferrule combination together with glue application method had to be found that did not degrade the cleaved fibers performance. Finally a method of aligning the end of the fiber with the end of the ferrule had to be established.

Figure 4.8 shows the results of collimated FRD tests of different generations of PFA fibers including both cleaved and polished ends. Panel b of this figure shows the end finish achievable with a cleaved fiber.

The ferrule will be coupled to the actuator using fixtures that precisely registers the fiber-entry axial position to the focal plane surface and that will not induce FRD from mechanical stress over the prime-focus thermal range.

The 5,000 Positioner Fiber Assembly units will be fabricated as 2,500 joined pairs, i.e., as 6 m long units with each end being optically terminated. Having science-quality ferrules on each end allows for 100% verification of FRD and ferrule optical axis performance. Such verification appears necessary as it is expected that a small percentage of terminated fibers will require rework to meet performance standards.

A broad band anti-reflection (AR) coating will be applied to the ferrule ends to reduce reflective losses from $\sim 4\%$ to $\leq 1.5\%$. A low temperature coating process will be used for compatibility with the ferrule bonding. Ion-assisted-deposition will be used to densify the coating film for environmental stability. The short length of clean, high-vacuum compatible materials used in the position fiber assembly facilitates AR coating by minimizing the coating chamber out-gassing load and mechanical volume required to support the fiber assembly in the coating chamber.

After coating performance and spot checking, the joined assembly pairs will be cut and delivered for positioner integration using shipping containers that protect the terminated fiber ends. The fiber can be back-illuminated through the cut end for actuator performance verification. The free fiber end will be threaded through focal plane fiber guides to a Spool Box after the positioner

is integrated to the focal plane. Optical performance testing (Collimated FRD and optical axis alignment) can be conducted on the final integrated positioner assembly by using simple collimated illumination of the free fiber end after high-quality cleaving.

4.4 Fiber Management

4.4.1 Top-End Guides

Optical fibers originating at each positioner will be gathered into fiber bundles and supported behind the focal plane. Each fiber is mechanically constrained to its positioner via a steel adapter that is fixed only to a surrounding protective 0.8 mm diameter Hytrel[®] furcation tube. The fiber itself is anchored only at the actuator ferrule and is free to move within the Hytrel tube. The furcation tubes are gathered and anchored into commercial, molded-plastic fiber manifolds (by Miniflex); wherein fibers are collected into sub-bundles within a polymer tube (e.g., M2fX) that exhibits a desirable trade of mechanical properties such as flexibility, toughness, crush and extension resistance.

The manifolds and tubes are held by a support structure fixed to each focal plane segment. The routing tubes are collected into a single Spool Box wherein they are terminated at a support manifold. The Spool Box is also supported by ancillary structure to the same focal plane segment as its fibers so that each complete focal plane segment can be entirely and independently integrated and handled. The Focal Plane fiber guide and management system is shown in Figure 4.9.

Two variations of Fiber Spool Boxes are planned, located at each end of the Fiber Cable. Both Spool Boxes are used for fiber routing management and contain free loops of fiber that act as a length reservoir for stress free connection to the positioners and spectrograph slit assemblies by compensating for fiber length differences due to manufacture and routing. The spools also isolate tensile stress and longitudinal fiber movement that can arise from flexing motions or thermal

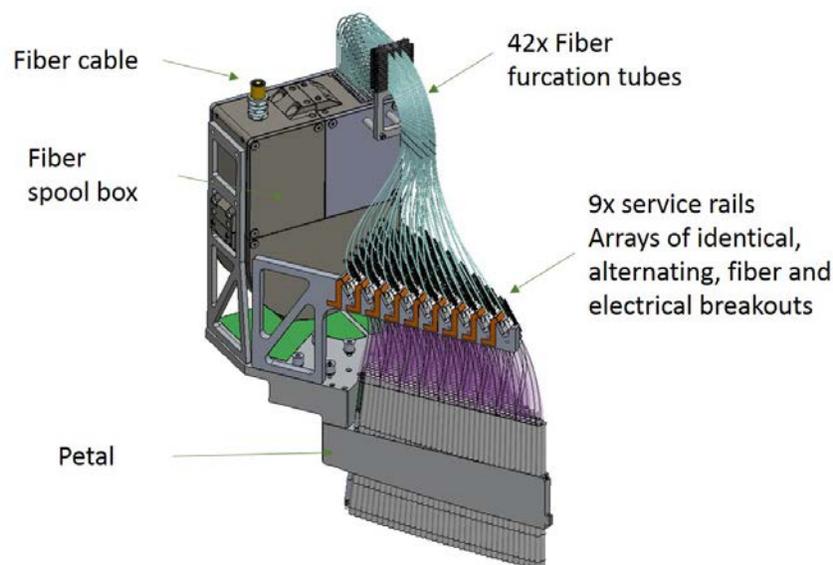


Figure 4.9: The focal plane is modularized via 10 petals, each holding 500 fibers. The fiber cables that contain the fibers are routed to the spool boxes in a way that allows each petal to be individually installed and removed if necessary. Fibers between the spool box and the focal plane are managed via focal plane hardware in order to ensure that the minimum bend radius requirement is not violated.

excursions within the main fiber cable.

Each fiber routing tube (M2fx) is directed into an associated box divider where its fibers can be looped in turns. The box includes a mechanical constraint that enforces the life-rated 50 mm minimum bend radius during fiber handling. After transit through the spool box, the fibers are again collected into M2fx routing tubes that are wound through a Fiber Cable. A total of ten spool boxes with their attached fiber cables service the full focal plane. The spool boxes are designed for layered access to the routing divider sections so that an orderly fiber integration process can be followed.

The hexapod, which holds the prime focus corrector, flexes laterally by up to ± 5 mm and this will be included in the requirements of fiber lengths between the spool box and the focal plane guides.

4.4.2 Fiber Cables

Ten Fiber Cables, each containing over 500 fibers, will be built following under-sea cable construction techniques as developed by Durham University for astronomical telescope application (including the SUBARU/FMOS fiber system which was found to have throughput $> 80\%$). Figure 4.10 shows a cross section through the cable. At the cable center is a strong Aramid-yarn tensile element that limits length excursions due to axial loads or thermal changes. The tensile element's diameter is built up with a polymer coating so that the M2fx routing tubes can be spiral-wound in a uniform radial packing. The spiral winding avoids cumulative tension at the end terminations that can arise from differential length strain when bending the cable. Each spiral tube is loosely filled ($\sim 60\%$) with fibers so that friction between individual fibers is minimized. The tubes are pre-loaded with fibers by the tube vendor prior to cable winding. Customized cable end fittings allow fixture rotation about one end of the cable while anchoring the M2fx tubes. The helical cable is wrapped with a protective ribbon of polymer tape and a hygroscopic gel layer that maintains a dry environment within the cable volume. Each of the ten primary cables will have a rugged outer protection layer consisting of an industry-standard 25 mm diameter PVC clad steel spiral wrap (e.g., Adapataflex) conduit. The mass is estimated as 0.65 kg/m^2 (see also DESI-0570 for the fiber length requirement).

The Fiber Cable will include 6% spare fibers to allow for damage mitigation during fabrication, integration and maintenance episodes. The spare fibers will terminate in the Spool Boxes at each end of the Fiber Cable so that they may be drawn from the boxes to a positioner and slit replacement location and fusion spliced.

The Fiber Cable runs across the prime-focus corrector support vanes, stacked to avoid obscuration, and then down the telescope truss structure toward the primary mirror cell. The cable routing to the spectrograph room has been developed based on fabrication and field test of scale and full size telescope bearing fiber-cable pivots, with particular attention to minimizing the route length and to the ease of cable assembly integration to the telescope. The cables are routed through a declination bearing pivot using guides and link belts (Iigus[®]) to route to and through a polar bearing pivot shown in Figure 4.11. From there it is routed to the spectrograph room where each cable terminates in a spool box that feeds a spectrograph slit assembly.

The cable guides limit twist and enforce a minimum bend radii of 200 mm that is established by the cable construction. Two 25 m lengths of mechanical sample cable were fabricated on a modified cable winding machine at Durham's Net Park facility. The sample cable was divided into ten cables, each 5 m long with complete termination connectors. The samples were used to measure the spring stiffness and hysteresis of the fiber cables when integrated to the telescope bearing pivots, and to confirm compatibility of the cable properties with the telescope's pointing control system.

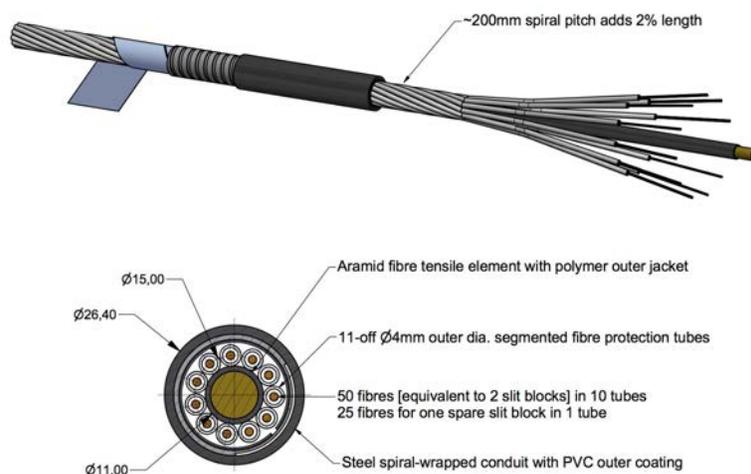


Figure 4.10: Proposed Fiber Cable cross section.

No degradation in the performance of the drive system was found (DESI-0752).

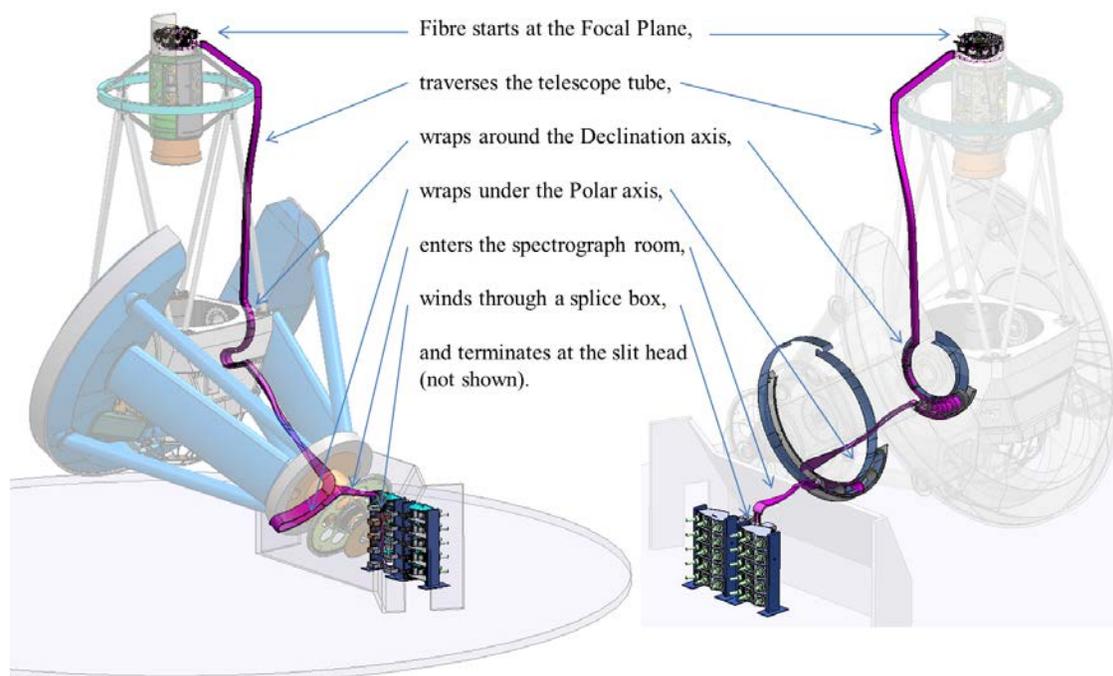


Figure 4.11: The routing of the Fiber Cable starts at the Focal Plane Spool Box, traverses the telescope tube and pivots, enters the spectrograph room, and terminates at the spectrograph spool box. Two routing options are shown with the one on the left preferred.

4.4.3 Fiber Connection

The focal plane spool box houses a fiber connection between the positioner fiber assembly and the remaining fiber cable. A connection is necessary to allow for positioner installation from the front of the focal plane and to facilitate the project schedule flow by isolating the positioner and focal plane fabrication, integration and test effort from the fiber cable development. (The connection also eases the process demands for AR coating of the positioner fiber assembly, as previously described.)

We have selected fusion splicing as the method of connection, following the comparative test of a variety of mechanical connector and splicing technologies. The key performance issue for connection schemes is their impact on throughput and FRD. Our demand of a low loss from these effects has proven difficult to demonstrate with commercial mechanical connectors, including single and multiple connector styles. Generally, significant connection losses occur at the mechanical interface due to lateral displacement and Fresnel losses at the junction. In addition, FRD performance is degraded by termination stress and angular misalignment. Our tests included the US Conec MTP[®] connectors (used by the SDSS-III APOGEE project) that are available in units that simultaneously connect 32 fibers. We also tested ceramic-ferrule military style single fiber connectors (Glenair) that can be ganged into multi-pin housings, and specialty single pin connectors by Diamond S.A. that promised precision lateral alignment.

Our investigation of the fusion splicing process as applied to the DESI optical fiber type has shown performance results far superior to mechanical connections. The high precision of fiber core alignment and resulting continuous glass interface yields bulk transmission losses of about 1% and minor impacts on FRD (≤ 0.2 deg increase in collimated FRD). These results were developed in a test campaign at the application laboratories of three major splice equipment vendors (Vytran, 3SAE, AFL). Competing methods for the key process steps of stripping, cleaving, fusing and re-coating, were tested and optimized. The FRD impact for fusion spliced fibers are shown in Figure 4.12. We are continuing tests with a Vytran splicer in order to determine the rate and yield of fiber splices that meet performance requirements.

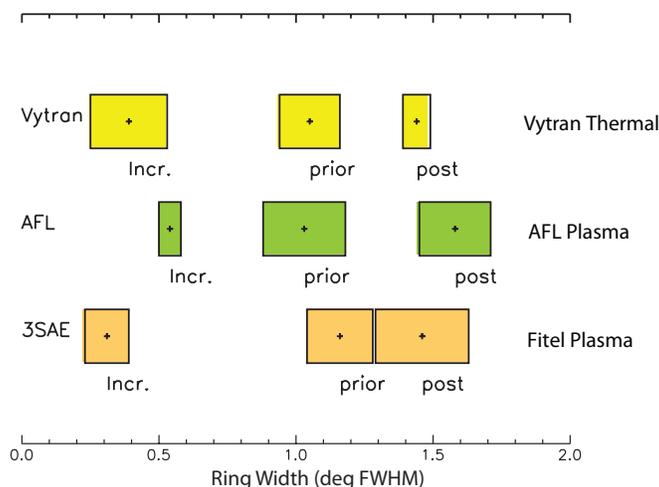


Figure 4.12: Summary of collimated FRD ring width increase for fusion spliced fibers by different commercial methods. A number of fibers were measured prior to splicing so that a baseline could be established. This range of baseline performances are shown as the width of the “prior” boxes; the range of post-slice performances are shown with the “post” boxes; and the range of incremental increases are shown with the “Incr.” (post minus prior) boxes. The 120 μm core FBP fibers were illuminated at an angle corresponding to $f/4.5$.

The fiber spool box has been designed to contain sufficient free fiber to fit splicing machinery for multiple fusion splice cycles. The box design includes segments of soft urethane foam (Poron[®]) for splice support and protection. The foam support has been proven to not induce measurable FRD while directly holding the optical fiber.

4.5 Spectrograph Slit

There are 10 science slits, 2 test slits which are sparsely populated and one flatfielding slit. The science slits will be temporary removed to allow insertion of one of the other slits when necessary. A slit is comprised of 20 blocks each containing 25 fibers. The naming convention is Block B0 through B19 from bottom (nearest to the bench) to top (furthest away from the bench). Within a block, fiber F0 (lowest in the block) to F24 (top of the block).

4.5.1 Science Slits

Each spectrograph input is formed by a fiber slit assembly. The slit consists of a group of 500 fibers arranged in a linear array with a convex surface that satisfies the spectrograph axial focal prescription. The fiber slit parameters are outlined in Table 4.2 and the geometry is shown in Figure 4.13.

Ideally, each fiber would be pointed toward the spectrograph entrance pupil with the optical axis slightly diverging from the axis of it's neighbors. This would mean a flared slit with all fibers coming from the radial center 468.3 mm behind them. In practice the 500 fibers are grouped to 20 blocks with 25 fibers each which are cemented into parallel v-grooves, with each block pointing into a slightly different direction. While this causes a linear shift in pupil illumination along one slit block, this effect is smaller than the natural pupil shift that happens anyhow along the whole slit even if each fiber axis would originates exactly from the same radius of slit curvature. ZEMAX simulations have shown that there is no additional light loss caused by this simplification, as the optical elements are oversized.

The fiber on-center spacing is established by the spectrograph field size together with the desired unilluminated regions between the spectra on the sensor. Optical tolerances demand a precise location for the fiber tips with respect to focal distance. However lateral and fiber center tolerances are undemanding because the relative positions are set by the v-grooves which are manufactured to tight tolerances.

Table 4.2: Fiber Slit Geometry Specifications for f/3.57.

Specification	Requirement
Fiber Diameter [d]	107 μm
Slit Height [h]	120.9 mm
Number of Fibers [N]	500
Fibers Per Group [n]	25
Number of Groups [g]	20
Fiber Spacing [s]	230 μm
Group Spacing [x]	556 μm
Radius of Curvature [convex]	468.3 mm
Fiber center-center tolerance	5 μm (TBC)
Fiber tip axial location	± 25 μm (TBC)

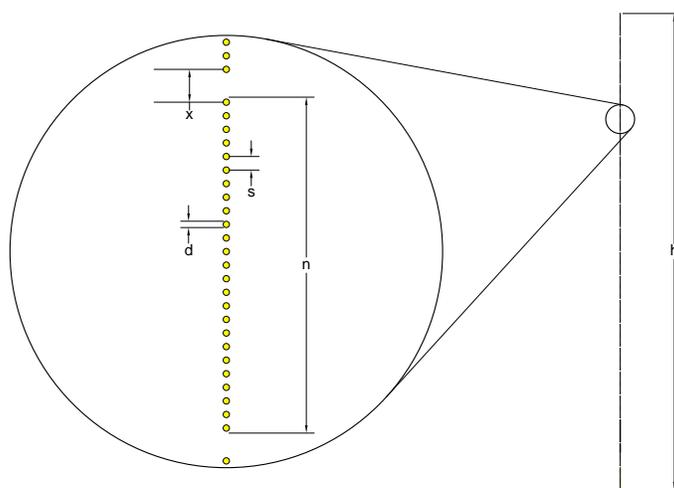


Figure 4.13: Fiber Slit geometry.

The slit array mechanical assembly can be compared to that used for the BOSS spectrograph slit [16]. However, the 20 fiber blocks are bonded to a slit plate that is either ceramic or metal and includes machined structures acting as datum surfaces during assembly. The plate provides the mechanical interface to the spectrograph and is installed using a linear stage and a datum surface to allow reproducible installation inside the narrow gap of the spectrograph dichroic beam splitter. The assembly plate also supports and constrains each block's fiber bundle and terminates the protective sheaths of the bundles. The fiber blocks are the basic fabrication unit for the fiber system.

There are many possible configurations for the mapping between the fiber cable and the slit so various trade studies were carried out to optimize the slit design with a view to making the assembly simple while conforming to the required tolerances. The preferred solutions are presented in documents DESI-0830, which detail the slit optical geometry and mapping between cable and slit components respectively.

The adopted solution has 20 slit blocks mapped to 10 Miniflex tubes (diameter 4 mm) within the cable (plus an unpopulated tube to aid packing). Therefore, each tube contains 50 fibers, which maps to 2 slit blocks, each of which contains 25 fibers.

The blocks are essentially regular cuboids with v-shaped grooves cut in one surface parallel to one axis. The fibers are therefore parallel within each block despite the finite location of the virtual spectrograph input pupil which means that the focal surface containing the fiber slit is convex. Modeling by ray-tracing shows that there is no significant degradation of image quality using this simplifying configuration. The slit blocks, however, are angled and positioned along a curved surface.

The fiber blocks are fabricated by bonding the ends of the individual fibers between v-shaped grooves and a cover plate. The fiber ends are then cleaved and co-polished with the block surface. The v-grooves are machined in fused silica.

This allows the fibers to be tested, without adding an additional termination, with light input into one slit block emerging from another slit block fed into test apparatus. After testing is complete, the fiber can be cut where it runs free at the top-end to separate the fibers into independent bundles of 25 where they can then be spliced with the top-end fibers.

A prototype slit block with diverging grooves has been fabricated. This is a greater challenge to fabrication than the proposed parallel-groove blocks so makes for a more stringent test than

required. Metrology showed compliance with the mechanical tolerances for groove position and direction and FRD (DESI-0619).

4.5.2 Calibration Slits

For spectrograph calibration purposes it is planned to temporarily replace the science slits with replacements that allow to sample the point spread function along the slit extension and to allow a flatfield calibration of the collimator-spectrograph train.

4.5.2.1 PSF calibration Slit

This consists of a sparse array of single fiber outputs. Each block contains one fiber only to create 20 spectra widely separated for PSF and stray light analysis. The fiber population consists of the bottom blocks B0-B9 with the bottom fiber F0 installed only, the mid block B10 which is fully populated (F0-F24) and the top blocks with the upper fiber position F24 populated only. In total 44 fibers are installed which on the input side are densely packed in a stacked connector that is illuminated by an f/3.57 beam by the 12 mm round field of the Offer relay.

4.5.2.2 Flatfield Slit

This consists of a leaky fiber that emits light laterally. This creates a single, broad white light slit that can be use for flatfield calibration of the collimator/spectrograph train. The specifications for this component is tabulated in Table 4.3. A candidate is the Corning Fibrance with an OD of $230 \pm 10 \mu\text{m}$ and an operational wavelength range between 405 nm and 1000 nm at least. Calculations show that an attenuation of 0.3 db/km results in 0.8% variation along the slit, hence the large scale variation along the slit seems easy to be met. The continuum light source can be fed through the fiber itself.

Table 4.3: Specifications for the flatfielding slit.

Uniformity along slit	50%
Uniformity along wavelength	50%
Variation along 300 μm of slit	1%
Spectral variation	< 1% over $\lambda/4000$
Width of illumination	< 300 μm
Lateral slit location	$\pm 50 \mu\text{m}$
Piston tolerance	$\pm 30 \mu\text{m}$
Beam intensity	$4 \times 10^4 \text{ Hz}^{-1} \text{ mm}^{-2} \text{ nm}^{-1}$

4.5.3 Mechanical Design

The slit is located in a slot in the first spectrograph dichroic. The mechanical design of the slit must be compatible with the space envelope defined in DESI-0543. The main challenges foreseen in mounting the slit blocks are that:

1. The maximum overall slit assembly thickness is 3 mm (at the beam) to minimize optical path obscuration. Consequently a significant support structure which enforces a minimum curvature radii is required to route fibers to bundling points outside the beam area.

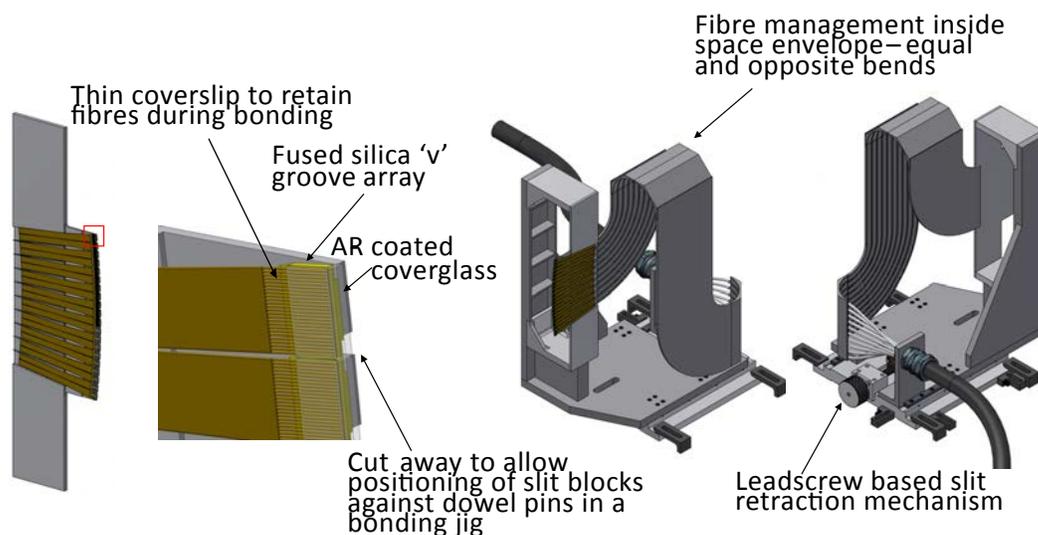


Figure 4.14: The fiber slit block fabrication (left) and strawman slithead assembly (right)

2. The slit is co-located with the front surface of the dichroic mirror and must be positioned through a narrow slit cut into that glass optic. A repeatable method of retracting the slit is required to allow the science slit to be exchanged with the flat field slit. The Piston location of the slit repositioning is expected to be of the order of $\pm 30 \mu\text{m}$. Lateral positioning of the slit is to be within $\pm 50 \mu\text{m}$.

A “strawman” mechanical design has been developed which is shown on the right hand side of Figure 4.14. In this design the slit is mounted on preloaded linear rails which and is translated using a leadscrew assembly. There are potential issues with access to the drive mechanism when the slit is mounted in the spectrograph, hence, alternative methods of retracting and positioning the slit are being considered.

To support the fiber ends with the required fiber spacing a three-part assembly has been designed (see left panel of Fig. 4.14). The fibers will initially be placed in the grooves and bonded in place with a low-shrinkage epoxy with a thin coverglass on top. This assembly will provide sufficient lateral support to hold the fibers during polishing. After polishing, an AR-coated coverglass will be glued to the front of the array using a suitable optical adhesive (e.g., Norland NOA88). The final stage will be to bond the v-groove arrays onto a backing plate following the exact radius of curvature of the slit. The required tolerances will be achieved by using a bonding jig which will locate each array against two pins along the front of the AR window and one that contacts with a feature cut into the side of the v-groove arrays through slots cut into the backing plate.

After the finish polishing and fiber support bonding, the pairs of slit blocks that contain the same fibers will be tested with light input at one block and emerging from another. Tests will be for throughput, FRD, and optical alignment. An AR coated thin ($250 \mu\text{m}$) coverglass will then be bonded over the fiber block face. The AR cover bonding uses optical index matched glue that will mitigate surface roughness or flaws in the fiber block polish. Using an AR cover plate avoids subjecting the bonded block assembly and its attached fiber and cable to coating chamber vacuum or thermal excursions.

4.6 Fiber System Assembly and Integration

In order to ease integration flow the fiber system will be produced in lots of 500 fibers. In addition to this, the PFA production will be decoupled from the cables and slit blocks. This allows the PFAs to be manufactured while the cables are being built and the slits polished. The fiber cable and slits will be manufactured at Durham Univeristy. The PFA bonding and fiber system splicing must be performed in a clean tent at LBNL.

Performance of the fiber system FRD and throughput are verified for each subsystem by testing prior to integration. Extensive fiber testing during the research and development phase has led to the development of optical testing setups which will be modified and automated. The testing happens at component, engineering model level, and production level.

4.6.1 Component Level Testing

Component level testing includes the acceptance of components as they arrive from the manufacturer. FRD and transmission testing will be performed on the bulk fiber when it is received in order to ensure it has sufficient performance before it is used in any sub-systems.

- Optical fiber: FRD and throughput measurements on sample fibers of the received batch to verify the fiber meets the specification. The collimated laser FRD setup can be used as well as the throughput setup.
- V-groove arrays: Visual inspection by microscope of chosen sample to verify compliance of groove number and dimensional properties.
- V-groove lids: Visual inspection and dimensional metrology.

4.6.2 Engineering Model Level Testing

Engineering model level testing targets the first production arrays where it is particular important to monitor performance compliance to validate component selection and assembly methods.

- Slit block: FRD and throughput measurements of each fiber along a slit block. This will verify that the slit block architecture and assembly method is able to provide a compliant slit.
- Block pointing accuracy: The parallelism can be quickly checked by illuminating all fiber inputs with the collimated laser beam of the FRD setup. If the superposition of the 25 annuli do not deviate from the theoretical expectation, the block is compliant. This test can be quickly done during FRD tests.
- Slit pointing accuracy: Can be measured by laser metrology using the reflection of the polished front face and a screen.

4.6.3 Production Level Testing

Production level testing includes, at a minimum, spot checks to flag potential problems. Depending on experiences during prototype testing it can be decided what sampling rate is required. If for example prototype testing revealed that there is no significant scatter in FRD performance along a slit block, one fiber per block can be measured to spot check compliance. In-situ verifications during assembly are possible at the slit assembly state.

- FRD and throughput: A sub-set of fibers along a block will be FRD and throughput measured. The size of the sub-set depends on the outcome of prototype testing.
- Block pointing accuracy: Use of the annulus projection again while illuminating all fiber inputs with the collimated laser beam at the FRD setup. If the pattern follows the theoretical expectation, the block is compliant while deviations from the pattern indicate either a pointing direction or FRD problem that has to be investigated further.
- Laser metrology at the polished and reflective v-groove front face: This can be done in-situ while cementing the arrays onto the slit plate, providing a second guide in addition to the mechanical datum. A screen with tolerance circles for each block position can be produced to streamline this process further.

As the fibers are terminated, all tests can be performed on double ended fibers of twice the final length before being cut in the middle. This assures the optical quality of the input surface is high enough without the need to polish input surfaces. After the fiber system has been spliced, a collimated FRD test will be performed before the system is released to telescope integration.

5 Spectrographs

The major spectrograph requirements are given in Table 5.1 (extracted from DESI-0613). The bandpass, spectral resolution, point spread function (PSF) stability, and noise variance requirements flow from the science requirements document (DESI-0318). The throughput requirements flow from the system throughput budget (DESI-0347). The temperature requirements flow from the DESI environmental requirements document (DESI-0583). The fiber diameter was chosen to optimize the signal-to-noise ratio in emission line galaxies (DESI-0304). The focal ratio was chosen to ensure greater than 90% throughput due to the focal ratio degradation of the fibers given the $f/3.85$ beam input into the fibers by the corrector (Figure 4.4).

Table 5.1: Spectrograph Requirements.

Item	Requirement	Current Design
Bandpass	360–980 nm	complies
Resolution ($\lambda/\Delta\lambda$)	$\geq 1,500$; $360 \text{ nm} < \lambda \leq 555 \text{ nm}$	2,000–3,200
	$\geq 3,000$; $555 \text{ nm} < \lambda \leq 656 \text{ nm}$	3,200–4,100
	$\geq 4,000$; $656 \text{ nm} < \lambda \leq 980 \text{ nm}$	4,100–5,100
End-to-end throughput	$\geq 21\%$; $\lambda = 360 \text{ nm}$	39%
	$\geq 30\%$; $\lambda = 375 \text{ nm}$	51%
	$\geq 43\%$; $\lambda = 400 \text{ nm}$	60%
	$\geq 55\%$; $\lambda = 450 \text{ nm}$	73%
	$\geq 57\%$; $\lambda = 500 \text{ nm}$	69%
	$\geq 54\%$; $\lambda = 550 \text{ nm}$	68%
	$\geq 50\%$; $\lambda = 600 \text{ nm}$	69%
	$\geq 56\%$; $\lambda = 650 \text{ nm}$	72%
	$\geq 58\%$; $\lambda = 700 \text{ nm}$	70%
	$\geq 56\%$; $\lambda = 750 \text{ nm}$	66%
Point Spread Function Stability	$\leq 1\%$	TBD
	Number of Fibers	5,000
	Fiber diameter	107 μm
	Collimator $f/\#$	≤ 3.57
	Noise Variance	$\leq 25\%$ of sky
Operational Temperature	-10°C to $+30^\circ\text{C}$	complies
Survival Temperature	-20°C to $+40^\circ\text{C}$	complies

The spectrograph specifications are derived from the requirements and the baseline design and are given in Table 5.2. These values lead to the optical design. Ten spectrographs must be used to support the 5,000 fibers of the DESI instrument. The temperature of the spectrographs must be controlled better than the operational limits in Table 5.1 to meet the requirements. The spectrographs will be mounted in two stacks of three and one stack of four in a temperature controlled enclosure in the Coudé room at the Mayall telescope.

5.1 Spectrograph Optical Design

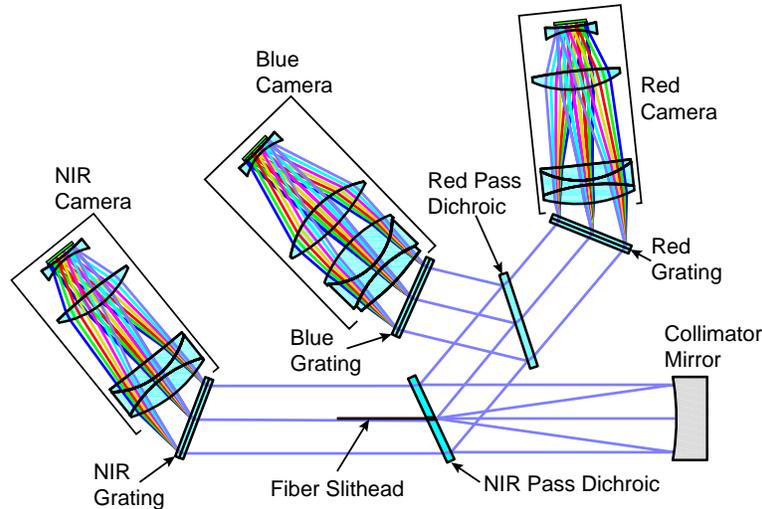
Once the specifications are defined a literature search (DESI-0755) of astronomical spectrographs was done to help limit the design space of the spectrograph. A trade was done on whether the

Table 5.2: Spectrograph Baseline Design Specifications.

Item	Specification	Current Design
Number of spectrographs	10	complies
Detector pixel pitch	15 μm	15 μm
Spectral detector elements	4,096 pixels	complies
Spatial detector elements	4,096 pixels	complies
Minimum resolution elements	3 pixels	3.4 pixels
Fiber spacing (slit plane)	230 μm	230 μm
Slit Height	120.9 mm	120.9 mm
Number of fibers (spatial)	500	500
Maximum rms Radius	$\leq 13 \mu\text{m}$	11.5 μm
Fiber - Fiber Crosstalk	$\leq 0.5\%$	0.05–0.46%
95% Encircled energy diameter	$\leq 110 \mu\text{m}$	61–82 μm
50% Encircled energy diameter	$\leq 50 \mu\text{m}$	37–45 μm
Operational Temperature	20°C \pm 2°C	complies

optics should be refractive or reflective (DESI-0757). More discussion of the results of this study will be in the collimator and camera sections. For more detail on the spectrograph optical design see DESI-0334.

Since the spectral range is more than a factor of two, the spectrograph bandpass needs to be split into at least two channels, using dichroic filters, to eliminate second order contamination. A trade study was done to find the optimal number of channels (DESI-0756). Three channels had the highest throughput and could use standard 4096 x 4096 detectors. The schematic of the optical layout of the spectrograph is shown in Figure 5.1. The light from the fiber slit is collimated by a spherical mirror. The light is then split into three spectral band passes using two dichroics. Each of the three channels disperses the light with a volume phase holographic (VPH) grating. The light is then focused onto the detector using a 5 lens camera.

**Figure 5.1:** The spectrograph schematic.

The magnification of the spectrograph is the ratio of the camera to collimator focal ratios. The collimator accepts the $f/3.57$ light from the fibers. The fiber diameter is 107 μm and it must project to a minimum of 45 μm (3 pixels) on the detector. This gives the minimum spectrograph

magnification of 0.42. Given the slit height of 120.9 mm, which must map to less than 60.02 mm on the detector, the maximum spectrograph magnification is 0.496.

If the optics of the spectrograph have no aberrations, the projected fiber diameter on the detector is just $m \cdot d$, where m is the magnification of the spectrograph and d is the diameter of the fiber. The spectral resolution of an arm of the spectrograph can then be estimated from equation 5.1.

$$R(\lambda) \approx \frac{2\lambda D}{\sqrt{3}md(\lambda_{max} - \lambda_{min})}. \quad (5.1)$$

R is the FWHM spectral resolution, λ is the wavelength, D is the size of the detector, λ_{max} is the maximum wavelength of the channel and λ_{min} is the minimum wavelength of the channel. Since the diameter of the fiber and the detector width are fixed the only variables in the spectrograph design are the magnification and the minimum and maximum wavelengths of the channel. Initial spectrograph design parameters were derived using equation 5.1 and the spectral resolution requirements from Table 5.1. There is no unique solution; the design chosen has the maximum magnification possible that met the resolution requirements. This results in the slowest possible camera, which is easier to manufacture. The bands chosen that meet the requirements are: 360–593 nm, 566–772 nm, and 747–980 nm for the blue, red and near infrared (NIR) channels respectively.

5.1.1 Fiber Slit

The slithead is very similar to the BOSS design [16] and consists of a thin, stiff plate with a curved edge of radius 468 mm having 500 fibers. The 107 μm diameter fibers are mounted in groups of twenty five in v-groove blocks, with 20 v-groove blocks being bonded to each slithead. The center-to-center spacing between fibers on adjacent v-groove blocks is 556 μm , compared to 230 μm between fibers within a v-groove block. The larger gap imaged on the CCDs is used to understand the PSF wings in the spectral extraction process (Section 7.3.1.3). The total length of the arc is 120.9 mm from outside edge to outside edge of the first and last fibers, 18 mm shorter than the BOSS design. The slit is inserted into a slot milled into the first dichroic with the center fiber tangent to the reflective surface of the dichroic.

5.1.2 Collimator

The collimator can either use reflective or refractive optics. A trade was performed (DESI-0757) which showed that a reflective collimator was the best. It has fewer optical surfaces (only 1) and slightly higher throughput than a refractive collimator. The spherical collimator mirror is similar to the BOSS design [16]. The collimator mirror is coated with an enhanced silver coating. A plot of the reflectivity of silver and aluminum is shown in Figure 5.2. The silver curve is from measurements of the BOSS collimator. The aluminum curves are from published vendor data. On average silver has about 10% higher throughput than aluminum. The $f/\#$ is 3.57 and the pupil is 126 mm.

5.1.3 Dichroics

Dichroic beam splitters are used to split the band pass into three. The dichroics can be placed between the fibers and the collimator or after the collimator. Dichroics in the diverging beam of the fibers will have a lower throughput than in the collimated beam. We have chosen to place them after the collimator to increase the throughput of the spectrograph.

The dichroic beam splitters reflect the short band pass and transmit the longer band pass. They are fused silica optical flats coated with the dichroic on one side and an anti-reflection coating on

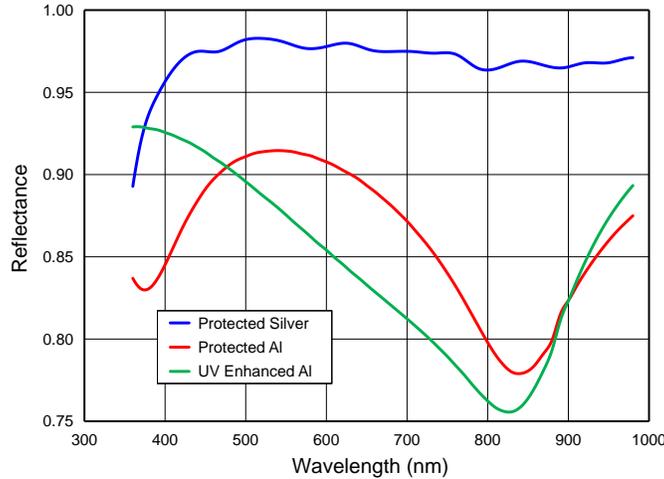


Figure 5.2: Reflectance of silver versus aluminum. Silver is the blue curve. two types of Al are the red and green curves.

the other. The specifications for the dichroic are shown in Table 5.3. More detailed specifications are given in DESI-1058.

Table 5.3: Dichroics Budgeted Requirements.

	NIR Pass Dichroic	Red Pass Dichroic	Throughput
Reflection Band (nm)	360–747	360–566	> 95%
Transmission Band (nm)	772–980	593–747	> 95%
Crossover Region R+T (nm)	747–772	566–593	> 90%
Crossover Width (nm)	25	27	

5.1.4 Gratings


The spectral resolution requirement, desired spectral overlap between the bands and the detector define the three band passes. The band passes and grating parameters are given in Table 5.4. Volume phase holographic (VPH) gratings have been chosen as the spectral dispersers. This type of grating delivers the best throughput over the relatively broad band passes of the three channels. The VPH grating is made by sandwiching a gelatin between two fused silica optical flat plates. Fringes are holographically recorded in the gelatin. $\Delta\beta$ is the dispersion angle, α is the incident angle, $1/\sigma$ is the line density, and ϕ is the tilt angle of the fringes. The fringes of the gratings are tilted to remove the Littrow ghost [17]. Our studies showed that high efficiency is maintained at the band pass edges when the grating spectral dispersion ($\Delta\beta$) was kept to less than 16° . The clear aperture of the gratings are kept below 145 mm so smaller holographic recording tables can be used to reduce the cost.

Full sized demonstration gratings for the three channels have been purchased and tested for their critical performance parameters of efficiency and wavefront error. Figure 5.3 shows a photo of the three gratings in a test mount. Figure 5.4 shows measurements of the wavefront error, from a Zygo interferometer. The peak to valley wavefront error for power and irregularity are below the budgeted 1.5 and 0.5 waves. The efficiency of the gratings have been measured by the vendor and remeasured at LBNL including as a function of incident angle α . The vendor results are shown in Figure 5.5. The LBNL results are shown in Figure 5.6. The efficiency performance is good and

Table 5.4: Spectrograph Grating Budgeted Requirements.

	Blue Channel	Red Channel	NIR Channel	Driver
λ_{min} (nm)	360	566	747	
λ_{max} (nm)	593	772	980	
$\Delta\beta$ ($^\circ$)	15.74	15.5	15.42	Throughput
α ($^\circ$)	10.44	18.12	20.76	Littrow ghosts
$1/\sigma$ (l/mm)	1101.9	1157.4	992.5	Littrow ghosts
ϕ ($^\circ$)	-3.18	-3.03	-2.97	Littrow ghosts
Band Edge Efficiency	> 65%	> 80%	> 80%	Throughput

performance optimization within $< 1^\circ$ of the specified incidence angle, α , is achieved as required.

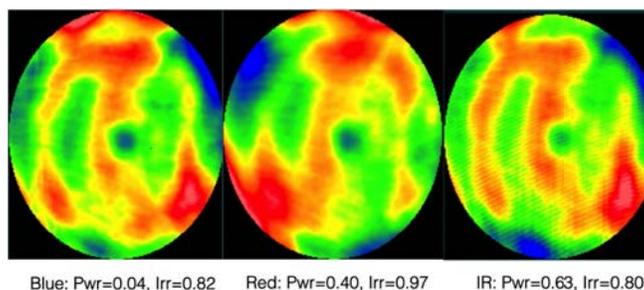**Figure 5.3:** Photographs of the blue, red and NIR gratings in test mounts, from left to right.**Figure 5.4:** Measured blue, red and NIR grating wavefront in -1 order, from left to right. Power and Irregularity wavefront are indicated by Pwr and Irr, respectively.

5.1.5 Camera

The cameras can use either reflective or refractive optics. The reflective Schmidt cameras use an aspheric corrector plate, spherical mirror and field flattener lenses. The detector obscures the beam with a loss of at least 10 - 15%. Refractive cameras have no obscuration but require more optical surfaces. The BOSS camera [16] used 8 lenses, two with aspheric surfaces. The refractive design was chosen since it has higher throughput. See DESI-0757 for more details on the trade.

The focal ratio of the camera will determine the spectral resolution of the camera and the focal length will determine the spectral coverage. The optical requirements for the cameras are given in Table 5.5. An area of the detector less than the full size was used to image the spectra in order to reduce the impact of edge effects and allow for alignment tolerances. The throughput requirements are budgeted from the requirements in Table 5.1.

The design considerations to reduce cost were: minimize the number of lenses, minimize the number of aspheric surfaces, minimize the volume of glass, use low cost glass with frequent melts.

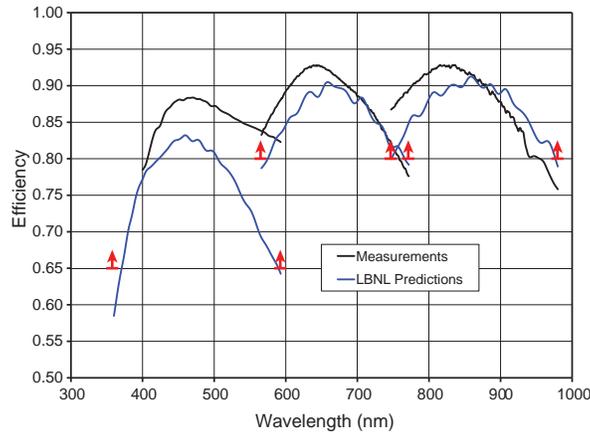


Figure 5.5: The vendor measured efficiency of the gratings is shown in black. The predicted efficiency is shown in blue and the requirements at the band edges are shown in red. The vendor could not measure the efficiency of the blue grating below 400 nm.

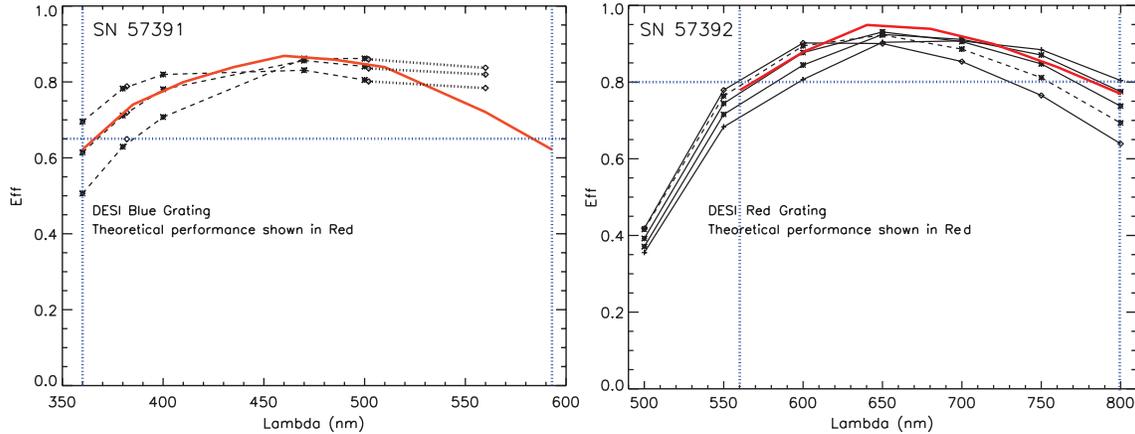


Figure 5.6: The LBNL measured efficiency of the blue (left) and red (right) gratings are shown as a function of the incident angle, α on the left and right, respectively. The predicted efficiency is shown in red and the specification is in blue. Tilting the gratings incidence angle within ($< 1^\circ$) of its specified value achieves efficiency optimization across the band, as desired. The vertical dashed lines are the bandpass edge locations and the horizontal dashed line are the required bandpass edge throughputs.

To maximize the throughput the number of lenses was minimized and only glasses with high transmission in the band pass were used. The last lens is fused silica since it is the vacuum seal to the cryostat. Fused silica is very strong and stiff and it is not radioactive which would increase the backgrounds in the detector.

The camera design was optimized using Zemax[®]. The optical design was only allowed to have a maximum rms radius of $< 10 \mu\text{m}$ to allow room for manufacturing and alignment tolerances. Physical constraints on the design were: window to CCD $> 3 \text{ mm}$, lenses 5 mm larger in radius than clear aperture for mounting, center thickness $> 10 \text{ mm}$, edge thickness $> 5 \text{ mm}$, total lens thickness $< 80 \text{ mm}$ (but as small as possible), contact surfaces 0.25 mm center thickness, non contact surfaces $> 5 \text{ mm}$ distance. The design started with variations on the BOSS design [16] which has 8 lenses, 2 aspheric surfaces and 7 glass types. An exhaustive study by three optical engineers on glass choice and design choice was done. The final design is a field flattened Petzval

Table 5.5: Camera Optical Budgeted Requirements.

	Blue	Red	NIR
Maximum rms spot radius (μm)	< 12	< 12	< 12
Angular field ($^\circ$)	7.72	7.72	7.72
Spectral field (nm)	360–593	566–772	747–980
Spectral field size ($^\circ$)	8.06	8.03	8.03
Focal length (mm)	212.8 ± 1	213.6 ± 1	214.0 ± 1
Focal Ratio	f/1.70	f/1.70	f/1.70
Spectral Detector Size (mm)	60.26	60.26	60.26
Spatial Detector Size (mm)	60.02	60.02	60.02
Throughput	> 86%	> 92.5%	> 92.4%
	@ $\lambda = 360$ nm	@ $\lambda = 560$ nm	@ $\lambda = 740$ nm
	> 90%	> 92%	> 91%
	@ $\lambda = 600$ nm	@ $\lambda = 650$ nm	@ $\lambda = 980$ nm
		> 93%	
		@ $\lambda = 780$ nm	

design with a contact triplet. All of the channels have 5 lenses with 2 aspheric surfaces (the front of the first lens and the front of the last lens). The optical optimization requires that the detector cryostat window and CCD are tilted and offset from the optical axis. The blue camera uses three glass types including CaF_2 . The red and NIR cameras have 4 standard glass types. A schematic of the cameras is shown in Figure 5.1.

The optical design of the spectrograph was analyzed using Zemax[®] to make sure that it meets requirements. The spot sizes for the spectrograph are shown in Figure 5.7. The maximum rms radius versus wavelength is in Figure 5.8. The design meets the requirement of $<10 \mu\text{m}$ rms at all wavelengths.

The red and NIR triplets are bonded with UV curing glue. An FEA analysis of the triplet was done to determine the stress and strain on the glass and the glue. Then a smaller doublet was made that would have twice the stress of the full size triplet. The doublet was manufactured and bonded. It was then put through three thermal cycles from -20 to $+40$ $^\circ\text{C}$ (DESI-1107). The shape error was measured and a visual inspection of the lens were performed both before and after the thermal cycle. The doublet lens passed the thermal cycle test.

The blue triplet was initially going to be bonded with Silicon RTV. A full scale triplet was made and bonded. It failed the thermal cycle test. Then the triplet was redesigned to use Cargille 1074 laser liquid to couple the lenses. The oil cell is very similar to the design used by the KOSMOS spectrograph [18]. The oil cell passed its thermal cycling test. In addition, the 1074 oil was exposed to the silicone o-rings and diaphragm for 30 months and the transmission was remeasured. The transmission of the oil did not change as a result of exposure to the materials.

The mechanical design of the blue camera is shown in Figure 5.9. The VPH grating mount is shown in dark blue on the right. The triplet oil cell is shown next in gray and purple. The lateral adjustable cell for the fourth lens is shown next in pink and purple. Finally the field lens cell is shown in light green with a orange baffle. All of the lens cells are thermally compensated axially and radially.

An optical thermal analysis of the cameras was done. For the operation range 18 – 22 $^\circ\text{C}$ the red and the NIR cameras did not require passive athermalization. The blue camera did need passive athermalization. This was done by inserting PTFE plastic in the cell of the fourth lens. See the white piece in the cell in Figure 5.9.

The prototype spectrograph fabrication has started. Photographs of several of the parts under

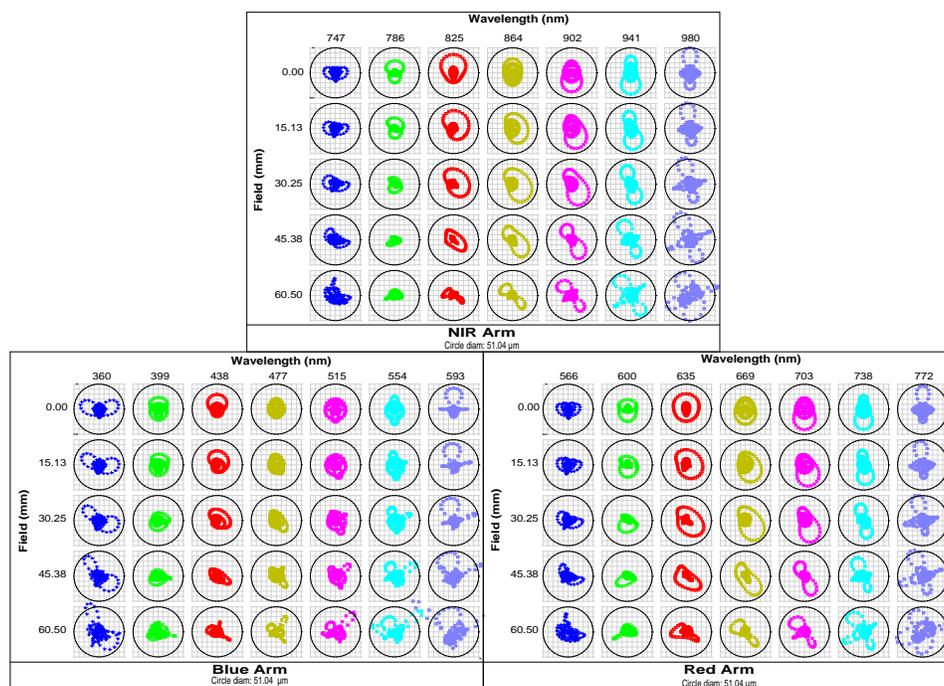


Figure 5.7: The ray traced spot diagram for the spectrograph. The lower left figure is for the blue channel, the lower right figure is for the red channel and the upper figure is for the NIR channel. The circle is the size of the projected fiber onto the detector.

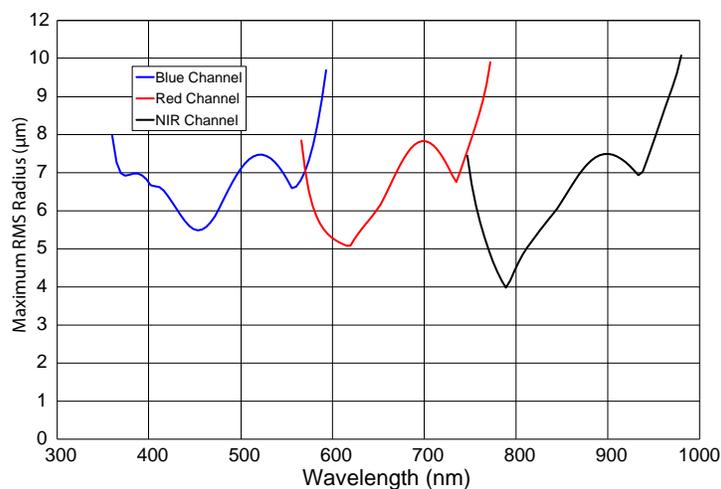


Figure 5.8: The maximum rms radius versus wavelength for the optical design is plotted. The blue, red and black curves are for the blue, red and NIR channels of the spectrograph respectively. All wavelengths meet the 10 μm rms requirement for the optical design.

manufacture are shown in Figure 5.10. The collimator mirror, L1 and L2 lenses for the red camera, test oil cell for the blue camera, lens barrel parts and the three lens barrels are shown.

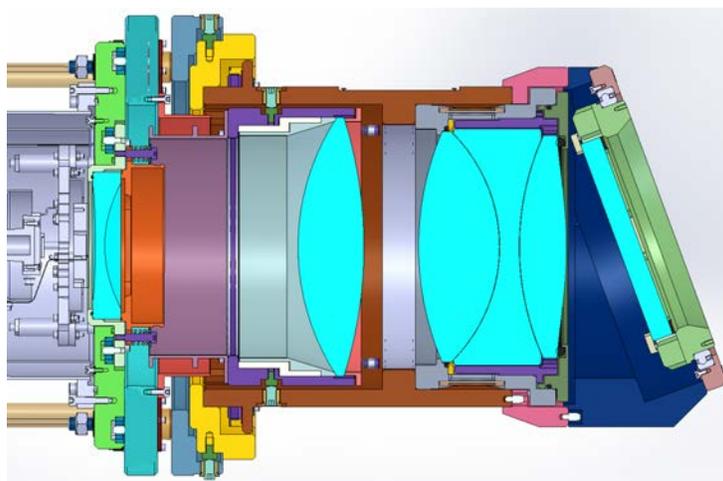


Figure 5.9: Section of the mechanical design of the blue camera.

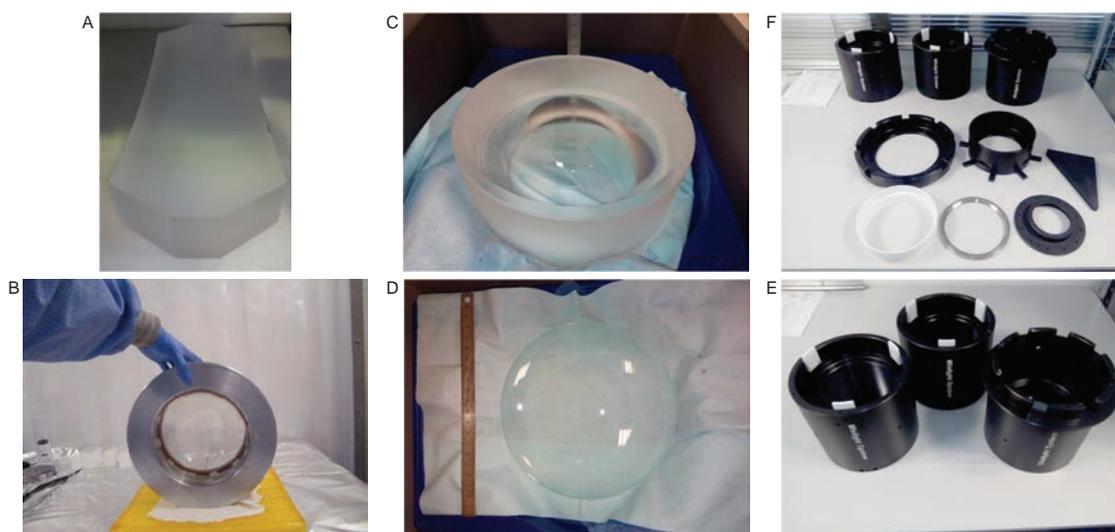


Figure 5.10: Photographs of several prototype spectrograph components. A: The ground collimator mirror. B: The test oil cell for the blue camera. C: 200 mm diameter L2 lens for the red camera. D: 180 mm diameter L1 lens for the red camera. E: Various camera barrel components. F: The three lens barrels for the red, NIR and blue cameras.

5.1.6 Tolerancing and Simulation

There are several effects that will change the imaging of the spectrograph from the optical design. The optics will not be manufactured or assembled perfectly. The illumination pattern from the fiber is not uniform. The detector will blur the images due to charge diffusion and depth of conversion. And diffraction will add wings to the images. These effects were simulated to see if the as manufactured spectrograph (including detector) will meet the imaging requirements of the spectrograph.

A preliminary tolerance study of the spectrographs was done to determine the as built performance of the spectrograph. The typical allowed tolerances for the cameras were 0.3% in the radius of curvature, 0.2 mm for thickness, 0.05 mm for the decenter of the lenses, 1 arcminute for the tilts, 1 wave for transmitted power optical path difference (OPD), 1/2 wave transmitted irregular

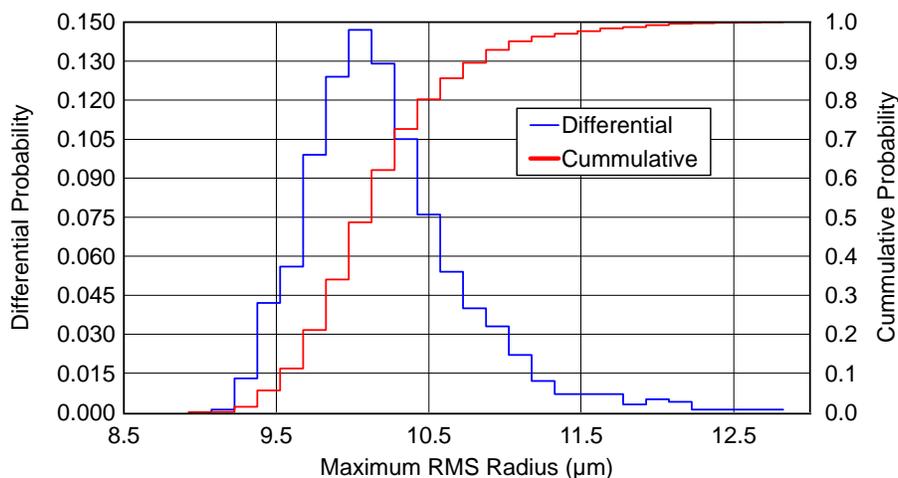


Figure 5.11: Statistics from the Monte Carlo simulations for the tolerancing of the red channel of the spectrograph. The blue curve is the differential probability distribution and the red is the cumulative distribution.

OPD. A few of the lenses for the red and NIR channels had to have slightly tighter requirements than listed above to meet the maximum rms radius of $12 \mu\text{m}$. Two of the radii of curvature in the blue channel have significantly tighter tolerances to meet the requirements. The detector tolerances were 0.015 mm P-V flatness, 0.125 mm piston and 2 arcminute tilt. The collimator mirror had a radius of curvature tolerance of $\pm 6 \text{ mm}$, an irregularity of $1/10 \text{ wave}$ OPD a tilt of 1 arcminute and piston of 0.125 mm for piston. Both dichroics had a power OPD of 1.5 wave and an irregularity OPD of 1 wave , 2 arcminutes of tilt and 0.125 mm of piston. The gratings had a power OPD of 1.5 waves , 1 wave of irregularity OPD, 2 arcminutes of tilt and 0.125 mm of piston. The compensator for the red and NIR channels was the distance and decenter of the window/detector assembly with respect to the other 4 lenses. The blue channel also added the spacing and decenter of the fourth lens with respect to the triplet as compensators.

A Monte Carlo simulation of 1,000 spectrographs was performed to determine if the tolerances meet the requirements. The results for the red channel are shown in Figure 5.11. All the channels were similar to this. The most likely spectrograph had a maximum rms radius of $\sim 10 \mu\text{m}$ and 95% of the spectrographs were better than $11 \mu\text{m}$. A representative description of the as built optics was chosen from the 1,000 Monte Carlos such that there is a 95% chance that the as built camera would be better.

A measured angular illumination pattern from a fiber was used as the input into the simulated as-built optics. Diffraction was then added to the output. This combined image was then input into a detector simulator to add the charge diffusion and depth of conversion effects. Two detector types were used in the simulation. For the blue channel a thin substrate detector with $5 \mu\text{m}$ diffusion was used. For the red and NIR channels a $250 \mu\text{m}$ thick fully depleted model was used with a $5 \mu\text{m}$ diffusion.

The FWHM spectral resolution ($\lambda/\Delta\lambda$) for the simulated spectrograph is shown in Figure 5.12. The red curve is the minimum spectral resolution for all fibers and the blue curve is the average. The requirement of Table 5.1 is plotted as the dashed orange line. The spectral resolution requirement is met at all wavelengths.

The 50% encircled energy diameter for the simulated spectrograph is shown in Figure 5.13. The red curve is the maximum for all fibers and the blue curve is the average. The simulated

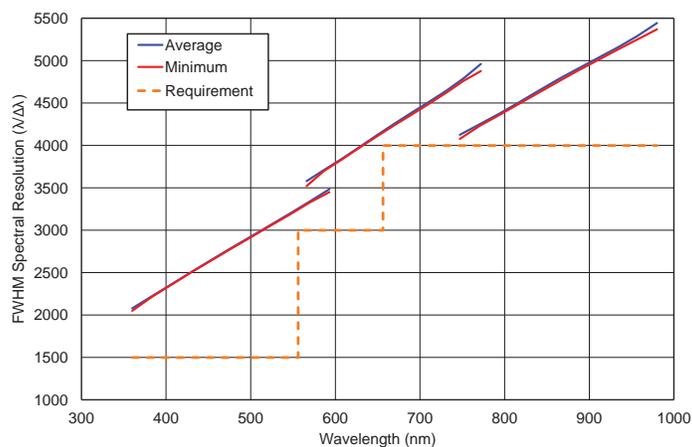


Figure 5.12: The minimum and average FWHM spectral resolution versus wavelength for the simulated spectrograph. The red curve is the minimum spectral resolution, the blue curve is the average resolution and the dashed orange curve is the requirement.

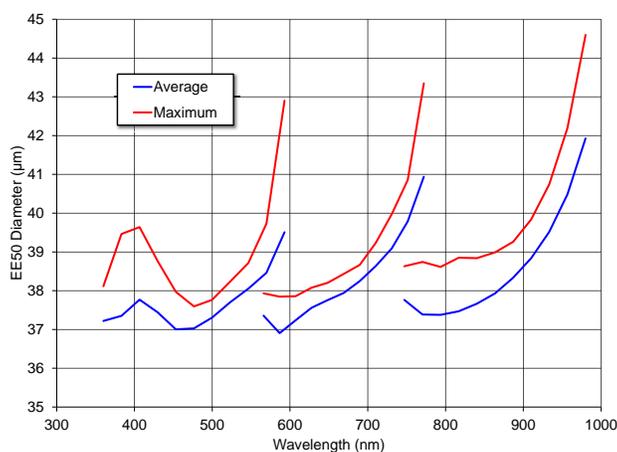


Figure 5.13: The average (blue) and maximum (red) diameters of the 50% encircled energy versus wavelength for the simulated spectrograph. The requirement is $< 50\mu\text{m}$.

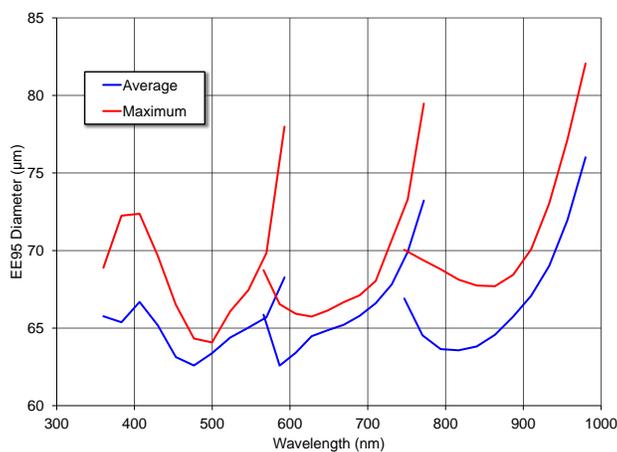


Figure 5.14: The maximum diameter of the 95% encircled energy versus wavelength for the simulated spectrograph. The requirement is $< 110\mu\text{m}$.

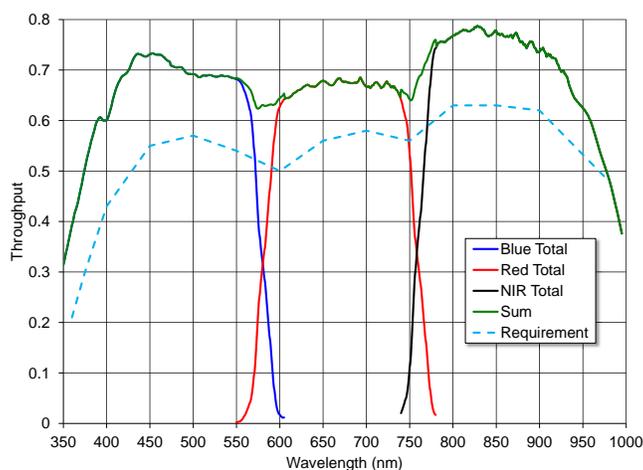


Figure 5.15: The estimated throughput of the spectrograph. The blue, red and black curves are for the blue, red and NIR channels respectively. The green curve is the sum of the channel throughputs and the dashed blue curve is the requirement.

spectrograph meets the requirement of $< 50 \mu\text{m}$ from Table 5.1 for all wavelengths and all channels.

The 95% encircled energy diameter for the simulated spectrograph is shown in Figure 5.14. The red curve is the maximum for all fibers and the blue curve is the average. The simulated spectrograph meets the requirement of $< 110 \mu\text{m}$ from Table 5.1 for all wavelengths and all channels.

The throughput of the spectrograph, from the fiber to the CCD, was also simulated. The transmission of the cameras were estimated using the published vendor data and Zemax. The antireflection coatings on the lenses were assumed to have a transmission of 99% in blue channel and 99.5% in the red and NIR channels. The collimator mirror reflectance is from the BOSS collimator measurements. The dichroic performance was estimated by scaling measurements of the BOSS dichroic beam splitters. Grating efficiencies were the measurements from the vendor. The quantum efficiency of the CCD detectors was estimated using measurements of current detectors. The estimated throughput is shown in Figure 5.15. The blue, red and black curves are for the blue, red and NIR channels respectively. The green curve is the sum of the channel throughputs and the dashed blue curve is the requirement from Table 5.1. The throughput meets the requirement for all wavelengths.

5.2 Spectrograph Mechanical and Electrical Design

A CAD rendering showing the major mechanical components of the spectrograph is shown in Figure 5.16. The major mechanical components of the spectrograph are the bench, shutters, Hartmann doors, fiber illuminator, CCD flat field illuminator, and thermal sensors.

The optical bench is an aluminum structure with precision machined interfaces to locate the seven opto-mechanical subassemblies: the fiber slit head, the collimator, the two dichroics, and the three camera/grating assemblies. At all of these opto-mechanical interfaces precision-machined reference datums and kinematic-locating features are employed to ensure accurate, repeatable alignment of the optical system. The optical components have passive thermal compensators in them to maintain the focus over the 18–22 °C operational temperature range. There is an enclosure that also mounts to the bench. It blocks external light and is semi-hermetic so that a purge of dry air will prevent condensation on the cold cryostat window. A schematic of the mechanisms for the spectrograph is shown in Figure 5.17.

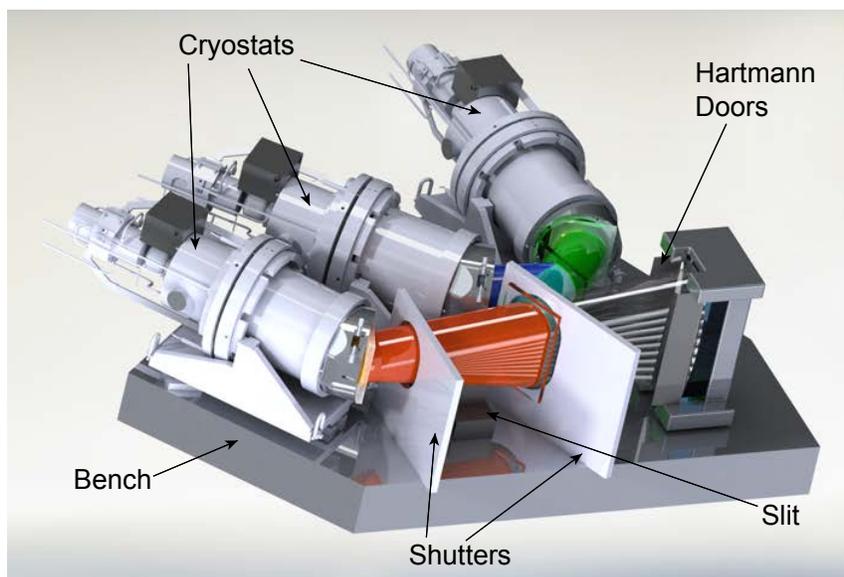


Figure 5.16: A CAD rendering of the spectrograph. The colored cylinders are the light beams. The fiber illuminator, CCD flat field illuminator, thermal sensors and light enclosure are not shown. The spectrograph is 1.8 m wide \times 1.4 m deep \times 0.6 m high.

The fiber illuminator is an LED light source that is moved in front of the fiber slit head when it is in operation. It is used to back illuminate the fiber tips at the corrector focal plane so the Fiber View Camera (Section 3.6) can measure the location of the fibers. The fiber illuminator should produce at least 10^{10} photons/second into the $f/2.2$ acceptance cones of each fiber (DESI-0652, -0939). These photons should be in the 400–557 nm bandpass to be detectable by the fiber view

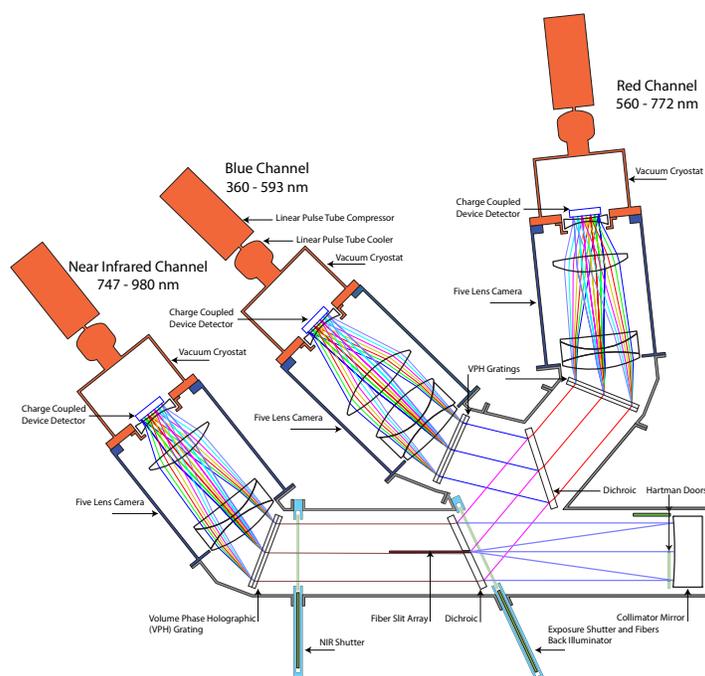


Figure 5.17: Schematic of the mechanisms of the spectrograph.

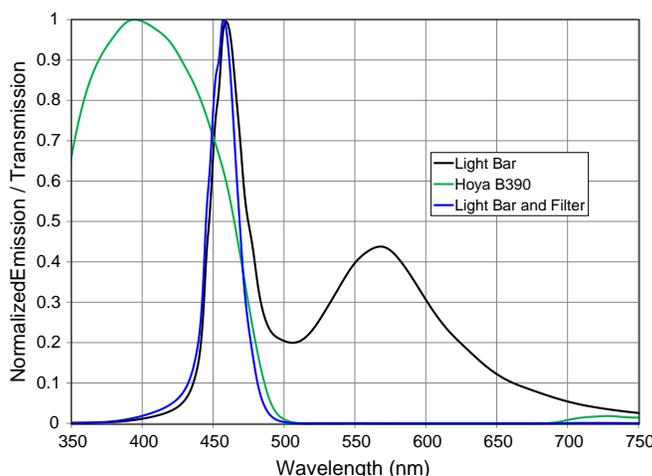


Figure 5.18: Spectral energy distribution of the Linear Chip On Board LED (*black*), transmission of the Hoya B390 filter (*yellow*), and output spectrum (*blue*).

camera, yet not interfere with the guiding CCD. A 3-Watt Linear Chip On Board LED, combined with a 3-mm thick Hoya B-390 filter, produces sufficient photon flux in the required bandpass (Figure 5.18). The LED will be mounted in a machined aluminum cell, covered with a thin film diffuser and the filter, and placed behind a narrow slit that will primarily direct light into the fiber ends. The fiber illuminator is mounted to the back of the exposure shutter (Figure 5.19) and positions the LEDs close to the fiber slit when closed.

The shutters are used to block light from the CCDs during readout, including light from the fiber illuminator. The fiber illuminator will usually be operated during CCD readout, so the shutters are required to transmit less than 10^{-7} of the photons at the fiber tip (DESI-0652). The exposure shutter is mounted in front of the first dichroic (Figure 5.17). The NIR shutter is mounted in front of the NIR camera. The exposure shutter is used to control the exposure of the three channels

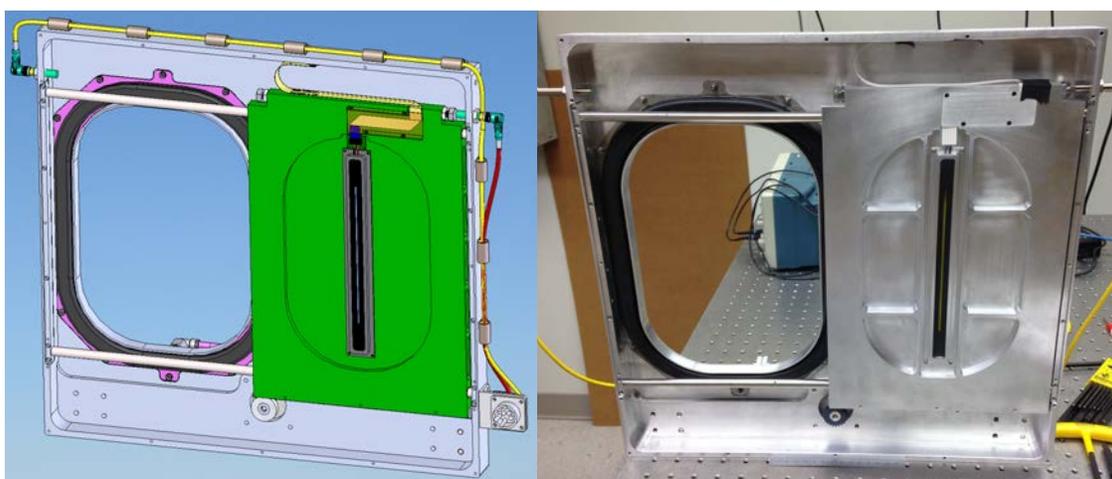


Figure 5.19: Left: Model for the Exposure Shutter shown in the open position and without one cover in place. This model shows the PneumaSeal inflateable seal around the aperture (*black*) and the fiber illuminator LED mounted in the middle of the shutter door (*green*). Right: First fabricated unit.

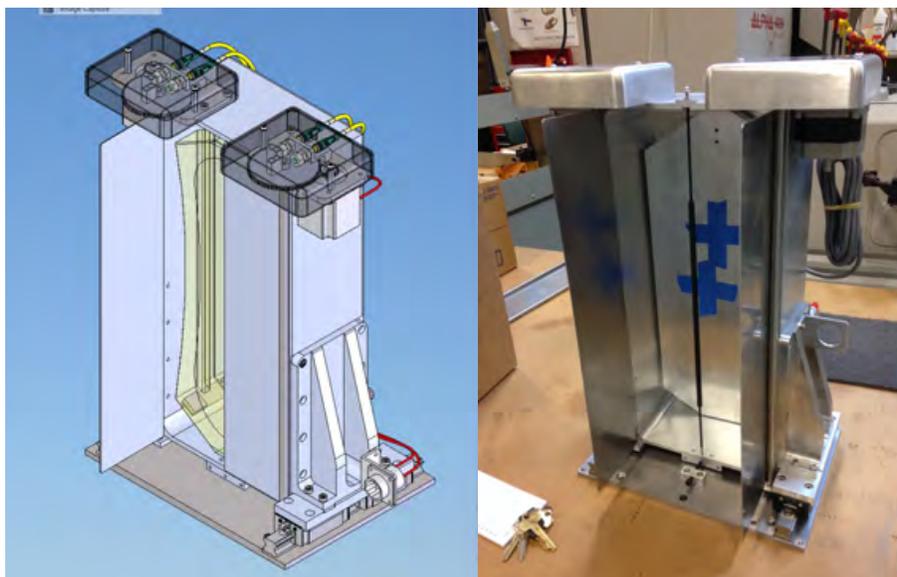


Figure 5.20: Model for the collimator mount and Hartmann doors. Left: Front of the mount with one door open. Right: First-unit mount with both doors open; the blue crosses are on a replica of the collimator mirror.

simultaneously, while the NIR shutter is just needed to block the light from the fiber illuminator. Both shutters are equipped with a PneumaSeal inflateable seal that has been measured to provide $> 10^{-9}$ attenuation of the LED flux. The seals operate at 10–15 psi and will only be inflated when the fiber illuminator is in operation.

All of the fibers in all channels will have the same exposure independent of the motion of the shutter because the shutter is near the pupil. The exposure shutter must open and close in less than 500 milliseconds, and must have a lifetime of at least 155,000 cycles (DESI-0584). The NIR shutter must open and close in less than 1 second, and have the same lifetime as the exposure shutter. The two shutters are identical mechanisms except the NIR shutter does not have a fiber illuminator. The shutters use a direct drive stepper motor with a rack and pinion gear, the blade slides on frelon-coated aluminum bushings, and the inductive proximity sensors detect when the shutter is fully open and fully closed.

The Hartmann doors are in front of the collimator mirror and part of the collimator mount (Figure 5.20). The doors are a simple bi-fold design, and each operates as an independent mechanism. They are used to determine the focus. The design is a smaller, modified version of the Hartmann doors used on BOSS [16].

The collimator mount has manual focus, tip, and tilt adjustments. The collimator is required to be insensitive to focus changes with less than $7.5 \mu\text{m}/^\circ\text{C}$ shift. The collimator focus is athermalized with a re-entrant focus mechanism of high CTE material, which compensates for the change in distance between the slit and collimator with temperature. Analysis of the design indicates it should produce a residual sensitivity of $\sim 2 \mu\text{m}/^\circ\text{C}$ due to uncertainties in CTE values. The collimator mirror is supported with three thin, stainless steel webs. These webs correct for the CTE differences between the aluminum mounting plate and the Zerodur mirror, yet minimize mirror distortion. FEA indicates that the mechanical mount produces less than 5 nm rms surface error in representative 128 mm diameter sub pupils (DESI-1077).

The CCD flat field illuminator is a replacement slit head with a “leaky” fiber that produces a nearly uniform illumination along its length. It has the same radius of curvature and interface

features of the fiber slit head. The leaky fiber is fed from a continuum light source to produce continuous light both, spatially and spectrally, onto the CCD detectors. This CCD flat field will be measured about once per year as was done for BOSS.

Environmental sensors will be mounted at several locations on the spectrograph. Platinum RTDs will monitor the temperature of the spectrograph to ensure that it is within the operational range. There will also be a humidity sensor near each cryostat window to ensure that the air is above the dew point.

In addition to the mechanical system there is a spectrograph controller. The spectrograph controller is housed in an electronics box on the optical bench. The controller includes motor controllers for the two shutters and two Hartmann doors, electronics for the fiber illuminator, air valves for the shutter seals, and connections for the temperature and humidity sensors. This controller is connected to the Instrument Control System (Section 6) via Ethernet. The spectrograph controller also contains a minicomputer that runs the code that operates the spectrograph and a router that isolates internal communication.

The ten spectrographs are mounted in five stacks of two in a climate controlled enclosure (Shack) in the Coudé room at the Mayall telescope (Figure 5.21). The temperature in the Shack is maintained within 18–22 °C and the relative humidity is kept below 85%. The cabling and access is designed to accommodate most maintenance operations without removing a spectrograph from the rack. The support rack will also include any vibration isolation that is needed.

The current concept for the Shack is to place the five racks in a row arrangement to allow access to the cryostat and slit sides of the spectrographs in their racks (Figure 5.21). There is also sufficient space to include an overhead gantry crane, which offers a safe way to perform maintenance with a minimal number of personnel. The Shack includes a Shack controller, which measures the Shack temperature and humidity, as well as monitors glycol and other utilities.

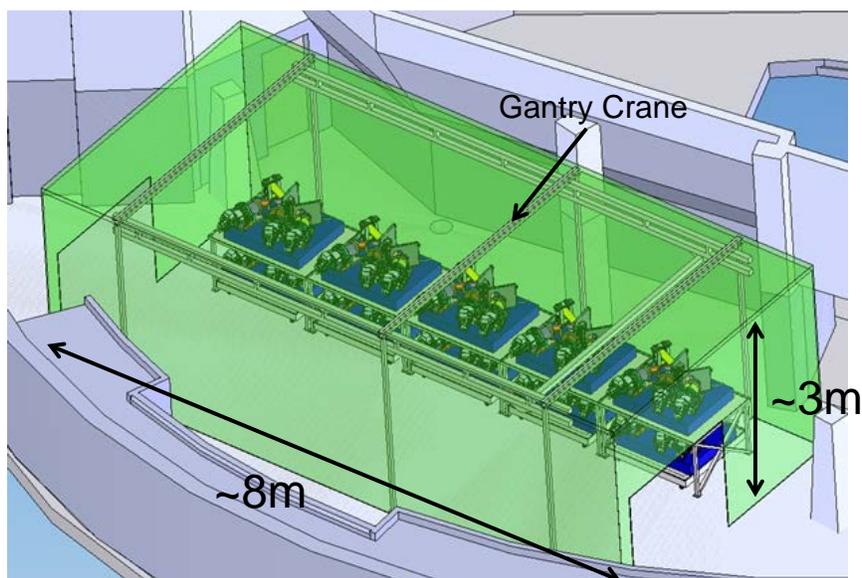


Figure 5.21: Concept for the arrangement of spectrographs within the climate-controlled, insulated “Shack.” There are five racks with two spectrographs each arranged in a row for easy front and back access. An overhead gantry crane is inside the Shack for installation and removal of mechanisms, cameras, cryostats, or even the entire ~500 kg spectrographs.

5.3 Spectrograph Integration and Test

The integration of the spectrograph occurs in four phases. First is the integration and alignment of the cameras. Second is the integration of the optics onto the bench. Third is the integration of the cryostats and mechanisms onto the spectrograph. Fourth is the integration of the spectrographs onto the racks at the Mayall telescope.

The integration and alignment of the cameras will be done by the camera vendor. They will align the lenses and measure the point spread functions (PSF) using a translating microscope with camera. The throughput will also be measured. In addition, the camera will undergo thermal cycle testing (to the survival limits) to ensure that the alignment does not change and the camera survives. They will also measure the PSF over the operational range to ensure that it does not change.

The gratings, dichroics, collimator and camera will be installed onto the camera bench by the spectrograph integrator. The grating angle will be adjusted to maximize the throughput. The spectrograph will be aligned using a tooling slit and the PSF measured using a microscope and camera. The PSF will be measured over the 18–22 °C temperature range to make sure it remains within specification.

The shutters, Hartmann doors, cryostat, and thermal and humidity sensors will be installed and aligned on the bench using a test fiber slit head. The throughput, PSF, and spectral dispersion of the spectrograph will then be measured. The PSF will be measured over the 18–22 °C temperature range to make sure it remains within specification. Finally scattered light will be quantified.

The spectrograph will then be disassembled and packed into its shipping container and shipped to NOAO. At Kitt Peak the spectrographs will be unpacked at the instrument handling facility (ISF). The functionality of the spectrographs will be verified there before being transported to the Mayall telescope. As it would be advantageous to unpack and test the spectrographs at the Mayall, rather than transporting them to the Mayall from the ISF after verification, two alternatives for reintegration are presently under consideration: an insulated room elsewhere in the Mayall and the Shack concept shown in Figure 5.21. After the spectrographs are placed in the rack, the last installation step is the addition of the fiber slit head.

5.4 Cryostats

The ten DESI spectrographs each require three CCDs for the blue, red, and NIR channels. Each CCD is housed in its own cryostat, each in turn with its own refrigerator and CCD control electronics. The main requirements for the design of the cryostat system are as follows:

- Cool CCDs to 140 K (LBNL CCDs) or 170 K (ITL CCDs) with a precision of 1 K and regulate their temperature to ± 0.1 K.
- Allow the CCDs to be aligned along the optical axis, in both transverse axes and tilt angles relative to the spectrograph optical axis.
- Provide easy access to the instrument for ease of maintenance and fast replacement (typically, one cryostat to be replaced in less than 24 hours by 2 persons).
- Monitor per cryostat the CCD temperature regulation, vacuum conditions, power supply, control and safety processes.

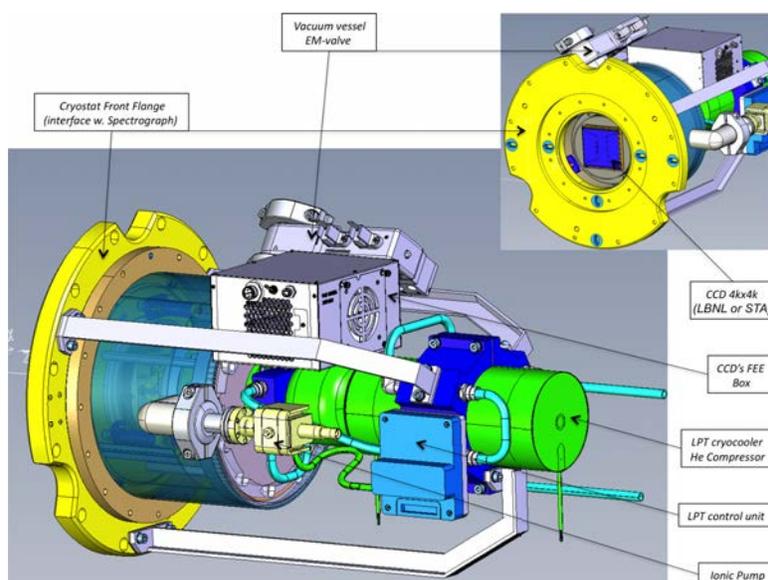


Figure 5.22: 3D model of the cryostat and view of the front side interface.

5.4.1 Cryostat Design and Interfaces

5.4.1.1 Mechanical Design

One of the most important cryostat requirements is to have identical units in order to be able to react quickly in case of changes or failures. So we adopt the same mechanical design for all cryostats (except for the front optical lens) in order to have interchangeability for each spectrograph arm.

The detector focal plane is determined by the optical configuration of the spectrographs and will be slightly different in each channel. The last lens of each spectrograph arm has to be part of the cryostat due to its short distance to the CCD plane. It will act as the vacuum window of the cryostat vessel. Figure 5.22 shows the cryostat 3D model. One cryostat weighs 25 kg, is 310 mm in diameter and 480 mm long.

The reference plane of the interface between the spectrograph and the CCD is the front face of the cryostat flange. The reference frame for the alignment is defined by high precision pin-holes located on this flange (Figure 5.23 left).

The last lens will be assembled and aligned in its mechanical mount, the Field Lens Assembly (FLA). Pin-holes will allow the camera and the FLA to be aligned by mechanical construction relative to the interface plane. Fine adjustment of the CCD plane position will rely on an $XY\theta Z$ stage and an optical measurement table. First, the CCD plane will be positioned parallel to the reference plane by adding shims between the front flange rear face and the feet of the cold plate bearing the CCD, controlling the position with the optical table. This ensures that the CCD plane coincides with the XY plane as defined in Figure 5.23 right. Then, the CCD $XY\theta Z$ position will be adjusted by moving the CCD with respect to the cold plate using the translation stage. The cold plate and its fixation elements were designed to ensure thermal expansion compensation between these pieces. The CCD is fixed on the cold plate with a screwing assembly. Thus the alignment achieved at room temperature will be valid in cold conditions. The above procedure will allow us to align the CCD plane within 100–200 μm along the optical Z axis and within 50 μm in transverse XY plane, the spectrograph optical requirements. The final focusing precision, $\pm 15 \mu\text{m}$ along Z , will be achieved by moving the camera relative to the cryostat, the camera vendor's responsibility.

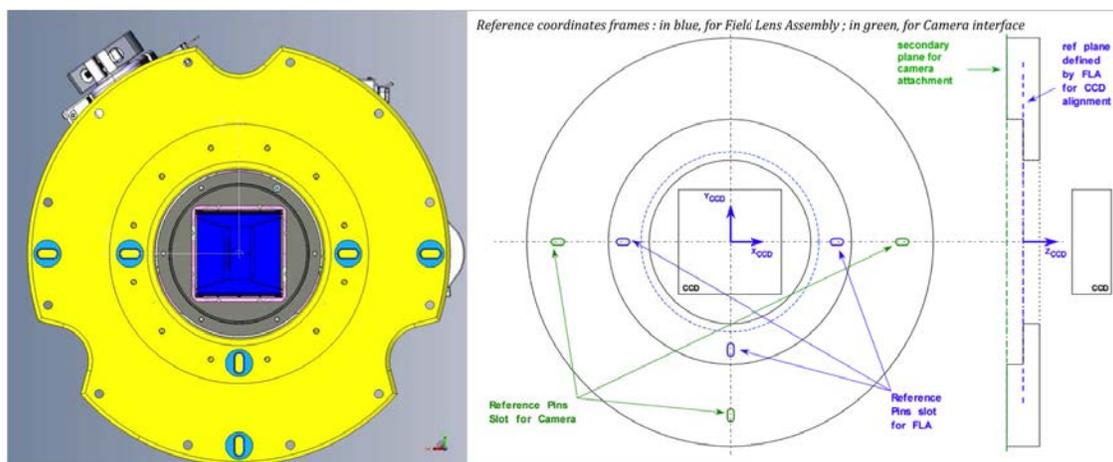


Figure 5.23: Reference frames system for the Cryostat Interface (blue for FLA, green for the spectrograph interface).

5.4.1.2 Cryostat Vessels

The cryostat vessel provides the mechanical connection to the spectrograph camera, supports the thermal and vacuum conditions, and interfaces with the control system and the CCD electronics. The cryostat is a metal cylinder which receives a front flange that integrates the FLA of the camera and supports the CCD on the vacuum side. A rear flange closes the vessel and supports the cryocooler (Figure 5.24). It has several hermetic connectors, one for the CCD flex to the front-end electronics box and two for temperature regulation and the monitoring by the control system. The cylindrical side is equipped with 2 ports for vacuum pumping and pressure gauges.

Cooling power is supplied from the refrigerator to the CCD through a set of mechanical links; the CCD on its Invar package is mounted on an Invar cold plate connected with flexible copper braids to a copper cold base screwed to the cold tip of the cryocooler. The Invar cold plate provides the mounting and positioning of the CCD and supplies cooling with minimal thermal losses. The CCD package and cold plate are made with low thermal expansion materials to reduce differential thermal constraints.

The copper cold base is dimensioned to have a thermal capacitance suitable for the CCD temperature regulation. Pt100 resistors fixed on the CCD package, the cold plate, the Cold Tip and on the front flange close to the FLA ensure thermal control and monitoring. A resistive heater is glued on the cold plate to control warm-up operations.

Thermal shielding of the cryostat is provided in three pieces, one for the vessel sides, one for the rear flange and one for the front lens. The latter is different for the 3 channels of the spectrographs, which have lenses of different diameters. The shielding will be provided by polished Al plates.

5.4.2 Cryogenic System and Performance

To produce cooling power for the 30 independent cryostats, a closed cycle cryocooler per cryostat is used, each with its own CCD temperature regulation. Pulse tube cooler technology is used in order to have a simple and robust system for the control of the 30 cameras, providing easy integration and maintenance.

To define an appropriate cryocooler model for DESI cryostats, we made a simple estimate of the power and temperature budget of the different elements of the cameras. The results are given in Table 5.6. The values are for a CCD temperature of 170 K and a maximum difference of 20 K

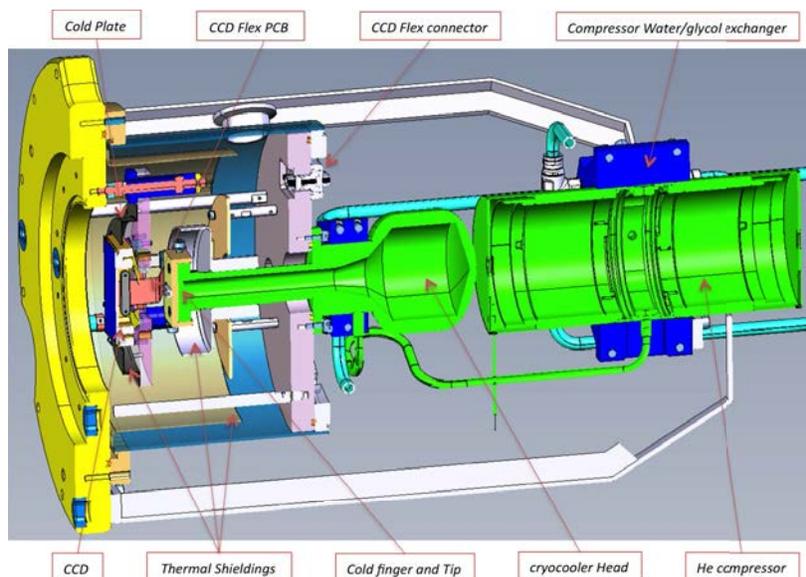


Figure 5.24: Cryostat cross sectional view.

with respect to the cold finger temperature. We would like the option to operate some CCDs as low as 140 K, which requires more than the 3 W. Thus we bought the Thales LPT9310 Cryocooler (4 W at 88 K) to evaluate in the prototype cryostat.

5.4.2.1 LPT Cryocooler

Linear Pulse Tubes (LPT) were developed by the “Service des Basses Temperatures” (SBT) at CEA in Grenoble (France). The technology was transferred to Thales Cryogenics BV Company which provides several models of LPTs with different power and temperature ranges (Figure 5.25). The LPT is a closed-cycle pulse tube cooler made of a compressor module and a cold finger, connected together by a metal tube. The compressor pistons are driven by integral linear electric motors and are gas-coupled to the pulse tube cold finger, which has no moving parts. This technology, combined with the proven design of the ultra-reliable flexure bearing compressors, results in extremely reliable and miniature cryocoolers with a minimum of vibrations. In addition, the compact magnetic circuit is optimized for motor efficiency and reduction of electromagnetic interferences. The compressor part is separated from the cold head by a He line which is bent in order to reduce vibration coupling.

The LPTs have a mean time to failure of more than 90000 hours at full power. To guarantee

Table 5.6: Estimated radiative and conductive thermal losses (at 10^{-5} mbar, convective heat transfer is negligible).

Element	Loss (W)	% of total loss
Lens (radiative)	1.9	62
CCD dissipation	0.12	4
CCD electronic cables	0.23	7
Cold plate / vessel (radiative)	0.16	5
Cold plate supports (conductive)	0.15	6
Cold base regulation capacity	0.5	16
TOTAL	3.06	100

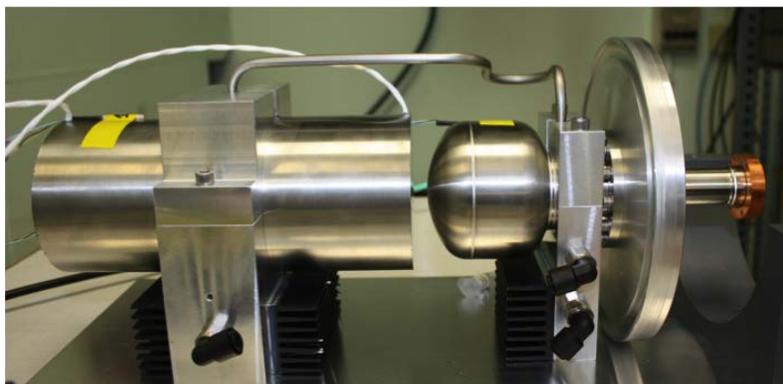


Figure 5.25: Thales 4W LPT9310 in DESI test stand.

this reliability over the lifetime of the instrument, we chose the LPT9310 model working at 25–30% of its maximal power. One unit (Figure 5.25) was integrated in a dedicated test cryostat at Saclay and its thermal performance validated. The results are shown in Figure 5.26. To obtain the latter, the cold head and compressor were cooled by a liquid distribution system, Glycol or Water, at about 5–10 °C with a flow of about a liter per minute and per LPT. This will be provided for each LPT by an existing cooling distribution at the Mayall telescope.

5.4.2.2 Device Monitoring and Temperature Regulation

The LPT compressor is powered with an AC voltage signal which sets the cold finger operating point in power and temperature. Changing this voltage allows the thermal performance to be tuned in a given range. The LPT is provided with an electrical interface called XPCDE (XP Cooler Drive Electronics) powered by an input DC signal (Figure 5.27). The CDE converts the input signal from DC to AC and adjusts the output voltage through a temperature regulation loop. This loop is based on an Proportional-Integral method, using a Pt100 temperature sensor. The XPCDE provides internal diagnoses about the thermal control process itself. Pre-tuning of the XPCDE is done by the manufacturer; fine tuning is done on each set of LPT unit in order to achieve extreme

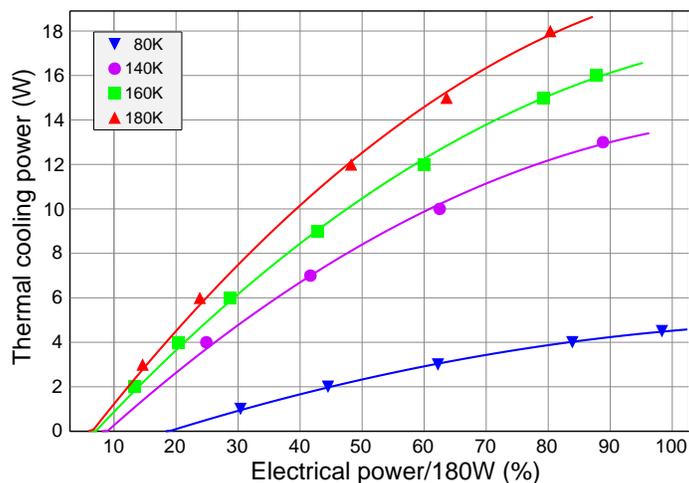


Figure 5.26: Saclay measurements of the LPT9310 thermal response for various cold-tip temperatures in a test cryostat.

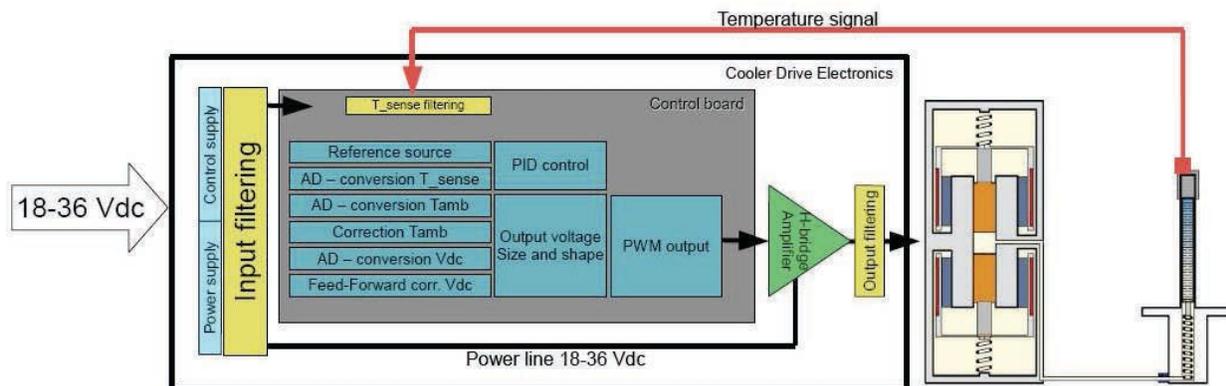


Figure 5.27: LPT9310 cooler drive electronics block diagram.

temperature stability. The tests (see Section 5.3) showed that the CDE is able to set and regulate the CCD temperature inside our cryostat provided that the regulation control loop P-I parameters are tuned.

5.4.2.3 Cryocoolers and Vacuum Maintenance

The LPTs have a mean time to failure of more than 90000 hours at full power and do not require routine maintenance. Monitoring the response of the LPTs will be implemented in the cryostat control system. In case of a unit failure, the LPT will be replaced by a spare and the faulty unit returned to the manufacturer for examination and repair.

The design of the vacuum system takes into account the mechanical assembly of the 10 spectrographs mounted in three towers. Each tower will be equipped with one vacuum unit. A vacuum unit is composed of a primary and secondary dry pumping machines (250 l/s) and a large conductance distribution line connected to the vertically aligned spectrographs (9 or 12 cryostats). With such a system, the time to reach 10 ± 5 mbar will be less than 5 hours. Each distribution line will be equipped with an automatic electro-magnetic valve to maintain the vacuum in the cryostats in case a pumping machine fails. Each cryostat pipe will be equipped with its own isolation and over-pressure valves.

As it is not intended to pump the cryostats during observation time, the vacuum will be maintained by an ion pump. This solution is currently being evaluated (performance, sizing and costing). The final design relies on the outgassing and leakage rate that will be quantified using the cryostats of the DESI spectrograph prototype.

Vacuum maintenance is planned between the observation periods. The cryostats will be warmed up and pumped. The actual periodicity of such operations will be defined when the tests on EM#1 are completed.

5.4.3 Prototype Cryostat Measurements and Model Validation

A cryostat prototype (Figure 5.28) was constructed including all the elements previously described. We used the LPT9310 cryocooler and its CDE to test the cooldown and temperature regulation of a mechanical grade LBNL CCD under real experimental conditions (DESI-0327):

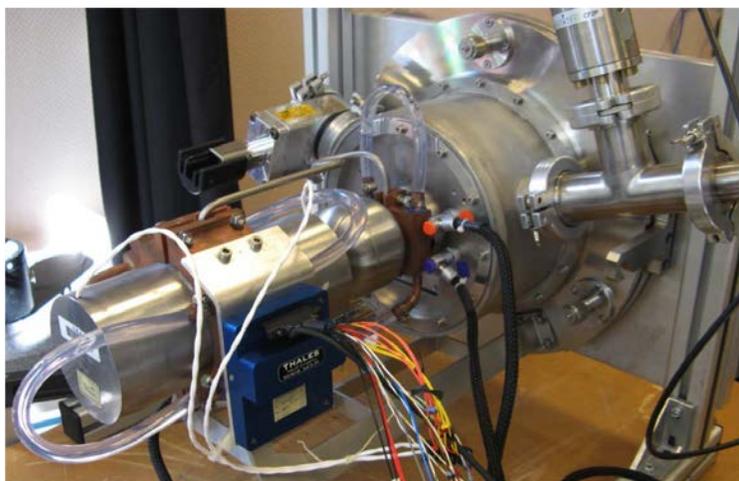


Figure 5.28: Saclay first cryostat prototype.

- Thermal losses were measured between 2.8 W and 3.2 W for the requested CCD temperatures (140–180 K), in good agreement with our estimate.
- LPT consumption was only 25–30% of its maximum allowed power (Figure 5.26).
- Temperature precision of the CCD was about 1 K.
- Temperature stability of the CCD was within 0.2 K peak to peak.
- Cool down temperature rate was 1.5 K/min and could be adapted if needed.
- cool down and temperature stability was reached in about 2.5 hours.
- Vibration amplitude was less than 3 μm (the instrument precision) at the detector in the directions parallel and perpendicular to the optical axis.

These show that we can easily reach all the requirements (CCD temperatures between 140–180 K, acceptable level of vibration, CCD temperature stability).

When extrapolating to 30 LPTs, the level of vibrations could be a concern. But, as each LPT is independently AC-powered by its own XPCDE and all XPCDE units are DC-powered, the vibrations of the 30 LPTs should not add in phase. We do not expect a higher vibration amplitude when operating with 30 LPTs, but this is carried as a risk. It is important to avoid mechanical resonance of the structure supporting the spectrographs.

5.4.4 Cryostat Control System

The control system will drive and maintain all 30 CCDs and cryostats at nominal operating conditions. A well-tested solution from prior projects has been adopted (MegaCam, Visir/VLT, LHC Atlas and CMS). The main components of the control system (Figure 5.29) are:

- Main unit MicroBox which integrate a Programmable Logic Controller (PLC) and a PC.
- Multi-channel RS232 Bus link interface to communicate with the XPCDEs of each cryocooler.
- Common group of Input/Output units to monitor the main parameters as pumping System, Chiller, vacuum distribution (pressure and valves).
- Several (x10) groups of I/O analog and digital units for cryostats parameter. So, each group is associated to 3 cryostats of one spectrograph.

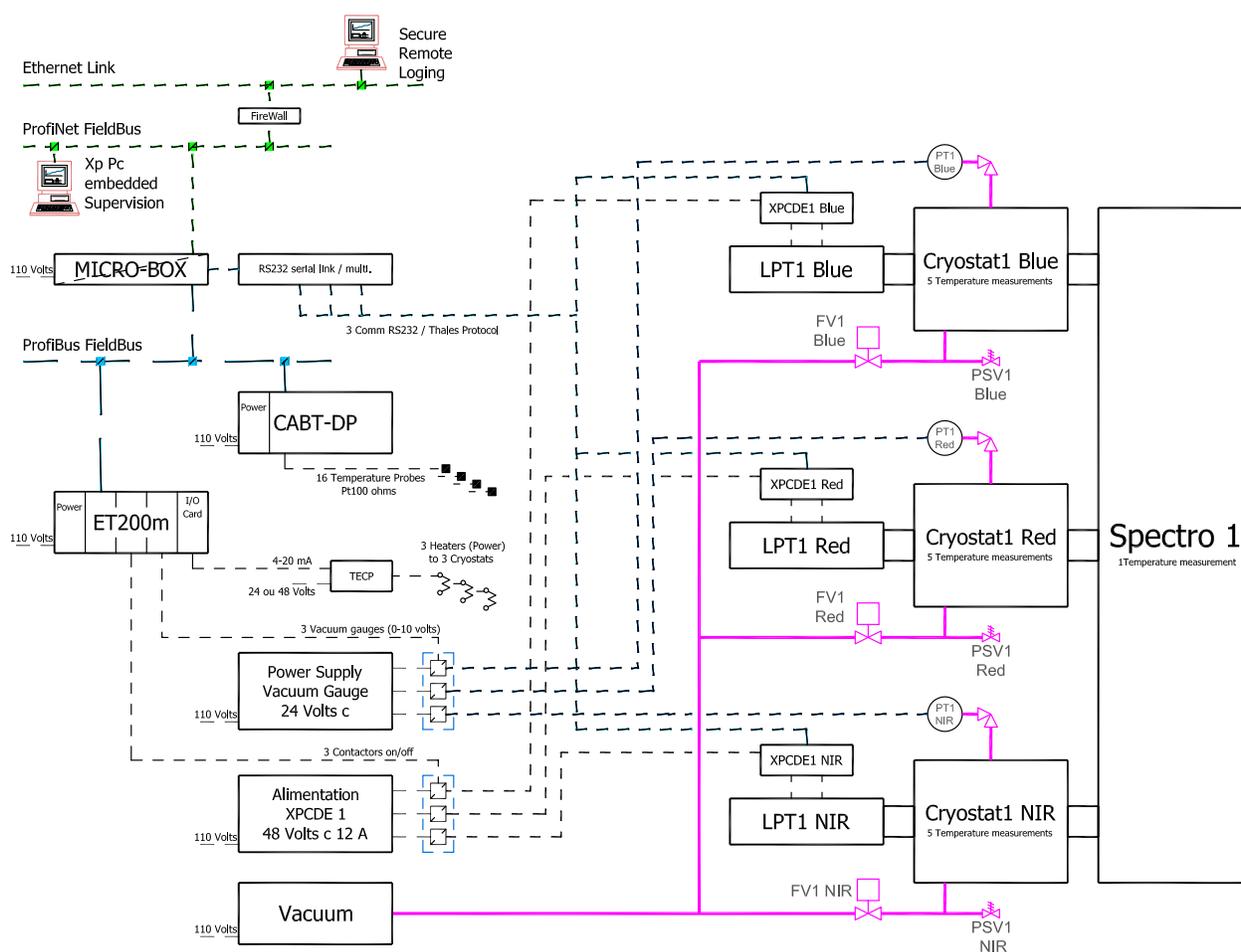


Figure 5.29: Architecture of the DESI cryostat Control System.

- OPC server for the communication with the Instruments Control System. It allows the ICS to download the Slow Control database which contains all analog values or parameter's states of the cryostats. It also transmits all commands from the ICS to the Slow Control.
- Supervisory unit, ported on an external PC to ensure safe functioning. It allows to display the state of the cryostat system in a graphical mode. It also allows to control all the elements in an SuperUser mode for maintenance operations or in case of failure.

The whole system is overseen by a Java module over Ethernet link. The general architecture of the system is based on the solution developed, implemented and tested on the Saclay prototype cryostat

The PLC is a Siemens Simatic S7-300 with a system core based on a UC319 mainframe. The program implemented in the PLC acquires in real time all variables corresponding to the monitoring and control of the instrument (vacuum and temperature monitoring), the control of the cold production unit (CCD cooling down and warming up), and the safety procedures on cryogenics, vacuum and electrical power. A local network (based on an industrial bus, e.g., ProfiBus or ProfiNet) ensures communication with the remote plug-in I/O modules and with the PLC.

Temperature measurements are provided by the Pt100 temperature probes connected to temperature modules acquired by the PLC. The other analog sensors (heaters, vacuum gauges) are connected on a 4–20 mA or 0–10 V module. All measurement modules will be located in two

Table 5.7: Electrical power consumption of the Cryostat System.

Unit Label	Description	Total max. Power consumption (kW)	UPS	Comments
Vacuum System				
turbomolecular group	2 units of 300 L/S speed pump	3.0	Yes/No ?	running during LPT cooling procedures and vacuum maintenance procedures
Ionic Pump	30 units of 3L/S	0.6	Yes	
vacuum gauges	30 units	0.1	Yes	
Vacuum electro-valves	3 units	0.1	Yes/No ?	
LPT Cryocoolers				
LPT power supply	30 units of DC 48V	6.0	Yes	during cooldown procedure, otherwise 2 kW in operation
Security/remote LPT	30 channels DC 5V	0.1	Yes	
Slow Control				
NICE PC	1 unit	0.1	Yes/No ?	Supervision PC
MicroBox Controller	1 unit	0.1	Yes	embedded PC and PLC
Communication interfaces and switches	2 modules	0.2	Yes	rs232, Ethernet communication
CABTF	10 units	0.2	Yes	temperature sensors acquisition 10x (16channels)
PLC I/O modules	1 unit of 6 modules	0.2	Yes	6x (16 channels)
PLC Analog modules	1 unit of 6 modules	0.2	Yes	6x (16 channels)
24Vdc power supply	1 unit	0.1	Yes	generic for I/O modules
5Vdc power supply	1 unit	0.3	Yes	generic for Analog modules
Total Power w/ 30% safety factor		11.3 14.7	8.1 10.5	

cabinets.

Supervision software with user interface is implemented in a NISE industrial PC connected to the PLC. It ensures the control of the cryocoolers, of the vacuum system and the monitoring/recording of all variables, with possibly different levels of user access rights. This access will be available to the Instrument Control System via an OPC server (OPC-UA communication Protocol). This system will also allow the set-up to be remotely controlled via the Ethernet network that will be accessible from the internet through a secured interface.

The total Electrical consumption for the cryostat system is estimated to be about 11 kW during cool-down. It is reduced to about 4 kW in nominal operation conditions, assuming the LPTs are at 30% of the maximal power and the pumping station is off (vacuum stationary state in cryostat during Science Observations). See details in Table 5.7.

5.4.5 Cryostats Integration and Tests

The cryostat integration requires dedicated tools that will be built in Saclay. In addition some elements will be provided by other members of the project:

- one special flat FLA to seal any cryostat during the test phase. This allows the CCD position to be optically controlled. The FLA will be provided by the spectrograph vendor.
- one CCD per cryostat and one front-end electronics unit (with software) to allow us to perform functional tests of the CCDs once integrated and cooled.
- one final spectrograph FLA per cryostat – provided by the spectrograph vendor – to close the cryostats before shipping.

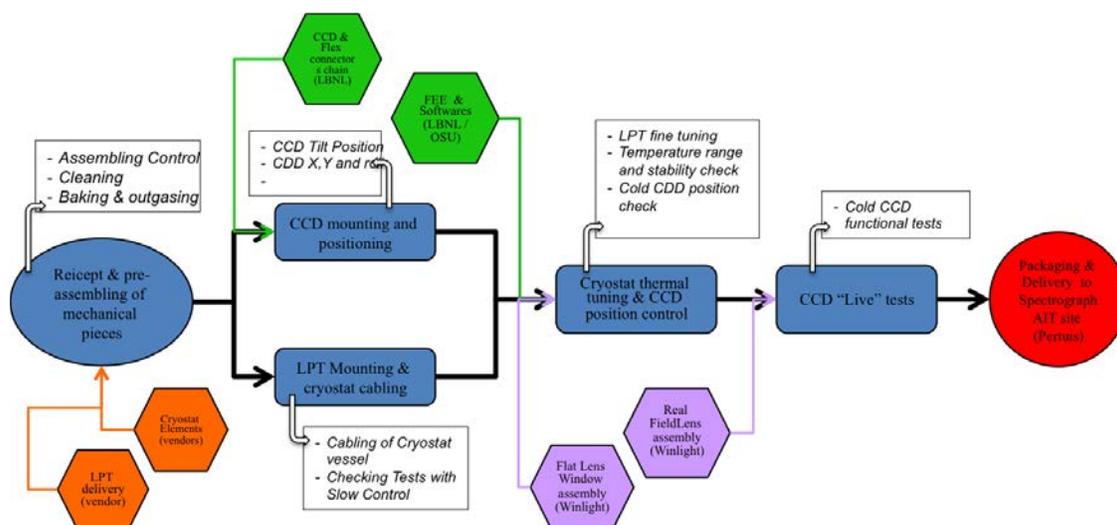


Figure 5.30: Cryostat integration Flow.

The cryostat integration procedures and tests are composed of 5 steps, as shown in Figure 5.30:

1. assembling control and cleaning-baking-outgasing operations of the mechanical elements of the cryostats.
2. CCD mounting and position tuning
3. LPT mounting and cabling/integration of all the sensors – Check of vacuum leakages – Tests with the Slow Control.
4. CCD integration in Cryostat - Fine tuning of cryocooler regulation with CCD
5. functional tests of the CCD once closed with final FLA unit

The mechanical elements of the cryostat, including sensors and cryocooler, will be assembled and closed in a class 10000 clean room. The control system will then be connected to check data acquisition, vacuum stability and Security processes. The CCD will be integrated in a class 100 clean room. Its 3D position w.r.t the reference frame defined in the spectrograph interface control document (Figure 5.23) will be measured by optical metrology. A specific 3 stages (XY θ) tool supporting the front flange, CCD cold plate, and CCD assembly will allow the precise positioning of the CCD to be achieved (Figure 5.31).

The cryostat will be closed with a “flat lens” FLA. This FLA will allow us to control the CCD position in the cryostat at low temperatures and for any orientation of the cryostat. After all tests are completed, the flat lens FLA will be replaced by the spectrograph FLA and the fully integrated cryostat will be packaged and shipped. .

5.5 Sensors and Electronics

The ten DESI spectrographs each require three CCDs for the blue, red, and NIR channels. Each CCD is housed in its own cryostat, each in turn with its own refrigerator and CCD control electronics.

5.5.1 CCDs

Each of the three channels of a spectrograph will use a 4k \times 4k CCD with 15 μ m pixels. The CCD specifications are defined in DESI-0071. The subset of performance specifications are given

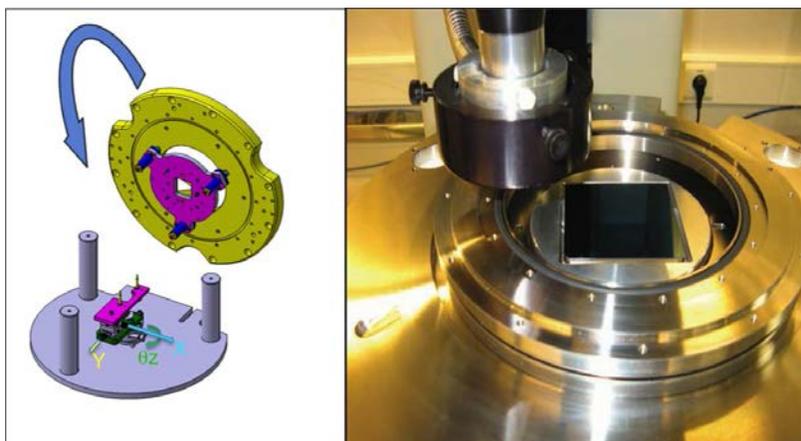


Figure 5.31: Left: 3 axes stage tool for precise positioning of the CCD. Right: optical machine used for CCD position measurements in the Saclay class 100 clean room.

in Table 5.8. There are also specifications for the mechanical and electrical interfaces that are not presented here. For the blue arm we baseline the ITL STA4150A provided by University of Arizona Imaging Technologies Lab. For the red and NIR channels we baseline the LBNL $4k \times 4k$, $250 \mu\text{m}$ thick CCD to optimize quantum efficiency. The CCD format is the same as for BOSS, but has a lower read noise output.

Both CCDs are known to meet the dark current, diffusion, and cosmetics requirements. The QE requirements are within measured values. For readnoise, Semiconductor Technology Associates report $< 2.9 e$ at 100 kilopixel/sec with $3.2 e$ achieved to date by ITL. For the LBNL CCDs, lab measurements find a read noise of $1.8 e$ at 100 kilopixel/sec.

Figure 5.32 shows the existing packaging for LBNL CCDs and a packaging concept from ITL that is compatible with DESI cryostats. The production of the LBNL CCDs will follow the DECam model where LBNL will produce and cold probe unpackaged CCD die that will in turn be packaged and characterized at FNAL. FNAL has packaged seven devices to date using various quality die. ITL CCDs will be provided as packaged and tested devices.

The quantum efficiency performance of both CCDs is well established. The red curve in Figure 5.33 shows measured QE for an LBNL CCD with a broadband antireflection coating. The high-side cutoff is determined by the CCD thickness. We note that the QE in the red band for

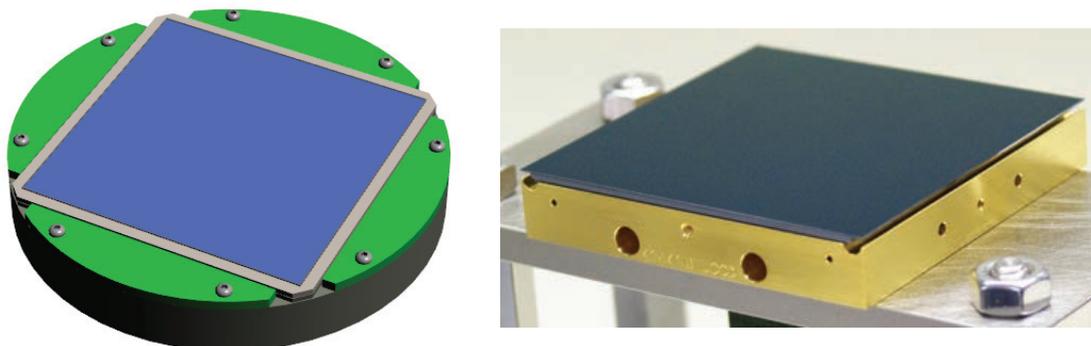


Figure 5.32: $4k \times 4k$, $15 \mu\text{m}$ CCD packaging: ITL concept for STA 4150A and LBNL $4k \times 4k$, left to right.

Table 5.8: CCD performance specifications.

Item	Specification
Format	
Pixel size	15 μm
Pixel count	$\geq (4096 \times 4096)$
Readout channels	4
Dark current	
Readnoise at 100 kpixel/sec	$< 3 \text{ e}$
Full well (3% linearity deviation)	$> 75,000 \text{ e-}$
Non-Linearity (from 200 e- to 75% full well)	$< 1\%$
Charge transfer efficiency	
Parallel	> 0.99999
Serial	> 0.99999
Quantum efficiency	
360–400 nm	$> 75\%$
400–600 nm	$> 90\%$
600–900 nm	$> 90\%$
900–980 nm	$> 60\%$
Lateral diffusion (rms at surface)	
	$< 5 \mu\text{m}$
Cosmetics	
Column defects - black or white	$< 10 \text{ max}$
White spots	$< 800 \text{ max}$
Total (black & white) spots	$< 1500 \text{ max}$
Traps $> 200 \text{ e-}$	$< 15 \text{ max}$
Flatness	
Blue channel	$< 20 \mu\text{m P-P}$
Red and NIR channel	$< 15 \mu\text{m P-P}$
Corner pixels location knowledge	$\pm 50 \mu\text{m}$

the CCD only meets the requirement on average at the moment. Figure 5.33 shows measured AR coating data from ITL (blue curve).

5.5.2 LBNL CCD Packaging

The LBNL CCDs will be packaged at FNAL using the packaging technique developed by LBNL. An exploded view of the package for the $4\text{k} \times 4\text{k}$ DESI sensors is shown in Figure 5.34. The detector is attached to a Si substrate with Epotek adhesive. The Si substrate is attached to the custom readout flex circuit, which brings the signals to a 64-pin connector. The flex circuit is wire-bonded to the CCD. Finally an Invar pedestal foot is attached to the substrate to provide mechanical support for the detector.

The most critical step to produce a flat sensor is attaching the sensor to the Si substrate. The $80 \mu\text{m}$ gap between the sensor and the substrate needs to be precisely controlled. This is achieved with an optical system permanently mounted on the packaging fixture. This step is shown in Figure 5.34.

Seven mechanical and engineering grade detectors have been assembled using this fixture at FNAL. Room temperature and cryo flatness measurements have been performed. An example is shown in Figure 5.35 where the maximum deviation from a flat surface is $6 \mu\text{m}$, this is acceptable

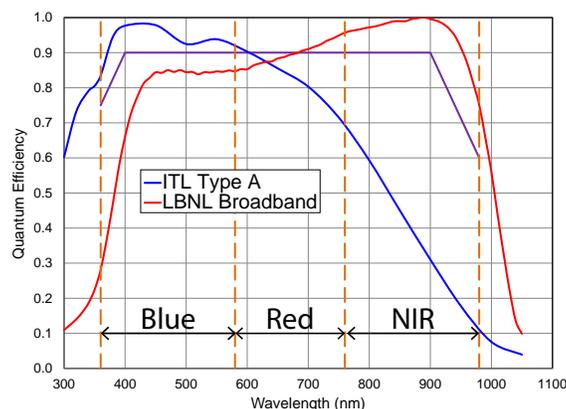


Figure 5.33: Quantum efficiency for DESI : ITL STA5140A and 250 μm thick LBNL CCDs. Data are lab measurements. The purple line is the CCD specification. The vertical orange dashed lines are the locations of the band transitions for the three spectrograph channels.

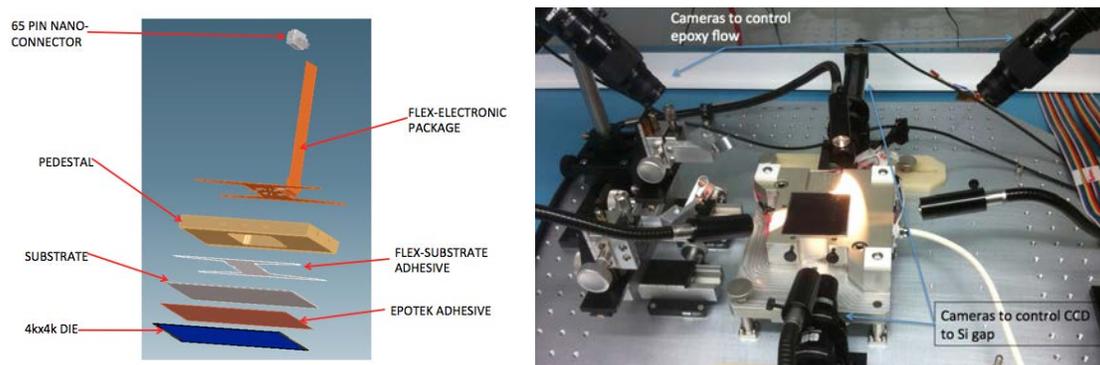


Figure 5.34: Left: Blowup of CCD package for the DESI 4kx4k LBNL CCDs. Right: CCD packaging fixture showing four digital cameras to control the process. Two are used to measure the gap between the CCD and the substrate, which can be adjusted with micrometers (not shown in the image). The other two cameras are used to monitor the flow of epoxy during the gluing process. The fixture holding the substrate is not shown in this image.

for the instrument but is still under study for improvement.

Given the two gluing steps on this process, four working days are required to complete a package. Taking this into consideration we estimate a packaging production rate of one CCD per week.

5.5.3 CCD Characterization

Each LBNL detector packaged at FNAL will be tested against the technical requirements for the instrument. The detectors passing the requirements will be fully characterized in the CCD testing laboratory at FNAL. This facility was developed during the construction of DECam [19]. The characterization will include: noise measurements, linearity measurements for the complete dynamic range of the instrument, QE measurements in the range between 360 nm and 1000 nm, and dark current. The CCDs will be exposed to x-rays to characterize the diffusion of the detector and charge transfer efficiency. The characterization will also include scanning clock and bias voltages around the nominal operating parameters.

The baseline plan includes having two dedicated test stations for DESI detectors at FNAL.

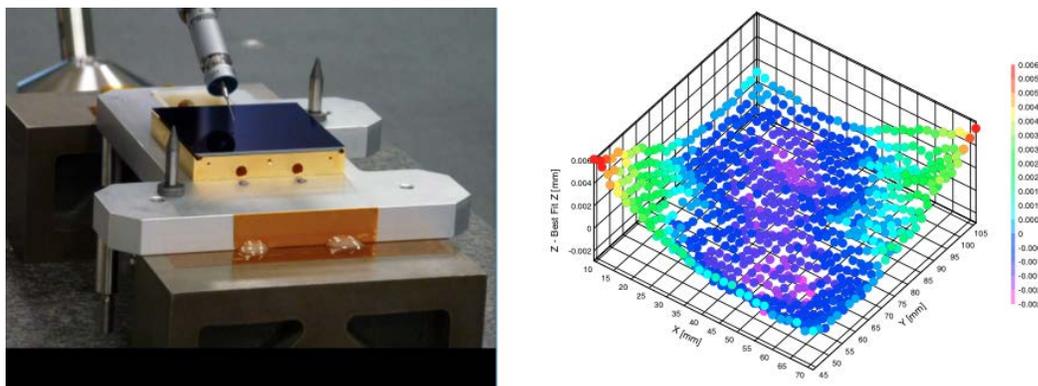


Figure 5.35: Left: CMM touch probe measurements of the package flatness for a completed mechanical grade device. Right: Deviations from the best fit plane on the mechanical grade device.

Test Station 1 (TS1) will be on an optical bench with a stabilized illumination source, coupled to a monochromator with a wavelength range of 360 nm to 1000 nm. TS1 can operate with a stable temperature from room temperature to 145K. This test station is shown in Figure 5.36 left.

Test Station 2 (TS2) shown in Figure 5.36 right will be used to measure the flatness of detectors at the operating temperature of 145K. This measurement will be done using a confocal lamp focusing light on the cold CCD surface, and capable of determining the reflecting plane with a precision of $1 \mu\text{m}$. This light source is mounted on a precision X-Y stage to produce a topological map of the detector. This technique was successfully used by the FNAL team for flatness measurements in the DECam focal plane [20].

The testing cycle for each DESI detector will be about one week long divided in three stages. Each detector will be installed in TS1 for the initial check against technical requirements. This initial test stage (Stage-1) will last about 1 day. After a detector passes Stage-1 testing, a full characterization consisting of 2 days of data collection will be performed also using TS1, Stage-2. Stage-3 testing consists of flatness measurements. For this purpose, the detector will be moved into TS2 for flatness measurements. These measurements are about 1 day long. Detectors completing Stage-1, Stage-2 and Stage-3 testing will be ready for installation in the cryostats.



Figure 5.36: Left: Test Station 1 (TS1). The illumination source consists of a power regulated broad-band lamp, automated monochromator and filter wheel, shutter and integration sphere. An x-ray source is located inside the vacuum vessel. Right: Test Station 2 (TS2). TS2 with a mechanical grade 4k x 4k DESI CCD mounted inside the vacuum vessel. The optical window has been removed to show the sensor inside. The front of the image shows the confocal light source.

Automated software will control the testing of the detectors, in a manner similar to what was done for DECam CCDs. The CCD testing facility at FNAL has four additional test stations with different capabilities typically used for other projects. The additional infrastructure could be made available to the project if the schedule for DESI demands a higher rate of testing, or new testing needs develop during the fabrication process.

5.5.4 Electronics

The electronics module for each CCD is mounted on the warm side of the cryostat wall. This provides easy access for replacement without disturbing the detector or spectrograph. The LBNL-developed modules include local power generation from an isolated single DC voltage, CCD bias voltages generation, programmable clock levels and pattern, CCD signal processing and digitization, and operating settings readback. The module runs Linux supporting a suite of remotely callable routines for normal and special CCD operations. Configuration and control of the electronics and delivery of science data is over Ethernet. A block diagram is shown in Figure 5.37.

A level of complexity is introduced into this electronics because of the mixture of n-channel (ITL) and p-channel (LBNL) CCDs. The CCD output structures required opposite sign DC biasing voltages and the electron-to-voltage gains are of opposite sign. The controller uses the same regulators and drive circuits for these with different power rail strapping. Common clocking circuitry can work for both. In addition, the LBNL devices require a high voltage depletion supply.

LBNL has developed a generic four-channel CCD readout controller that supports both flavors of CCD. The analog signal processing and digitization is accomplished with an oversampling 100 MHz 16-bit ADC. Summation (and potentially more sophisticated algorithms) and correlated double sampling are done in an FPGA. Images are transmitted as FITS files to the Instrument Control System. The production-ready hardware is shown in Figure 5.37.

Several LBNL CCDs have been operated with system. It has shown equal or better readnoise performance than a commercial dual-slope integrator controller from 50–300 kpixel/s. At 100 kilopixel/sec, 1.8 e for the LBNL CCD has been attained. Configured for ITL CCDs, the controller has successfully operated an ITL-provided STA510A 800×1200 small CCD, achieving the readnoise reported by ITL for the device.

5.6 Calibration System

Multiple calibration sources will be used in DESI, including sky lines, stars, continuum and line (arc) lamps, and a CCD flat field illuminator. Since the DESI spectrographs are mounted on stationary optical benches in a temperature controlled environment, their calibration should remain quite stable. Continuum and line lamps will be used daily to monitor this stability and establish a baseline PSF and fiber-to-fiber relative throughput. Sky lines present in each fiber can be used to track stability from exposure to exposure. Additionally, within each exposure, fibers assigned to blank sky locations will be used for measuring the sky spectrum to subtract from object fibers, and fibers assigned to standard stars will enable an approximate spectrophotometric flux calibration. The CCD flat field illuminator is internal to the spectrograph. Presently it is anticipated that this will be used once a year since it entails removal of the fiber slitheads.

5.6.1 Lamps

Calibration lamps are used to illuminate the pupil of the telescope. They can be broad band or emission line lamps. They require warm up and stabilization time that is significant compared to a science exposure time. As such, these will be used during the day to establish a baseline

Table 5.9: Some potential arc lamp sources.

Element	Line range (\AA)
Hg–Cd	1570 – 5790
Ar	7503 – 9784
Ne	5330 – 9665
Fe	8571 – 9802

calibration, but they will not be used throughout the night. They will be mounted on the telescope and illuminate a flat field screen mounted inside the Mayall dome. Alternatively, if calibrations need to be taken at specific telescope positions, they could illuminate the back of the closed petals which cover the primary mirror.

Continuum lamps (e.g., quartz iodine halogen) provide a mostly smooth spectrum that evenly illuminates all fibers. These are used to measure the xy trace location of the spectra on the CCDs and to correct for *relative* fiber-to-fiber throughput variations.

Arc discharge lamps provide spectra with sharp lines at known wavelengths. Combining a variety of gases (options listed in Table 5.9) enables complete coverage of the DESI wavelength range. These lines are used to establish the wavelength solution and to measure the point-spread-function (PSF) shape of the spectrographs. The wavelength solution and PSF shape are fit to a functional form between the available arc lines.

5.6.2 Sky Lines

All spectra of all science exposures will unavoidably have multiple sky lines. Fibers assigned to blank sky locations distributed throughout the focal plane will be used to measure the sky on an exposure-by-exposure basis. Each observation guarantees 40 sky spectra per spectrograph per exposure. These are used for the detailed wavelength calibration and modeling of the sky spectra to subtract from the science target spectra.



Figure 5.37: CCD frontend electronics module components supporting both n- and p-channel CCDs. Boards clockwise from top right are: backplane with Xilinx FPGA card, network connectors, and connector to the CCD (on the backside); controller power supplies; clock-level drivers and substrate HV voltage generator; and CCD DC bias voltages generators, preamps, and 4-channel ADC.

Since the sky lines are resolved and have known wavelengths, they will be used to monitor the stability of the spectrographs (Section 7.2.3).

5.6.3 Stars

Standard stars will be selected as main-sequence F-stars based upon color and magnitude cuts, with the detailed selection dependent upon the available targeting datasets. These stars have well understood and mostly smooth continua that may be modeled using stellar templates with temperature and surface gravity as tunable parameters. By comparing the observed standard star spectra with their modeled spectra and photometry (from the targeting data), a spectrophotometric solution is derived. This solution is modeled across the focal plane to provide spectrophotometric calibration to the spectra. This spectrophotometric solution describes the calibration of counts on the detector to flux on the sky, which includes the instrument throughput and atmospheric absorption bands.

5.6.4 CCD Flat Field Illuminator

CCD pixel-level response will be measured using a flat field illuminator as described in Section 5.2. This mechanism evenly illuminates the CCD in the spatial direction with a smooth spectrum such that each pixel receives the same wavelength of light as it would from a science spectrum. By comparing each pixel to the median of other pixels with the same wavelength, a wavelength-dependent pixel level response is measured. This is used by the raw data pre-processing to make pixel-level response corrections. BOSS employs a similar mechanism to calibrate its spectrograph CCDs, taking measurements approximately once per year or after any operation which breaks the CCD dewar vacuum. DESI also plans yearly CCD flat field calibrations since the illuminator mechanism requires removing the slit heads.

6 Instrument Readout and Control System

The design of the DESI online system is based on the readout and control system architecture our team developed for the Dark Energy Camera [21]. This system was deployed on Cerro Tololo in 2012, and has been used successfully for both the DES survey and the community observing program. A detailed description of the DECam data acquisition system can be found in [22] and [23]. Important components of the DESI online system such as the dynamic exposure time calculator, the real-time data quality assessment and complex algorithms to convert on-sky target coordinates to fiber positions on the focal plane are based on the SDSS-III/BOSS online system. The DESI instrument control system (ICS) is tasked to perform all control and monitor functions required to enable successful operation of the DESI instrument and completion of the DESI science program. The requirements for ICS are:

- Performance and Design
 - In order to ensure maximum survey efficiency the ICS shall complete all activities between exposures on average in less than 120 seconds. A design goal shall be to achieve this in 60 seconds. A lower limit is set by the CCD readout time of 42 seconds.
 - The ICS shall be robust and modular in the sense that the system shall meet operating requirements subject to total failure of any single computer or disk drive. Dedicated hardware interfaces are excluded from this requirement.
 - The ICS hardware and software shall be designed so that system up-times of greater than 97% can be achieved no later than the end of the first year of the survey.
 - The ICS architecture shall support small-scale test systems and sub-component integration tasks.
- Monitor
 - The ICS shall continuously monitor the operational parameters of the DESI instrument. The values of these parameters and other telemetry information shall be archived in a database for offline analysis.
 - The ICS shall provide both a web-based and a programmatic interface to the telemetry database.
 - The ICS shall provide a connection to the existing Mayall monitor systems to collect and archive environmental information.
 - The ICS shall provide an alarm and error notification system. All alarm and error messages generated by the instrument shall be archived.
 - The ICS shall not be responsible for the hardware protection of DESI components.
- Control
 - The ICS shall provide all user interfaces required by the observer to operate the instrument. Secure remote access shall be supported.
 - The ICS shall interface with the Mayall telescope control system to automatically position the telescope to ensure high survey efficiency.
 - The ICS shall provide sufficiently fast and reliable communication paths between DESI sub-components. This includes the connection between the guider (GFA) and the telescope control system and between the alignment system (GFA) and the hexapod.
 - The ICS shall include a dynamic exposure time calculator.

- The ICS shall provide the process to map the target coordinates received in RA/DEC format from data systems to focal plane coordinates that can be loaded into the fiber positioner.
- Data Flow
 - The ICS shall provide sufficient network bandwidth to retrieve the data from the front-end electronics without causing any additional deadtime and without extending the time between exposures.
 - The ICS shall format the data in multi-extension FITS format with a set of DESI specific header keywords. The images will be compressed with the Rice/tile algorithm before they are transferred off of the mountain.
- Online Hardware
 - The ICS project shall be responsible for all DESI computer hardware at the Mayall. This shall include the online computers, disk storage, the internal network hardware and two multi-display workstations for the Mayall console room.
 - The ICS shall provide sufficient storage capacity to continue to operate DESI for at least three nights should the data transfer links off the mountain fail.

The design of the DESI online system is based on these requirements. The overall architecture is shown schematically in Figure 6.1. At the core of the system sits the observation control system (OCS) that orchestrates the complex DESI exposure sequence. It interacts closely with the focal plane systems including the fiber positioner, the fiber view camera, and the guider, focus and

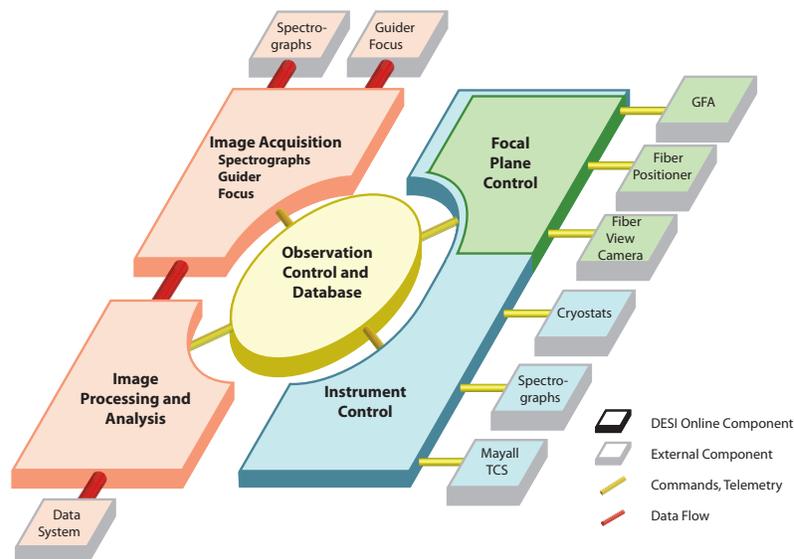


Figure 6.1: Schematic view of the DESI readout and control system. The observer console and other user interfaces are not shown.

alignment system. Data is acquired from the guider and the front end electronics in the spectrographs and flows through the image processing stage to a storage device from where the images are picked up by the DESI Data Systems group. The connection to the Mayall telescope control system (TCS) and the Mayall telemetry database is provided by the TCS Interface component also shown in Figure 6.1. The readout system is tightly integrated with the DESI instrument monitoring and control system (IMCS). The IMCS monitors every component of the instrument and detailed information about instrument status, operating conditions and performance will be archived in the DESI operations database. The final component of the DESI online system (not shown) is a set of web-based user interfaces that includes the observer console.

Our detailed description of the DESI readout and control system begins in the next section with a discussion of the OCS followed by a review of the DESI exposure sequence and the activities that need to be coordinated by the online system between exposures. The dataflow architecture, the operations database, the interface to the Mayall telescope, and the instrument control and monitoring system are covered in the next sections. We conclude with a discussion of the online software we are developing for DESI.

6.1 Observation Control

The OCS is the central component of the DESI readout system coordinating all aspects of the observation sequence. We have adopted a multi-threaded, pipelined architecture to maximize throughput. Exposure requests are handled by the OCS QueueManager and the Next-Field-Selector script that will be developed by the Data Systems group. The format for exposure requests has been defined (DESI-0560) and includes the 5,000 fiber coordinates, the pointing coordinates for the telescope, a list of guide stars, an expected exposure time and some book keeping information. The QueueManager can handle multiple requests, supports exposure scripts and provides a number of functions to manage the exposure request queue. The Exposure Sequencer is at the core of the OCS. It receives exposure requests from the QueueManager and orchestrates the complex DESI exposure sequence as described in the following section. At the end of an exposure the OCS will initiate readout, digitization and image processing including quality assessment. Once the exposure has been written to a disk cache, the OCS notifies the data transfer system developed [24] by the Data Systems group that image data are available to be transferred to the NOAO archive and the DESI processing site(s).

In addition, the OCS maintains the overall status of the DESI instrument and the online system. Software interlocks are used to monitor the readiness of the components that participate in the exposure sequence. An exposure can only be started when all required interlocks are set. When an interlock breaks or another error condition is detected, an alarm is issued to alert the observer.

6.2 Exposure Sequence

A typical DESI exposure sequence is shown in Figure 6.2. The observation control system (OCS) is responsible for coordinating the different activities. In order to maximize survey throughput we will employ a pipelined architecture and set up for the next exposure while the previous image is being digitized and read out.

When the Dynamic Exposure Timer described in Section 6.2.4 informs the OCS that the accumulation period of an exposure has ended, the OCS signals the spectrographs to close the shutters and instructs the frontend electronics to read out the CCDs.

Information about the next pointing, target coordinates and guide star data has already been received from the Next-Field-Selector during the previous accumulation phase. Once the spectro-

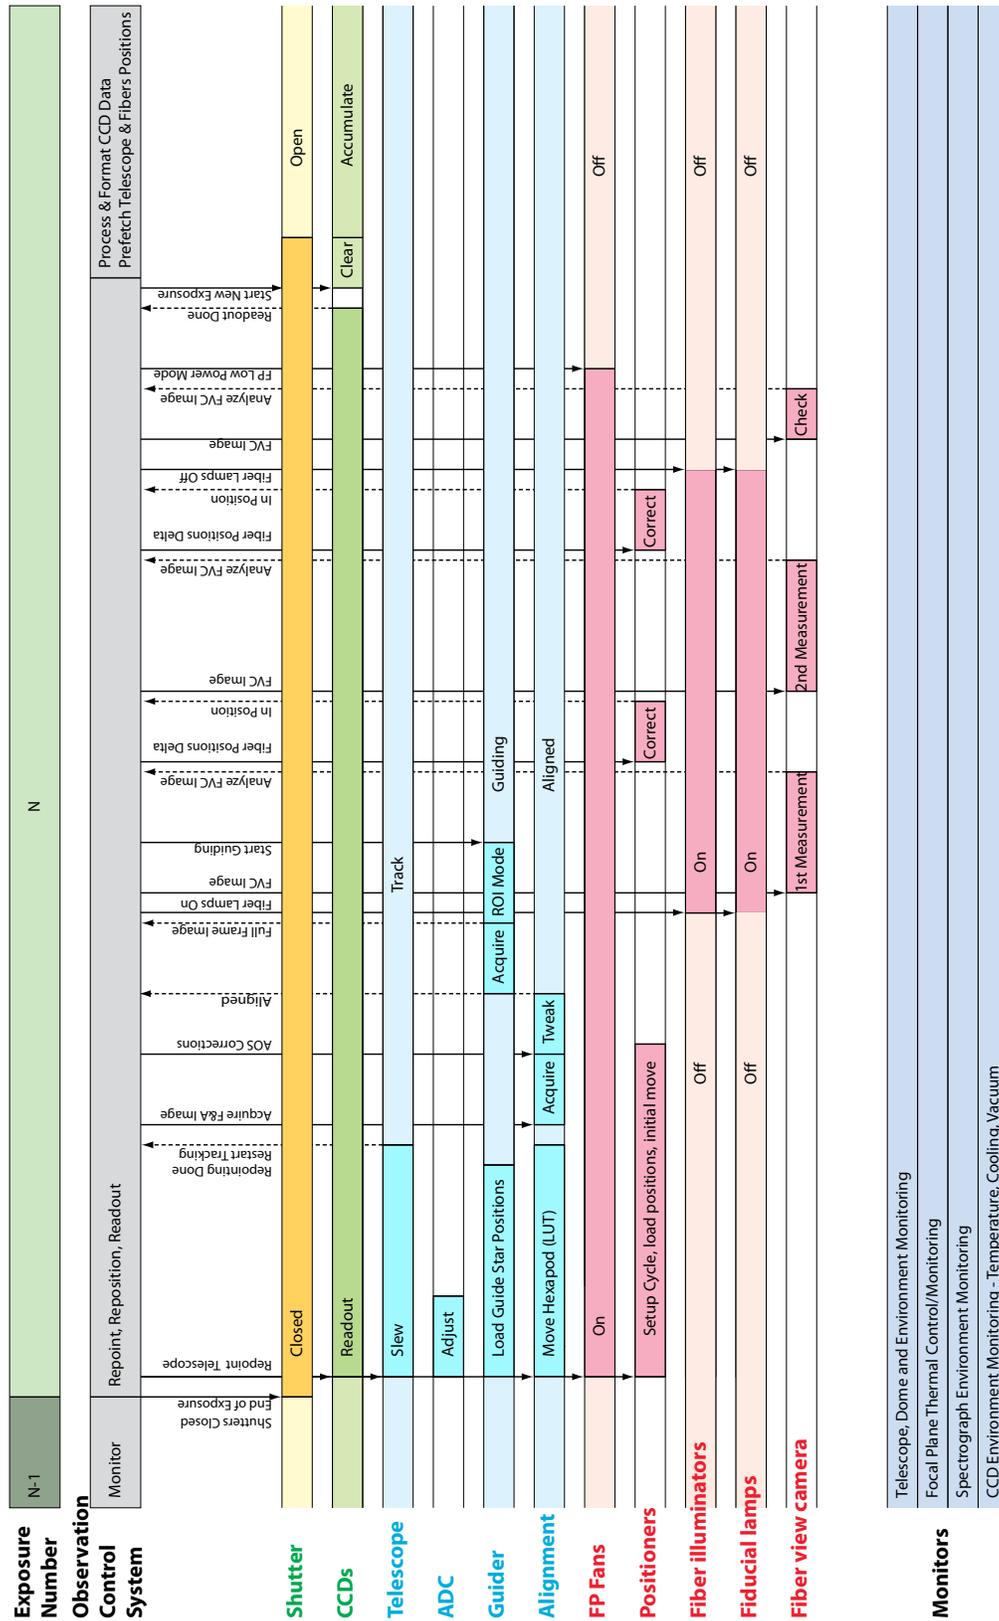


Figure 6.2: A typical DESI exposure sequence timeline. Lengths of the bars do not represent activity durations.

graph shutters are closed, the OCS transmits the coordinates of the new field to the telescope. DESI uses a hexapod to control focus and alignment of the instrument. While the telescope slews to the new position, a lookup table is used to retrieve base values for all six hexapod parameters. These are combined with accumulated correction signals obtained by the active optics component of the GFA and sent to the hexapod to initiate the adjustment. The ADC is instructed to update for the new telescope pointing. The focal plane fans are turned on. The PlateMaker application (see Section 6.2.2) uses an optical model of the DESI corrector and corrections based on the previous exposure to convert the 5000 on-sky target coordinates to focal plane coordinates. These initial coordinates are sent to the fiber positioner to perform the initial move to the new configuration.

Once the telescope and the hexapod are in position, the four focus and alignment cameras of the GFA system take a full-frame exposure. The out-of-focus star images (donuts) are analyzed to determine the wavefront and small adjustments are sent to the hexapod (“tweaks”) to complete telescope and focal plane alignment.

With the alignment complete, full-frame exposures are taken by the six guide cameras of the GFA system. Using the astrometric solution derived from these images, the PlateMaker determines the offset between actual and requested telescope position. If a large offset is detected, a move command is sent to the Mayall telescope control system to correct the pointing and another set of full frame exposures is taken. This sequence is repeated until the telescope pointing is within 20 arcsec of the requested position. At this point in the exposure sequence, the guide CCDs are switched from full-frame to region-of-interest mode and the telescope tracking feedback loop is closed. Via the guide corrections the telescope position is tweaked to correct the residual offset and to match the desired target location. During an exposure, guider correction signals are sent at a rate of about 1 Hz which is well matched to the characteristics of the Mayall TCS.

The PlateMaker refines the mapping of target coordinates to focal plane coordinates using telemetry information from the ICS and astrometry information obtained from the final set of full frame guide camera exposures. When the fiber positioner signals completion of the initial move, the fiducial and fiber illuminators will be turned on and the fiber view camera acquires a first snapshot of actual fiber locations. The Fiber Positioner Control System, another component of the OCS, receives the updated target coordinates in the focal plane system from the PlateMaker, determines the corrections for each actuator and sends the new coordinates to the positioner system. One or two additional cycles will be required to complete the positioner setup. The maximum number of iterations is bound by the requirement to keep the time between exposures below 120 s (60 s). At the end of the fiber positioning cycles, the focal plane fans as well as the fiber and fiducial illuminators are switched off. The fiber view camera takes a last image to verify that all light sources are off before the next exposure begins.

Concurrent with these operations the OCS waits for CCD readout complete messages from all spectrograph cameras. With the readout complete and the fibers, telescope, hexapod and ADC in position the OCS sends an open command to the shutters and the next accumulation phase begins. While the spectra are being acquired information about the next exposure, including telescope coordinates and target positions, is loaded into the OCS, and the cycle repeats.

The DESI DAQ system is designed to complete the entire sequence outlined above of activities between exposures in less than 120 seconds with a goal to accomplish these tasks in as little as 60 seconds.

Several of the key components that participate in the exposure sequence are discussed in following sections.

6.2.1 Active Optics System

The Active Optics System (AOS) will adjust focus and alignment of the DESI corrector using out-of-focus stars in the four F&A cameras of the GFA system. Each of these four cameras will contain a 30 mm by 15 mm CCD, arranged so that half of the sensor is intra-focal by 1.5 mm and half extra-focal by 1.5 mm. The resulting out-of-focus stars (donuts) are images of the exit pupil distorted by optical aberrations. The AOS will analyze an ensemble of donuts, with a forward fit of the images to a pupil-plane Zernike expansion. The measured aberrations are then used to infer deviations from optimal focus and alignment. The AOS will be based on the highly successful system developed for DECam [25, 26, 27], and will reuse almost all of the relevant online and offline code. The DECam AOS is operating highly reliably, unsupervised and in closed-loop for all five degrees of freedom (focus, hexapod x and y decenter, tip and tilt). Typical control of focus is maintained to better than 30 μm , decenter to 300 μm , and tip/tilt to 15 arcsec. These values are likely limited by the repeatability of the mechanical alignment between the primary mirror and prime-focus camera, or by time-varying distortions caused by in-dome seeing, but not by the measurement error of the AOS itself. As such, similar quality performance may be expected for DESI.

There are some differences between the AOS and the donuts for DESI compared to DES, and each will require some small changes to the existing code. First, the code which locates donuts in the GFA image, *dfdFinder*, has all hard-coded parameters and will need to be tuned for the GFA CCDs, to yield good donut finding efficiency. Next, the donut fitting code, *donutengine*, will need a detailed model of the DESI corrector's pupil function, accurately characterizing the vignetting for each of the four GFA cameras. The DESI pupil function is actually much simpler than the DES one, which must model the complicated inner obscuration. The non-linear fitting code, *donutfit*, and the donut analysis code, *donutana*, will be reused unmodified. The donut analysis code will however require the appropriate calibration data for DESI.

Several AOS calibration products will be required. First, a series of images must be taken, dithered in a region with appropriate stellar density, to produce a map of the aberrations across the GFA cameras. The DESI optical model predicts a significant change in astigmatism, coma and trefoil across the GFA cameras, and these variations must be characterized using measurements to account for differences between the as-built system and the idealized optical model. Second, the effect of focus and hexapod alignment on the astigmatism and coma must be measured, with images taken over a range of focal settings and hexapod decenters and tip/tilts. This data will be used to infer the 4x4 sensitivity matrix between astigmatism (or more accurately the focal plane slope of astigmatism) and coma and the hexapod decenter and tip/tilt. Once these calibrations are complete a look-up table of the typical focus and hexapod alignment across the sky may be built. Finally, a look-up table of the astigmatism of the Mayall 4-meter primary mirror can be constructed as well.

6.2.2 Plate Maker

The function of the PlateMaker application is to map the target coordinates received in RA/DEC format to focal plane coordinates that can be sent to the fiber positioner. This task must correct for mechanical and optical distortions using a combination of guider images, Fiber View Camera (FVC) images, and a set of fiducials at known location in the focal plane. Ancillary information from the ICS such as temperature, hexapod settings, and telescope pointing information are also needed.

The PlateMaker task has six modules, which function as follows:

1. Target positions: The target selection database will provide J2000 coordinates along with other information for 5000 targets and a list of stars that overlap the guider CCD fields; additionally, the field center, telescope coordinates, UTC, and focal plane temperature are provided. The PlateMaker receives this information via the Next-Field-Selector and the OCS. It is then used to apply precession, nutation, aberration, refraction, and polar axis misalignment to produce apparent coordinates for all objects relative to the apparent field center.

A nominal distortion pattern is applied to the target positions and sent to the fiber positioner for the initial positioning.

2. Guider images: Once the telescope has finished slewing and settled, and the ADC has rotated to the desired position, a set of guider exposures is obtained. These exposures are analyzed to identify stars, and the star instrumental coordinates (corrected for a nominal distortion pattern) are matched to the star lists from the target selection DB in order to determine the sky position, scale factor, and any residual position angle offset for each guider CCD. This information is combined with knowledge of the focal plane temperature in order to determine the absolute sky coordinates of each pair of fiducials attached to each GFA assembly.
3. FVC image: In parallel with obtaining the guider images and once the fiber positioners are at the nominal target location, an image is taken with the FVC of the back-illuminated target and fiducial fibers. The image is analyzed to produce x, y spot positions of each fiber. These spot positions are matched with a pattern-matching algorithm to identify which fiber corresponds to a particular spot.
4. FVC astrometric calibration: This small module takes the measured spot positions of the GFA fiducials and matches them with the absolute sky positions determined in step 2. These matches are used to determine an absolute astrometric calibration of the FVC focal plane. If the FVC camera lens and/or CCD introduce distortion, it is presumed that this distortion has been calibrated in the laboratory, since it cannot be determined at the telescope.
5. Distortion calculation: The spot positions of all the fiducials are matched to their known positions (adjusted for focal plane temperature) and used to determine coefficients for the distortion introduced by the DESI corrector and ADC. This mapping occurs from DESI focal plane to the FVC focal plane and the reverse.
6. Calculate fiber positions: At this point the apparent target positions are mapped to the FVC focal plane and matched to the appropriate spot position from the FVC image. Errors are calculated, and corrected positions are sent to the fiber positioner system.

The last few steps are iterated until all fibers are in position.

6.2.3 Guider

The DESI guider system provides correction signals to the Mayall telescope control system (TCS) to maintain a stable and accurate position during science exposures. It consists of six guide cameras described in detail in Section 3.4 and code for star finding and centroiding algorithms that we call the guider. The guider's task is to analyze the images taken by the GFA detectors, to determine the position of the guide star centroids and to derive corrections signals that are sent to the TCS. Tracking uncertainties have to be less than 0.03 arcsec.

A detailed study of the GFA cameras showed that signal-to-noise ratios better than 10 can be achieved with stars brighter than magnitude 17.5 in R band. Six of the ten DESI GFA modules are dedicated to guiding on up to 24 guide stars, as the electronics will allow to configure up to 4 region-of-interest (ROI) per detector. The actual number of guide stars used in an exposure will depend on the availability of enough high-S/N stars. Combining all guider sensors we expect to have an average of 11 stars that meet the target SNR even for the worst-case scenario near the galactic pole.

The DESI guider distinguishes two stages: the acquisition stage where guiding stars are selected and the tracking stage where guide stars are continuously monitored and corrections are sent to the telescope. Several different operating modes have been implemented. All share the same code for the tracking stage but employ different acquisition strategies. By default, the guider operates in catalog mode, where guide stars have been preselected from an external catalog. In self mode, the guider analyzes the entire full-frame GFA images, and automatically selects the best guide stars, based on signal-to-noise, isolation, saturation, and location with respect to the chip boundaries, whereas in manual mode, the observer will be able to manually select the stars detected in the GFA images.

As part of the DESI exposure sequence, the PlateMaker converts the guide star positions received as part of the exposure request to pixel coordinates for each of the 6 GFA sensors. This information is then submitted to the guider. The guider determines suitable regions of interest around the stars and uploads the configurations to the GFA cameras. With the acquisition phase complete, the GFA cameras start to produce guide star images at a configurable rate, typically around 1 Hz. The guider enters tracking mode continuously analyzing the guide star images. Shifts in the overall centroid position are determined and error signals are sent to the Mayall TCS to correct telescope tracking.

The guider supports a shift function to change the reference centroid position. DESI will employ this functionality for the final adjustment of the telescope pointing to match the requested target coordinates. When the difference between the measured centroid position and the reference position goes below an adjustable threshold, the guider signals the OCS that the telescope is in position and that the next exposure can begin.

During the tracking phase, the first step in each iteration is to locate the guide stars in each of the ROI postage stamps. In order to avoid losing or mismatching a reference guide star, the guider algorithm always chooses the star with position and flux most similar to the reference guide star. For each of the guide stars found, the centroid is measured and the offset to the reference position is determined. Given the different orientations of the GFA cameras, the guider uses WCS information to convert the individual positions to world coordinates in the equatorial system. As higher signal-to-noise stars provide more accurate centroids, the guider weighs each offset by the corresponding star's signal-to-noise before calculating the final offset that is sent as error signal to the telescope control system. In order to avoid combining spurious detections, the algorithm will analyze the agreement/discordance among the different guide star offsets (from 3 to 24) to discard the outliers and those stars that provide very inaccurate centroids.

As guide star images are analyzed during the course of a science exposure, additional information such as atmospheric seeing, transparency and sky levels is extracted. This information is used by the exposure time calculator to determine the optimal exposure time that will maximize overall survey throughput.

6.2.4 Exposure Time Calculator

Most DESI targets will require only a single exposure. In order to maximize survey throughput, exposure times cannot be fixed in advance and must adapt to the changing conditions that determine the integrated signal-to-noise ratio. The online exposure-time calculator (ETC) is responsible for estimating the optimal exposure time during the open-shutter integration time, using real-time updates from the guide sensors.

The ETC is initialized for each exposure using the following inputs obtained via the DESI Online System:

- Target integrated signal-to-noise ratio (SNR) for an average spectroscopic target.
- Configuration data for the Guide and Focus Array (GFA), including:
 - Magnitudes and colors of guide stars that will be read out.
 - GFA camera readout cadence and exposure time.
 - Parameters for temperature dependence of GFA camera dark current.
- Exposure t_0 when all targets should nominally be centered on their fiber and refraction effects should be completely removed by the Atmospheric Dispersion Corrector (ADC).
- Telescope pointing in RA and DEC and corresponding nominal airmass.
- Predicted sky spectrum based on recent calibrated sky-fiber observations. This last item is desirable but not strictly required.

The inner loop of the ETC consists of ingesting calibrated GFA images and sensor temperature measurements at about 1 Hz and deriving estimates of the corresponding incremental spectroscopic signal and background. Specifically, the ETC uses the following GFA outputs from each iteration of the guide loop:

- Up to 24 calibrated postage stamp images containing guide stars. These are used to estimate the focal plane PSF size and shape and to monitor relative changes in atmospheric transparency.
- Pixel data for regions containing no stars or bright galaxies. These are used to estimate the combined sky level and dark current and could either come from the margins of sufficiently large postage stamps containing stars, or else from dedicated background stamps. We estimate that a total signal-free area of ~ 1000 pixels per GFA exposure will be sufficient.
- Measurements of each GFA's sensor temperature. These are used to separate the sky and dark-current contributions to the background estimate. We estimate that an absolute rms temperature measurement error of 1.0 °C is sufficient.

DESI-1100 provides a detailed error analysis with forecasts of the expected ETC performance under various assumptions. The relevant quantities are the estimated integrated SNR ν and its error σ_ν , with

$$\frac{\sigma_\nu^2}{\nu^2} \simeq \frac{1}{n} \left[\frac{1}{4} \left(\frac{\sigma_B}{B} \right)^2 + \left(\frac{\sigma_S}{S} \right)^2 \right], \quad (6.1)$$

where n is the number of accumulated guider exposures, and S and B are the independent estimates of the accumulated spectroscopic signal and background. We find that the relative error on S

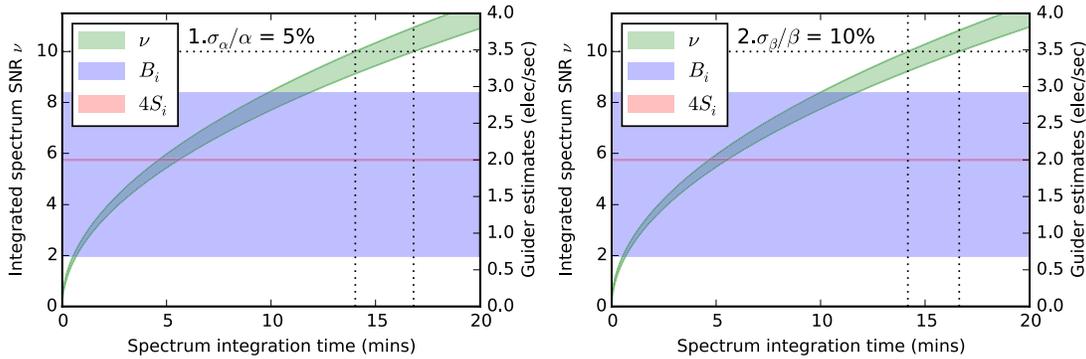


Figure 6.3: Projected evolution of background (blue), signal (red) and integrated SNR (green) estimates during a 20-minute spectroscopic integration. The left-hand plot uses $\sigma_\alpha/\alpha = 0.05$ and the right-hand plot uses a larger error $\sigma_\beta/\beta = 0.10$ that gives a comparable error on σ_ν/ν . The width of each band shows estimated 1- σ errors, including the (red) signal curve where the error is not visible. Background (blue) and signal (red) estimates are per guide exposure and use the right-hand axis, in units of detected spectroscopic electrons per second.

is negligible compared with the relative error on B , but that both are sufficiently small under reasonable assumptions that they are not likely to dominate the overall ETC error. Instead, the cross calibrations between the guider and spectrograph responses to signal (α) and background (β) are expected to dominate. Figure 6.3 shows a sample forecast for the integrated SNR during a 20-minute exposure with different assumptions about these cross-calibration errors. Overall, we expect that the ETC will be able to determine the optimal time to end a typical exposure within a window of ± 90 seconds.

6.3 Readout and Dataflow

The DESI instrument consists of ten identical spectrographs each with three cameras covering different wavelength regions. Each camera uses a single $4k \times 4k$ CCD with four readout amplifiers that operate in parallel. A default pixel clock of 100 kpixels/s results in a readout time of approximately 42 seconds. The charge contained in each pixel is reported as a 16-bit unsigned integer yielding a data volume of 34 MBytes per camera or about 1 GByte per exposure for the entire instrument. A schematic view of the DESI readout system is shown in Figure 6.4. We have adopted a modular approach consisting of 30 identical data sources, one for each camera. Data flows from the top starting with the CCDs and ending with the images stored as multi-extension FITS files on disk arrays in the computer room. Each CCD is connected to a CCD frontend electronics module described in detail in Section 5.5.4. Besides the digitizer, clock signals and voltage generators, the module includes a full frame buffer, a powerful ARM microprocessor, and a high speed network interface. The CCD controllers run regular Linux which enables us to fully integrate them with the DESI on-line system without the need for an additional interface. As shown in Figure 6.4 a DOS application (Camera) runs on each CCD controller. Besides CCD readout and the data transfer to the Image Builder farm, this application handles the front end electronics configuration, collects telemetry information and monitors operating conditions. The integrated network connection combined with the modular design allows us to operate individual cameras with only a laptop computer, a network cable and of course the online software suite. We expect this to become a very valuable tool during construction, commissioning, and maintenance. The design of the CCD controller is complete and

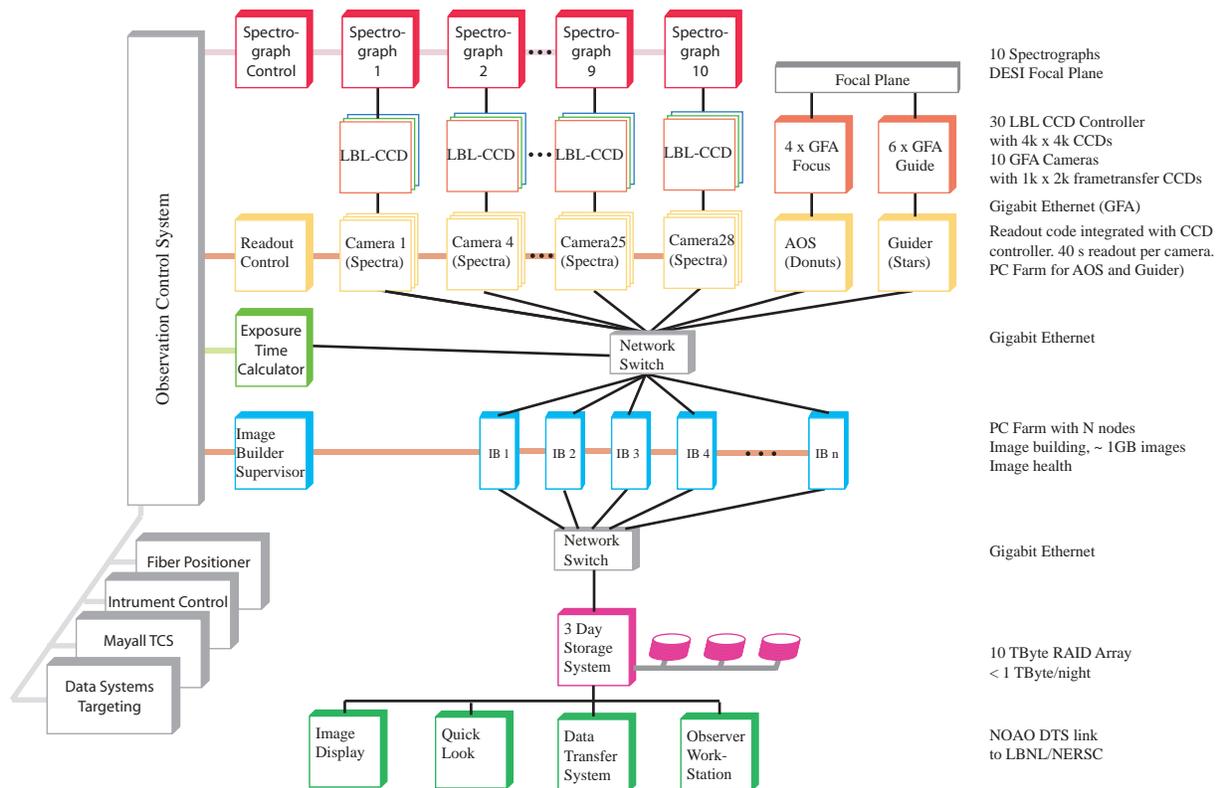


Figure 6.4: Block diagram of the DESI data acquisition system.

a software interface library has been developed. The integration with the DESI Online System is underway.

It is the responsibility of the Image Builder to collect data from all 30 CCD controllers, to combine the fragments to a single, multi-extension FITS file and to insert additional information about the current exposure into the FITS header. The images are compressed using the standard Rice/tile algorithm and saved to the 3-Day storage system. This disk array has sufficient capacity to record several nights worth of images should the link off the mountain be unavailable for an extended period. When an image is complete, the Image Builder notifies the DTS to start the transfer off the mountain and the quicklook pipeline is alerted that the next exposure can be analyzed. A display in the console room shows the CCD images (or an observer selected subset) and summary information is shown on the observer console user interface. The images from the 10 GFA cameras are also recorded in the 3-Day storage system from where they are eventually transferred to the DESI processing facility at LBNL NERSC.

Data transfer from the CCD controllers will begin shortly after the start of digitization and will proceed concurrently with CCD readout. System throughput will be designed to match the CCD readout time of 42 seconds to avoid additional dead time between exposures. The required bandwidth of approximately 10 Mbits/s is easily achievable with current technology.

The DESI readout and dataflow system is based on the same architecture we developed for the DECam online system. Functional prototypes of the camera and image builder applications have been developed and are operational.

6.3.1 Quality Assessment

Continuous monitoring of both the hardware and the data quality is required to control systematic uncertainties to achieve the science goals of the project and to allow continuous, error-free operation of the DESI instrument. Several components of the DESI online system are designed to implement these quality assurance procedures. ImageHealth, a first check of the data quality of every exposure, runs during the image building stage. The image health algorithms determine mean and noise values for each CCD amplifier in both the overscan and data regions and perform additional simple tests at the pixel level to ensure that the spectrographs are functioning properly. During the night, the observer at the telescope will also require automated feedback on the data quality to gauge progress of the observations and to ensure that the instrument is performing as expected. We will build on the experience of the BOSS team which has a quick reduction pipeline in operation on the Sloan Telescope. This quicklook pipeline is a simplified version of a full reduction pipeline, replacing the most expensive computational steps with simpler (and in some cases more robust) algorithms. Quicklook determines sky levels and calculates S/N estimates per exposure as a function of wavelength and object magnitude. This allows a robust, near-real-time assessment of data quality as a cross check of the exposure length and tile completeness as determined by the guider data and exposure time calculator. Results from the quality assessment processes will be logged in the telemetry database that is part of the DESI operations database system.

Additional quality assurance tools will be available to the observer including full data access. The DESI online system will automatically copy every exposure to an observer workstation where it can be accessed by standard tools such as ds9, idl or iraf for an in depth interactive analysis. The observer can choose to process the spectra and guider images with their private, customized algorithms. These operations are completely decoupled from the DESI image pipeline and do not affect the overall throughput.

6.4 Operations Database

At the heart of the DESI online system is the database system that hosts the databases for DESI mountain-top operations. The system consists of a number of different components, with each component having its own schema within the database. This structure keeps the different sets of tables organized while still permitting queries that join together tables in different schema. This would not be possible if we kept the different components in separate databases. For convenience in what follows, we refer to the various components as databases.

The **Telemetry Database** will capture information obtained from the Instrument Control System, the online QA software, the Mayall TCS and environmental systems, as well as from other DESI online components. The method of storing data in the telemetry database during DOS operation will be via the Shared Variable Engine (SVE). The data will be stored by a DOS application called telemetry. It uses the asynchronous call back feature of the SVE to trigger the data storage. The application queries the database for the table schema so it does not need be provided with schema. This makes it easy to add new tables as required. It will also be necessary to log telemetry from systems even when the DOS is not running. This will be done by a set of scripts that retrieve data from the various systems and write it to the database. There will be monitoring tools that check to see that the scripts are running and data is being stored so that data does not get lost. There will be a Telemetry Viewer web-based application that allows users to make plots of quantities in the telemetry schema and retrieve data via SQL queries.

The **Constants Database** is intended for data that is required to configure the ICS and the instrument. This is data that changes infrequently but need to be version controlled. The tables are

stored in the constants schema. A consistent set of constants is called a snapshot and is made up of groups that collect together related elements which contain the actual constants. We define the concept of a snapshot tag as a tag that can be assigned to a different snapshot at different times. There will be an API that allows the user to retrieve constants from the database in a variety of ways. A web-based tool will be provided for manipulating the contents of the ConstantsDB. Access control will be required in order to make changes but viewing will be open. The web tool will allow the contents of the ConstantsDB to be manipulated in a consistent way.

The **Alarm Database** is part of the DOS Alarm System. These tables are stored in the alarm schema. Both DOS and non-DOS applications can raise alarms by inserting them into the alarm database. The database sends out notifications that include information about the alarm level and the name of the DOS instance that raised the alarm. Any number of programs can connect to the database and listen for these notifications. DOS provides a set of standard actions including support for auto-dialer/phone calls, emails and forwarding of alarms to the DOS shared variable system. The software will be designed so that it can be used by both DOS and non-DOS applications. The only requirement is that the alarm database is operational and accessible. A web-based viewer will be provided that allows users to view the alarm table in the database. This is intended for archival use as the real-time display of alarms will go through the DOS GUI.

The **Exposure Database** tracks the status of an exposure as it passes through the system. The tables are stored in the *exposure* schema. There is a Python API that allows programs throughout the system to read and write the status of an exposure. The exposure table is responsible for automatically generating the exposure numbers of each exposure. There will be a web-based viewer that allows users to view the exposure table in the database. This is intended for archival use as the real-time display of exposures will go through the DOS GUI.

The **Survey Strategy Database** used by the Data Systems group will record the field centers of the full survey, the fibers assigned to each field, the priority of each field for observing, the date each field was observed and the approximate date that each field is expected to be observed according to the long-term simulations.

The **Electronic Logbook** is provided by DOS group for recording operational details during installation and commissioning and continuing on into survey operations. We are planning on using the ECL product from FNAL. This is a web application with a PostgreSQL database backend. It is in widespread use by multiple experiments at FNAL as well as by the DECAM instrument at CTIO.

6.4.1 Guider Image Data Management

Currently the plan is to keep about one year's worth of guider images and their associated metadata within the DOS system. The locations of the images on disk will be tracked in the database but the actual images will be stored in a file system rather than in the database. There will be an association in the database between a given guider exposure and the science exposure from the ExposureDB. The guiding rate is expected to be about 1 Hz so using a maximum exposure time of 1800 seconds along with the 6 guide cameras and two postage stamps per camera there will be about 22000 guider postage stamps per science exposure. Taking the assumption of 1940 hours of observing per year yields 80 million stamps per year that have to be managed. Each stamp is assumed to be about 10KB which is 800 GB of data per year. To avoid managing large numbers of small files on disk, they will be aggregated so that all the postage stamps from a single science exposure are collected into something like a zip file.

6.4.2 Technology Choices, Reliability and Development Status

The database server will be PostgreSQL¹. We will use the current stable production release at the time that the DOS system is installed at KPNO. The interface to the database will be developed using SQLAlchemy². The underlying database driver is psycopg2³. The web viewers use mod_wsgi to connect with the Apache server. The plotting in the Telemetry Viewer is done using ChartDirector⁴

We will use the PostgreSQL streaming replication to make a standby copy of the database at KPNO. In the event of a disk failure on the master this will allow us to switch to the standby and continue operations with minimal downtime. This arrangement is used for the Dark Energy Camera and has already demonstrated its usefulness during a disk failure, only a couple of hours of downtime were incurred while the switch was made. We will also use the same streaming replication to have a query-able read-only copy of the database at one or more offsite locations, referred to as a mirror. This will allow access to all the telemetry and other data from outside the KPNO firewall. We will also run copies of the various web viewers against this mirror database(s). We will also make static backups of the database on the appropriate timescale. These will be stored on another machine in the online system but will also be transferred back to NERSC for storage. We will also develop tools to monitor the health and status of the database.

Many of the key parts of the database system have been operating reliably for the last four years for the DECam instrument at CTIO [23]. These components will undergo some modest evolution as a result of the experience gained with DECam. This allows us to focus effort on the new parts needed for DESI such as the GuiderDB. The use of a hot standby for quick failover and the use of an offsite mirror to provide collaboration-wide access to the telemetry data have proved to be extremely beneficial for DECam and will be a key element of the strategy for DESI.

6.5 Instrument Monitor and Control System

Hardware monitoring and control of the DESI instrument is the responsibility of the instrument monitor and control system (IMCS). We distinguish three sets of ICS applications: The first set consists of critical systems such as the CCD cryostats and the monitor system for the frontend electronics have to operate at all times. Fail-safe systems and interlocks for critical and/or sensitive components will be implemented in hardware and are the responsibility of the device designer. Control loops and monitor functions for these applications will use PLCs or other programmable automation controllers that can operate stand-alone without requiring the rest of the DESI IMCS to be online. Measured quantities, alarms, and error messages produced by these components will be archived in the DESI operations database where they can be accessed for viewing and data mining purposes.

The second set is made up by all the different systems that provide environmental data and other telemetry information. This includes the Mayall dome and telescope telemetry system, the spectrograph shack, computer system status and similar systems. We intend to record this information around the clock independent of the state of the DESI online system.

The third set of instrument control applications consists of components that participate more actively in the image acquisition process such as the shutters, the fiber positioning mechanism and the focus and alignment system. The control interface for these devices typically consists of a

¹<http://www.postgresql.org>

²<http://www.sqlalchemy.org>

³<http://initd.org/psycpg>

⁴<http://www.advsofteng.com>

network enabled microcontroller with firmware written in C. The online system interacts with the hardware controller via a TCP/IP socket connection although other interfaces will be supported if required. The DOS group provides the higher level software in the instrument control system while the microcontroller firmware will be developed by the groups responsible for the respective components. Similar to the first two sets, these applications will also use the operations database to archive the information. Devices and applications in the third group will be started and stopped with the rest of the online system and will not operate continuously.

DESI control applications can be categorized by the systems they are supporting. Each of the 10 spectrographs comes with a dedicated **Spectrograph Controller**, an embedded Linux computer that controls the spectrograph mechanisms such as the shutter, the fiber back illumination and the Hartmann doors. The Spectrograph Controllers are fully integrated in the DESI online system and are handled similar to other nodes in the system. The spectrograph software, a DOS framework application (see Section 6.7.3), provides observer and expert access to the spectrograph mechanisms and controls spectrograph related activities during the exposure sequence. A similar computer is used to control the spectrograph shack and to monitor environmental and operational parameters. The cryostat system for the spectrograph CCDs has an independent control system. The cryostat control system includes an OPC-UA server⁵ that allows DOS readonly access to monitor operating conditions and react to error and alarm conditions. All telemetry information collected from the spectrograph controllers, the cryostat control system and the spectrograph shack is archived in the operations database.

DESI will employ a software based **Time Distribution System** using the multicast protocol to inform the spectrograph controllers to open the shutter and to start an exposure. Several software solutions were evaluated and the multicast option achieved a typical jitter between the different spectrographs of less than 10 ms. This is less than the variability in the spectrograph mechanisms and meets DESI requirements. A dedicated timer is used on each spectrograph to control the actual exposure.

The complex DESI focal plane and the prime focus cage assembly require several control applications including the **Fiber Positioner Supervisor**, the **FVC interface**, the alignment system with the **Hexapod Controller** and the **ACD Controller**, and the **GFA System** already described in Section 6.2.1. Most of these applications are joint developments between DOS and the corrector barrel/cage system or the Focal Plane Systems with the responsibilities and deliverables defined in a series of Interface Control Documents (ICDs).

6.6 Telescope Operations Interface

The DESI Online System interfaces to the existing Mayall telescope control system (TCS) to communicate new pointing coordinates and to send correction signals derived from the guider. In return DESI will receive telescope position and status information from the Mayall TCS. Since the dome environmental system and most of the observatory instrumentation for weather and seeing conditions is already connected to the TCS, we will not access these devices directly but control and monitor them through the TCS. The DESI flat-field and calibration lamps are part of the telescope system and will be controlled through the TCS Interface. Similar to the design developed by our group for the Dark Energy Camera and the Blanco telescope, the DESI online system will include a TCS interface process that acts as conduit and protocol translator between the instrument and the telescope control systems. A block diagram of the associated software modules is shown in Figure 6.5. The message passing protocol and commands are detailed in DESI-0473 in the document database.

⁵<http://www.opcfoundation.org>

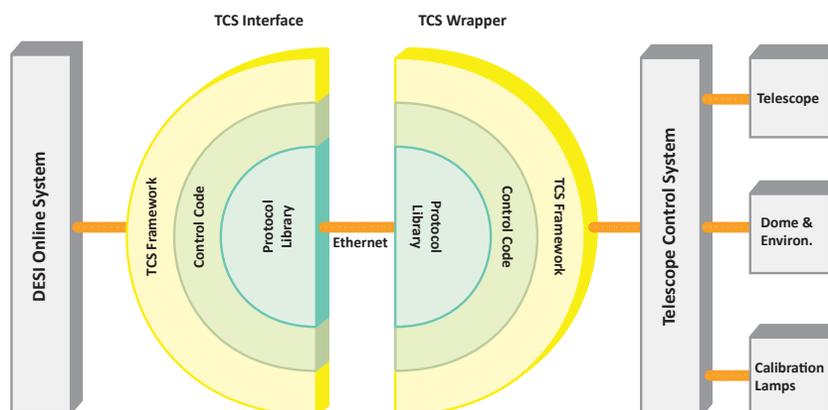


Figure 6.5: Block diagram of the Interface between the DESI Online System and the Mayall Telescope Control System.

During an exposure, the DESI guider and the telescope servo systems form a closed feedback loop to allow the telescope to track a fixed position on the sky. For an imaging survey it is sufficient to have a stable position. DESI, however, requires a precise absolute position so that the fibers are correctly positioned on their targets. Given a pointing request, the Mayall slews into position with a typical accuracy of 3 arcsec. Using the guide CCDs in the focal plane we will then locate the current position to 0.03 arcsec accuracy. As previously discussed, we will send a pointing correction to the TCS to adjust the telescope position, if the offset between requested and actual position is larger than a certain fraction of the fiber positioner motion. To improve telescope pointing accuracy, DESI will provide the current hexapod settings to the TCS for every exposure.

6.7 Online Software

The DESI online software will consist of a set of application processes built upon a layer of infrastructure software that facilitates message passing and information sharing in a distributed environment. The application layer includes functions such as the observation control systems, the different pieces of the instrument control system, and the TCS Interface that have already been discussed. In this section we will focus on the infrastructure layer of the DESI online software that provides common services such as configuration, access to the archive database, alarm handling and processing as well as a standard framework for application development.

6.7.1 Infrastructure Software

The DESI DAQ system will be implemented as a distributed multi-processor system. Due to the nature of this architecture, inter-process communication takes a central place in the design of the DESI infrastructure software. Copying the design of the DECam online system, our solution will be based on the Python Remote Objects (PYRO) software package. PYRO is a free, advanced and powerful distributed object technology system written entirely in Python. It allows objects to interact just like normal Python objects even when they are spread over different computers on the network. PYRO handles the network communication transparently. PYRO provides an object-oriented form of remote procedure calls similar to Java's Remote Method Invocation (RMI). A name server supports dynamic object location, which renders (network) configuration files obsolete. Using the name server, DESI processes can locate and establish communication links with each other

irrespective of the underlying hardware architecture; an important feature for any multi-processor communication system. In a test system, for example, most of the applications might share one or two computers whereas on the mountain everything is spread out over many computers to maximize performance.

We distinguish between Command messages and Telemetry data. Commands are used to request information from a remote application or to activate a remote action. The Command or Message Passing system will be implemented using a Client-Server design pattern with a thin software layer (PML) on top of PYRO. PML introduces the concepts of Component and Device to provide a uniform naming scheme for DESI online applications. The telemetry system will be based on the publish-subscribe design pattern using ideas similar to data distribution services, an emerging standard for publish-subscribe middleware for distributed systems. Again built upon the core functionality provided by PYRO, we developed a concept called Shared Variables that we will adapt to the DESI online system. Consisting of a client stub library and a central server (Shared Variable Engine, SVE), this system allows user applications to publish information such as temperature readings or readout status to a virtual data space. Other applications can subscribe to information placed in this virtual data space and will receive updates whenever a publisher submits a new value. Publishing and subscribing to a shared variable are completely decoupled. A publisher needs no knowledge of who will subscribe to this variable and vice versa. The shared variable system supports asynchronous callbacks, guaranteed delivery, multiple publishers of the same shared variable and group subscriptions.

6.7.2 Configuration

Initialization and configuration of a complex distributed system such as the DESI online system is a multi-step process. The complete system will have about 60 nodes ranging from embedded controllers to server class computers and an even larger number of applications. In order to start the online processes in the correct order, on the correct computer, and with the correct arguments with a single command, we have developed a flexible startup system called the Architect. It is responsible for connecting to multiple hosts and starting DOS services such as Pyro, shared variables and the logging system as well as the user applications. Initialization files in standard Windows .ini notation are used to describe the configuration. The .ini files selects the participating nodes, specifies which applications should be started on each node and provides calling arguments and other configuration information for each process. Once all applications and services are running, the Architect monitors the processes at the operating system level. The Architect implements a management interface to provide full process control so that individual processes can be stopped and restarted without having to restart the entire system.

6.7.3 Application Framework

All DESI online applications will be based on a common software model. This Application Framework (Figure 6.6) serves as a base class and gives the same basic structure to all applications. It provides a unified interface to all DESI services such as the configuration system (Architect), the DOS data cloud (Shared Variables), the message passing and remote procedure system (PML), alarms, logging, the constants database and the interlock and monitoring system. The Framework manages all resources centrally which allows it to unsubscribe all shared variables and to close all PML connections when the application is about to exit. Proper exit handling is critical for the ability to stop and restart individual processes without the need to end the entire instance. Additional functionality provided by the Application Framework include a heartbeat that can be used

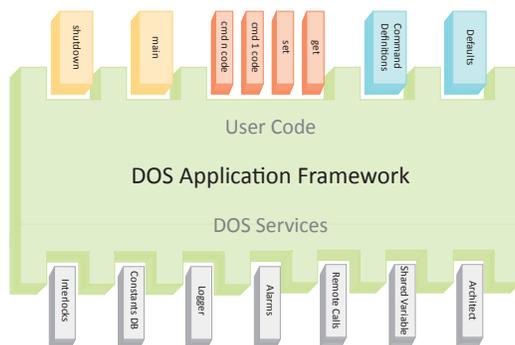


Figure 6.6: Schematic view of the DOS Application Framework. The Framework provides standardized access to DOS services such as the Architect configuration system, the DOS cloud (shared variables) and the messaging system (PML). The user provided pieces are shown on the top.

to monitor the overall state of the system and a standardized management interface with process control functions and access to an application state variable. The user code inherits the application framework class and provides default configuration settings and the list of commands that will be exposed to the online system. Configuration settings can be updated at run time by the Architect. The code to execute the commands has to be written by the user. If the application requires access to the runloop, the user can overwrite the `main()` method and custom exit handlers can be added by overwriting the `shutdown()` method. The DOS Application Framework significantly reduces the complexity of application development. It is lightweight and since it is written in pure Python code it is very easy to port to different host environments. For DESI the application framework will be available not only on workstations and servers but also on most of the embedded controllers of the instrument control system including the CCD controller module, the spectrograph controller and elements of the focal plane control system.

6.7.4 User Interfaces and Observer Console

The DESI DAQ observer console acts as the primary observer interface for day to day operation. This set of graphical user interfaces includes elements for system and exposure control, alarm displays and telemetry monitors. Combined, they present the user with the most commonly used information and everything that is needed to operate the DESI instrument. Near real-time performance is needed to provide quick access to more specific information and to achieve the responsiveness expected from a modern system. The DESI GUI architecture follows the Model-View-Controller (MVC) pattern first developed for Smalltalk but now in common use for large applications. The MVC pattern is based on the realization that all applications are, essentially, interfaces that manipulate data. Following our successful implementation of this approach for DE-Cam, we will implement the controller component as a web server so that standard web browsers can be used to render the views. Using a web browser provides many desirable features such as platform independence, remote access, a large number of 3rd party tools, and a certain level of security. Early concerns regarding usability and performance in a real-time environment have been addressed by recent advances in browser technology. Thanks to faster rendering and JavaScript execution as well as new standards such as HTML5 and the Web-Socket API that allow for advanced

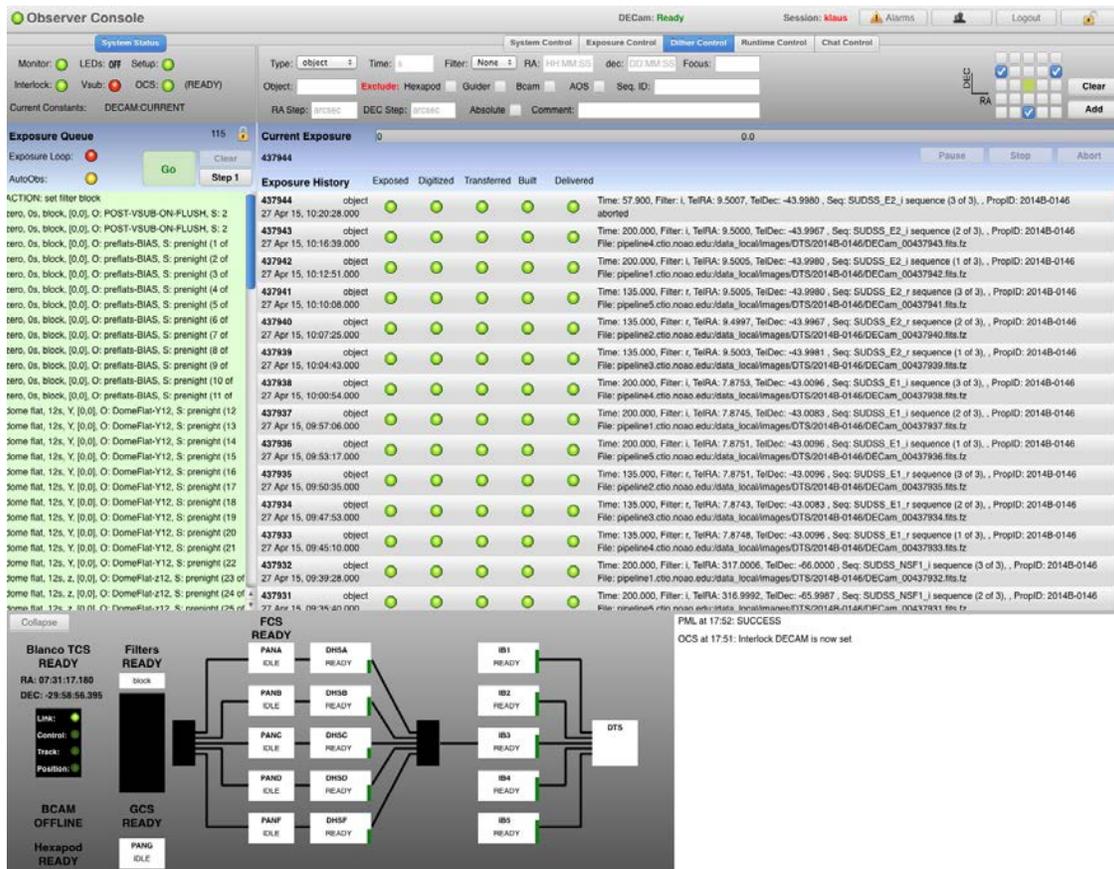


Figure 6.7: DESI will use web-based user interface similar to the DECam observer console shown here.

functionality such as bidirectional socket communication and 2D drawing contexts, web browsers are now on a near equal footing with desktop GUI toolkits. As an example, Figure 6.7 shows the DECam observer console GUI. A similar design will be developed for DESI.

The client side (web browser) code is based on HTML/CSS, JavaScript and an HTML5 application framework such as SproutCore. Websockets, defined as part of the new HTML5 standard and now supported by all major browsers, will provide the most responsive user experience. Conceptually similar to traditional TCP/IP sockets, they allow the DESI DAQ system to push information updates and state changes directly to the GUI. We have successfully ported the GUI system from DECam to the DESI environment and in the process updated many of the underlying software packages. A console for the spectrograph tests at Winlight, France, is currently under development.

6.8 Readout and Control System Hardware

The ICS project is responsible for all DESI computer hardware at the Mayall. This includes the online computers, disk storage, the internal network infrastructure and two multi-display workstations for the Mayall control room. The backbone network infrastructure in the Mayall building will be provided by the observatory. The observatory is also responsible for computer and network security and will provide a firewall and other access control solutions. The main user interface, the observer console, is modeled after the solution we developed for DECam and the Blanco console

Table 6.1: DESI online computer needs. Networking and infrastructure equipment is not listed.

Function	Configuration	Comment
Database Server	Rackmount Server (16 cores, 64GB RAM, 24 TB)	DESI Operations Database
Backup Database Server	Rackmount Server	Database will be mirrored
User Server	Rackmount Server	Repository, home areas
Backup User Server	Rackmount Server	Hot-Standby backup server
GFA System	Rackmount Workstation (12 cores, 64 GB, 2x2TB)	Guider, Wavefront analysis
Focus and Alignment	Rackmount Workstation (5 units)	Donut analysis is CPU intensive (Based on DECam experience)
Image Pipeline	Rackmount Workstation (5 units)	Incl. acquisition, processing
Quicklook Pipeline	Rackmount Workstation (2 units)	Based on BOSS experience
Fiber Positioner Interface	Rackmount Workstation	
Fiber View Camera	Rackmount Workstation	Based on performance tests
DAQ Core Processes	Rackmount Workstation (2 units)	Incl. webserver, PlateMaker
ICS	Rackmount Workstation	Includes TCSInterface
DTS	Rackmount Workstation	Interface to DTS system
Observer Workstation	Desktop Workstation (6 cores, 32 GB, 6 TB)	Includes 6 displays
Observer Console	Desktop Workstation	Includes 6 displays
Image Display	Desktop Workstation	Includes 1 display

room. The DESI and DECam computer systems are similar in scale and we use our experience with DECam to design the DESI system detailed in Table 6.1. In order to maximize system availability and reliability we operate the key server systems with hot-standby backup servers. This configuration provides synchronized backup copies of the filesystem and the DESI database and allows for rapid switch over should the primary server fail. We had one such incident with DECam. We were able to quickly switch over to the backup server minimizing the loss of observing time.

The computer equipment will be housed in the computer room at the Mayall telescope. Clean power and cooling will be provided by the observatory. The system will be configured to allow remote monitoring and system management as much as possible. The number of different workstation configurations will be minimized to facilitate maintenance. Additional smaller test systems are required for development and to support ProtoDESI.

6.9 Integration and Testing

The DESI instrument control system is connected to most major components of the instrument as well as the Mayall telescope. Given the large number of interfaces, we have designed a project plan that makes integration and testing an integral part of the ICS project. For each DESI component that interfaces with the online system, we developed interface control documents (ICD) that detail the hardware connection and define deliverables and responsibilities. These documents will be reviewed and then placed under change control. The ICDs are accompanied by implementation documents that specify details of the API such as data formats, methods, telemetry and alarms. While the hardware components are under development, the ICS team creates software simulators for the interface implementing the protocol as defined in the ICDs and the implementation documents. Adopting a spiral development approach with increasingly complex systems, we have

scheduled a DAQ demonstrator test for the first year of the construction project. During this test we will simulate the ICS DAQ system using prototypes of the core ICS software components and software simulators for hardware controllers. The first spectrograph cameras are in production and a three-camera test using DESI front-end electronics is scheduled in Fall 2015. The ProtoDESI integration test in 2016 will feature complete ICS prototypes and a number of prototype hardware controllers. While the project does not include a standard test-stand facility for all hardware and software components, we can take advantage of the modular architecture of the ICS and run the prototype system at the different production sites. During these tests we will integrate with the available hardware controllers and use our software emulators for the remaining components. Similar integration tests with the complete production system will be repeated at the end of the construction project.

7 Data Systems

Data Systems covers target selection, survey planning, data processing, and data management. Although separate topics, these are closely related in the design and execution of the survey and thus they are jointly planned and managed. The DESI construction project deliverables of Data Systems are:

- **Target Selection Pipeline:** Code to generate a catalog of targets (ELG, LRG, QSO, Standard Stars, and blank sky locations) given multi-band photometric catalogs and selection criteria as input.
- **Survey Planning and Integration with Operations:**
 - A defined set of observation fields that tile the survey footprint;
 - Code to algorithmically select the next field for observation, given current conditions and past observation history;
 - Code to assign input targets to focal plane fibers, prioritizing targets of different classes to maximize the overall survey impact;
 - Code to dynamically determine exposure times given real-time guider camera inputs;
 - Code to assess spectroscopic data quality shortly after observations complete.
- **Spectroscopic Pipeline:**
 - Code to convert raw data into wavelength-calibrated, sky-subtracted, flux-calibrated spectra;
 - Code to measure spectroscopic classifications and redshifts;
 - Code to track the 3D survey efficiency for generating large scale structure catalogs.
- **Data Transfer, Archive, and Distribution:** Tools to automatically transfer, back-up, and distribute raw and processed data. This system integrates with the Spectroscopic Pipeline to process new data as they arrive, and distribute processed data when they are available. This activity also has oversight of documentation, coding standards, and tagged releases of both reduced data and code.
- **Collaboration Tools:** Tools to facilitate the efficient operations of the collaboration including a wiki, code repository, bug tracking system, mailing lists, document repository, and website.

From the perspective of Data Systems, DESI is a modest expansion of what is already done with SDSS-III/BOSS: 10 spectrographs with 3 channels each instead of 2 spectrographs with 2 channels each — a factor of $7.5\times$ more data per exposure. Wherever possible, we have made technology and requirements choices based upon the experience of the highly successful BOSS spectroscopic pipeline and SDSS-III data management systems. The spirit of these systems also influences our design choices, for example:

- the primary interface between pipeline steps is defined by a “data model” for those files rather than function call signatures or object oriented class interfaces;
- simplicity and pragmatism are key design considerations;

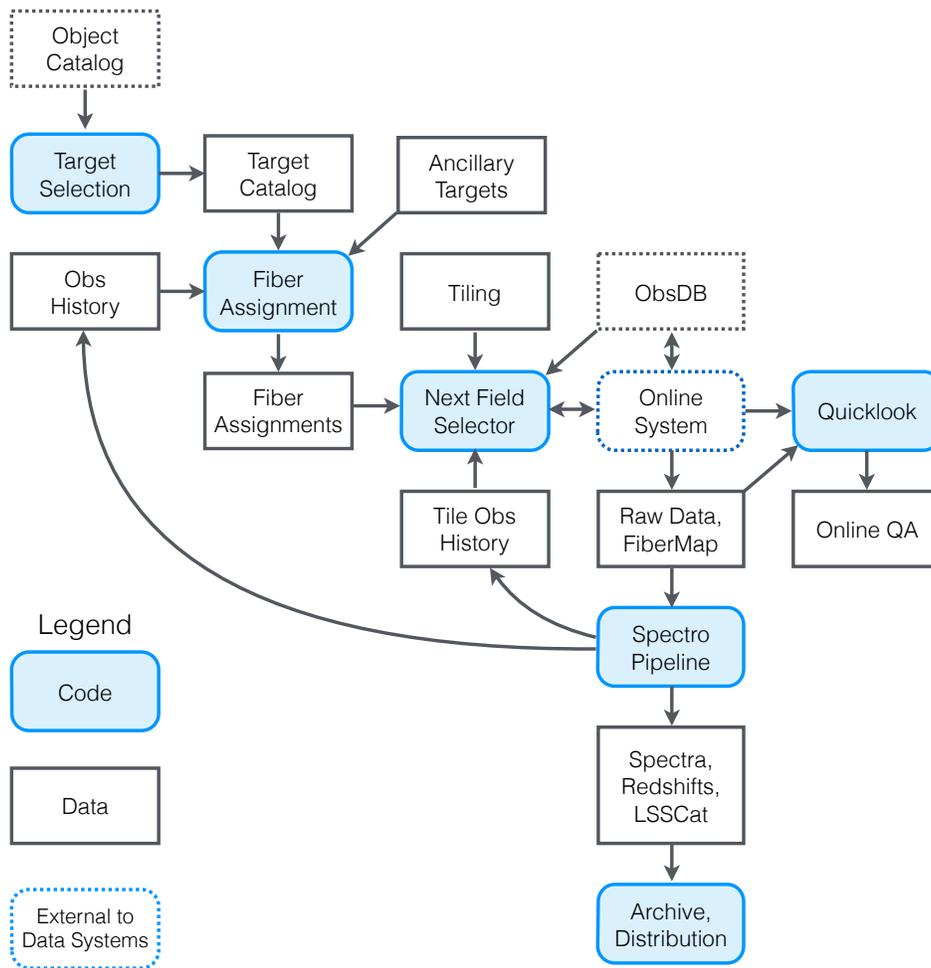


Figure 7.1: Block diagram of DESI Data Systems data flow.

- files on disk are the authoritative data product rather than a centralized database (though databases will be used);
- software should be runnable on a laptop without an internet connection for debugging and development.

At the same time, we are taking the opportunity to modernize significant portions of the system for updated algorithms and long term maintainability.

Figure 7.1 shows a block diagram of the DESI data flow, including interfaces between Data Systems and other parts of DESI.

- **Target selection** takes an input catalog of detected objects and selects which ones DESI should observe.
- **Fiber assignment** chooses which targets should be observed for each tile on the sky, using priority ranking as necessary to choose between multiple targets visible by a single fiber.
- The **next field selector** makes the real-time decision of what tile to observe next to achieve the survey strategy. It passes this choice to the Instrument Control System, which implements the actual observations to produce raw data.

- The **spectroscopic pipeline** processes these data to produce spectra, redshifts, and a Large Scale Structure catalog.
- **Quicklook** software performs a fast simplified version of the spectroscopic pipeline during observations to provide rapid turnaround quality assurance plots and metrics.
- Data are **archived** to tape and at a geographically distinct backup site; all stages of the data processing are available to the DESI collaboration via **data distribution** tools.
- **Simulations** and **data challenges** (not shown) are used for development and testing of these items.

7.1 Target Selection Pipeline

Target selection is described in detail in the Target Selection section of the Science Technical Design Report. This includes the astrophysical question of selecting ELG, LRG, and QSO targets from the imaging datasets, as well as the selection of regions of blank sky for sky subtraction and standard stars for flux calibration.

Data Systems is responsible for applying versioned selection algorithms to all of the versioned imaging datasets and generating a catalog of targets to observe. The catalog will provide a unique ID for each target that is traceable back to the input images, the processing version of the input catalogs, and the version of the target selection algorithm used. This target ID is passed forward through the data processing and provides traceable provenance of why each target was selected and which input catalogs contributed to that selection.

The target catalog contains approximately as many targets as are observable over the course of the full DESI survey. The target selection pipeline does not prioritize targets — that is the responsibility of fiber assignment in coordination with the survey planning team.

Figure 7.2 shows a block diagram of the target selection database which tracks these catalogs and their provenance back to the input imaging data. The Images table tracks the original input images. The Bricks, Tractor, Tractor2Images, and Single tables track how those images are processed to identify objects for the Candidates Table. Target selection then applies cuts to the Candidates table to produce the Targets table with the list of targets that DESI should observe.

The target selection uses of a PostgreSQL database hosted at NERSC; this can be dumped and loaded at another computer offsite if needed. Within the database we employ Q3C for fast spatial queries. Q3C (Quad Tree Cube) is a sky indexing scheme developed by [28] that has an SQL interface for main astronomical queries: cone searches, various spatial searches on the sphere, and cross-matches of catalogs. The performance is quite good and allows one to work easily with the largest existing catalogs simultaneously.

The data management team is responsible for archiving the targeting datasets and coordinating the data flow from the selected targets through fiber assignment, observation, and downstream to analyses. In particular, large scale structure analyses rely upon information both about the targets that were observed *and* targets that were selected but never observed due to limited fiber resources.

The target selection pipeline will be released to the community in an “as is” fashion, without continued maintenance or support. Note that the processed images used by the target selection pipeline are a deliverable of the DESI science collaboration, not the DESI project itself.

The computing requirements for target selection are presented in Section 7.7.1.

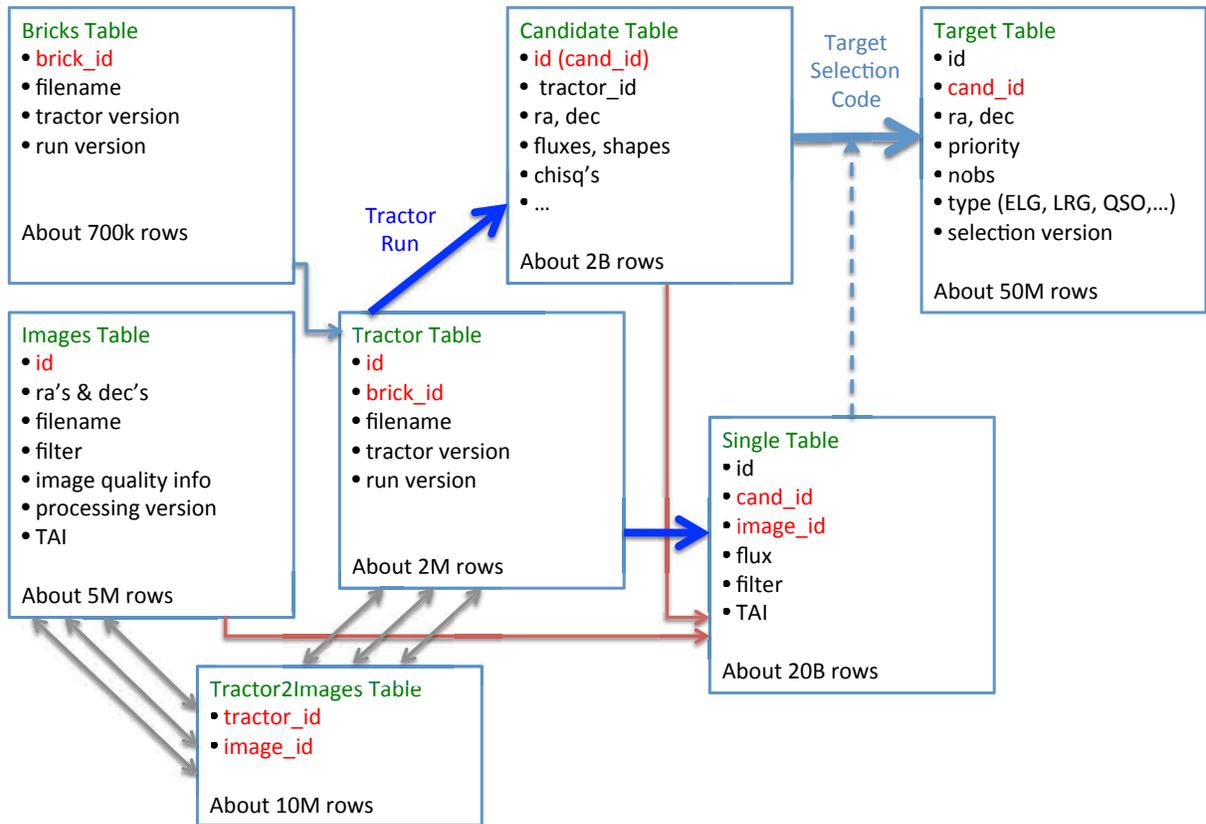


Figure 7.2: Block diagram of target selection database schema.

7.2 Survey Planning, Fiber Assignment, and Operations

The survey footprint, field centers, and overall survey plan are described in the Science TDR. Data Systems is responsible for developing and implementing this plan with fiber assignment, the next field selector, and quick-look, as described in the following sections.

7.2.1 Fiber Assignment

Fiber assignment is the process of selecting which targets are assigned to which fibers on which tile, and thus also which targets are *not* assigned to any fiber in the regions where there are more targets than available fibers. Fiber assignment depends upon the details of the fiber positioner layout, the survey tiling pattern on the sky, the input target catalogs, and spectroscopic pipeline feedback for targets that have been previously observed. For each tile, Fiber Assignment will provide the RA, DEC, and target ID selected for each fiber. These outputs are passed by the Next Field Selector to the Instrument Control System.

7.2.1.1 Merged Target List

A precursor step of fiber assignment is to generate a Merged Target List, which combines the information from multiple sources: the key project target catalog; results from any previous observations

of these targets; catalogs of standard stars and blank sky locations; and possibly ancillary target catalogs. Results from the spectroscopic pipeline will be used to inform which targets have been fully observed and which require additional observations. Each target (other than standard stars and sky fibers), whether from the original Targeting Catalog or from any other source, will come with a numerical priority. In the case of the Key Project, these will be fixed to provide the desired ranking among LRGs, ELGs, and QSOs. Ancillary targets will be provided priorities, assigned in a way that will assure that the Key Project is not significantly impacted. Each collection of ancillary targets will be assigned a new category label, analogous to the fundamental labels LRG, ELG, QSO, and each ancillary target will have a unique identifier, just as the Key Project targets.

The MTL provides flexibility in assigning target priorities for the Key Project, the Bright Time Survey, and ancillary programs. The priorities will not be built into the final Fiber Assignment code but rather the MTL will define the various types, extending the Key Project list of target types (LRG, ELG, QSO, ...).

7.2.1.2 Key Project Target Fiber Assignment

Roughly 25,000 Key Project targets will fall on a single plate and each spot will be revisited, on average, a bit over five times. So with 5,000 fibers we have a near match of fibers and targets. However, fluctuations either due to Poisson statistics or to clustering will result in domains where not all targets can be measured (and other domains where there will be fibers with no unobserved targets within reach). Thus choices need to be made.

As discussed in the Variations of Forecasts with Survey Parameters subsection of the Science TDR, the marginal Figure of Merit is higher for each Ly- α forest QSO, QSO, and LRG than it is for each ELG. This relative FoM for each target class and required exposure times leads to the following baseline prioritization scheme for DESI targets:

1. confirmed Ly- α forest QSOs with known redshift $z > 2.1$, except during grey time, during which only ELG targets will be observed. The grey-time program will extend over the course of five years, using the fraction of time with the highest illumination from the moon as described in the survey section of the Science TDR.
2. QSOs targets not yet observed.
3. LRGs that have been observed but not to their requisite depth (each LRG requires 1–3 observations depending on their magnitude).
4. LRGs targets not yet observed.
5. ELGs targets.

Every exposure also requires standard stars and sky fibers for calibration. For each tile we require that every one of the ten petals has at least 10 standard stars and 40 sky fibers. If the initial assignments don't permit this, some ELG targets are sacrificed for the purpose.

Because the ranges of the positioners overlap, care must be taken to avoid physical collisions. The Fiber Assignment code tests whether an assignment will lead to a collision with a previously assigned fiber. The test uses the specific shape and dimensions of the positioner. All potential assignments leading to a collision are rejected and an alternative assignment is sought. The final check that there are no collisions will be the responsibility of the Instrument Control System.

As will be shown in the following section and Table 7.1, this prioritization strategy results in nearly 100% rate of fiber assignment to the QSO and LRG samples, with roughly 78% yield for ELG targets.

Table 7.1: Performance of the baseline tiling simulated on 14k sq. deg. of the mock galaxy sample with 6-mm positioners for the full focal plane. All densities in (sq. deg.)⁻¹. Consecutive observations of a galaxy are required to be separated by an interval of at least 200 tiles.

	Times Observed						Initial Number.	Fibers Used	Number Observed	Fraction Obtained
	0	1	2	3	4	5				
QSO Ly- α	0	1	4	15	26	1	49	169	49	0.989
QSO Tracer	1	118	0	0	0	0	119	118	118	0.989
LRG	15	35	247	0	0	0	298	530	283	0.948
ELG	531	1,879	0	0	0	0	2,411	1,879	1,879	0.780
Fake QSO	0	89	0	0	0	0	90	89	89	-
Fake LRG	2	47	0	0	0	0	50	47	47	-

Table 7.2: Performance of the tiling simulated on 9k sq. deg. of the mock galaxy sample with 6-mm positioners for the reduced “Pacman” focal plane. All densities in (sq. deg.)⁻¹. Consecutive observations of a galaxy are required to be separated by an interval of at least 200 tiles.

	Times Observed						Initial Number	Fibers Used	Number Observed	Fraction Obtained
	0	1	2	3	4	5				
QSO Ly-a	1	1	4	14	28	0	49	169	48	0.979
QSO Tracer	2	117	0	0	0	0	119	117	117	0.979
LRG	16	31	250	0	0	0	298	532	282	0.944
ELG	487	1,924	0	0	0	0	2,411	1,924	1,924	0.798
Fake QSO	1	88	0	0	0	0	90	88	88	-
Fake LRG	2	47	0	0	0	0	50	47	47	-

7.2.1.3 Performance of Tiling and Fiber Assignment

The performance of the tiling and fiber assignment has been studied with mock catalogs from N-body simulations. Those simulations assign ELGs, LRGs and QSOs to dark matter halos at the areal densities and redshift distributions presented in the Target Selection section of the Science TDR. The completeness for each target class is presented in Table 7.1 for the full focal plane and in Table 7.2 for the reduced focal plane with 3000 fibers. The QSO targets are separately listed as those at $z < 2.1$ (QSO-tracer), which are used as tracers only, and as those at $z > 2.1$ which are used for the Ly- α forest. A fraction of the LRG and QSO targets will be targeting failures, and have been listed separately as “bad” targets. The Ly- α forest QSOs are not assigned to the fifth-pass grey time observations, but some of these targets still receive more than four observations.

The fiber assignment algorithm will have as input the Merged Target List (MTL). The true nature of the QSO and LRG targets is unknown until they are first observed. The fakes are not observed again. The QSO tracers and ELGs are not observed again, since a single exposure is sufficient to measure their redshift. The Ly- α QSOs continue to be observed to a maximum of five observations. The LRGs are observed to a maximum of two exposures. This may be modified in the future to allow LRGs to be judged as requiring one, two, or three observations, depending on their brightness.

7.2.1.4 Calibration Target Fiber Assignment

In addition to key project targets (ELGs, LRGs, QSOs), every exposure must include standard stars for flux calibration and fibers assigned to blank sky for modeling and subtracting the night sky spectrum from science fibers. These calibration targets will be assigned to remaining fibers after the key project target fiber assignment has been completed. When necessary, fibers assigned to ELG targets may be exchanged for standard star targets if density fluctuations result in an insufficient number of standard stars available on the spare fibers.

Based upon BOSS sky and calibration star studies, 40 sky fibers and 10 standard stars are required for each spectrograph, representing 10% of the total fiber budget. Locations of blank sky and standard star targets are provided by the target selection pipeline and included in the MTL.

Many more “blank sky” locations than the required density will be provided. These will be selected as random sky positions for which there are no detected objects within a sufficient distance to ensure that flux from extended objects is excluded. From this abundance of possible “sky” locations, the fiber assignment will select 40 per spectrograph per exposure.

7.2.1.5 Ancillary Program Target Fiber Assignment

The final and optional step in fiber assignment is for ancillary program target requests. These could be assigned to unused fibers, and may also override standard star and blank sky fiber assignment within the constraints of calibration target uniformity and minimum numbers required. However, in most cases, key project targets will be assigned first, then calibration targets, and then (optionally) ancillary targets. Performing the fiber assignment in these steps allows the survey to pre-plan the key project and calibration fiber assignments, while allowing flexibility for last minute target-of-opportunity style ancillary requests. This decouples the key project targeting from external program ancillary target requests, allowing both greater implementation freedom. All this will be managed through the MTL.

In exceptional cases, it may be possible for ancillary targets to override key project targets, with the necessary bookkeeping of this fiber assignment override passed forward to final analyses. We do not anticipate this to be a standard mode of operation but structurally this will be a collaboration management decision rather than an artificial constraint from the design of the fiber assignment and data management systems. The default operation will be to assign unused fibers to additional “sky” targets and spectrophotometric standard stars.

7.2.1.6 Target Assignment Bookkeeping

Large-scale structure clustering analysis depends upon a detailed knowledge of the efficiency for successfully observing each target. Upon the completion of fiber assignments for a suite of tiles, the fiber assignment status must therefore be tracked for each target. As described in Section 6.4, the status for each target will be updated following observations to reflect observing conditions and spectroscopic classification. This will be done by the MTL.

The interface with instrument control system (ICS) decouples the details of tiling and fiber assignment from the mechanics of actually observing. For each tile, Data Systems will provide a file defining the field center, the mid-point observation time, the sky coordinates (RA, Dec) of each assigned target, and the design wavelength for each target. The ICS will use this information to translate the sky coordinates to physical coordinates on the focal plane (in mm) for each fiber positioner (PlateMaker; Section 6.2). Although there is an atmospheric dispersion corrector (ADC), there are still small-term offsets due to the atmosphere that effect the translation to physical coordinates. In principle, each target location could be optimized to a different design wavelength,

although these effects are small within the ADC design range of $1 < \text{Airmass} < 2.0$. The default operation will be to use the same design wavelength for all targets.

The well-defined interface between target lists and PlateMaker allows flexibility for creating custom tile definitions for commissioning, debugging, and potential non-Key Project observing programs. A verification program will allow pre-testing that fiber assignments are physically possible, although responsibility for instrument safety (e.g., avoiding fiber collisions) rests with the ICS.

7.2.1.7 Bright Time Survey Fiber Assignment

The above description of fiber assignment has focused on the dark time key project survey, but the same code is directly applicable to the bright time fiber assignment as well. The basic structure fits both programs: each has a pre-defined tiling of the sky and input catalogs of various target classes with priorities and requested number of observations. They will differ only in the inputs, while using the same fiber assignment code.

7.2.2 Next Field Selector

The next field selector will implement the survey plan in real-time based upon current observing conditions, past observing history, and what part of the sky is currently visible. The DESI Online System (DOS) will run the next field selector as a Python module. The next field selector will choose the next field to observe and pass the information from fiber assignment to DOS for plate mapping and acquisition of that field. At a minimum, the information passed to DOS will include the field center, RA and DEC of each fiber assignment, guide star information, and expected exposure time. The next field selector should work naturally for dark and bright time programs and require the same basic formats.

To optimize survey progress, the results of survey simulations will be used to establish the algorithm to prioritize field selection every time a new field begins. This algorithm will be a function of sky conditions, moon position, and long term strategy. This algorithm will form the basis of the software for the next field selector which will be run in full operations during the five-year survey.

The global planning with hour angle assignments can be updated as often as every afternoon. These modifications to the design of each field will be recorded before the night begins, thus appearing seamless to the software that governs mountain operations. This step could also merge the information from the offline spectroscopic pipeline for tiles that have been observed but need additional exposures. We expect to pre-plan the entire survey while structurally reserving the possibility to make rolling updates.

7.2.3 Quicklook Extraction Pipeline

Unlike BOSS, where observations are accumulated in exposures of fixed duration, DESI will require more precise tuning of exposure times to minimize time lost to over-exposures. DESI will determine exposure depth during open-shutter time using information from the guide camera as described in Section 6.2.4. The guider images will be used to determine sky conditions such as atmospheric transparency, seeing, and sky background. The exposure time calculator will use this information to predict exposure times at the beginning of a field and update approximate exposure depths during each exposure to determine when the field meets a threshold depth to meet survey goals. These exposure depths will be tuned to a fixed S/N ratio for a fiducial target at a fiducial redshift. For example, spectral templates representing the ELG sample will be fed to the exposure time

calculator to estimate the required open shutter time to achieve $S/N=7$ per pixel integrated over the [OII] emission line doublet at the DESI flux limit.

While the real-time exposure progress will be judged by the exposure time calculator, there will be quick-look spectral reductions run on all science exposures to ensure that the data meet the quality predicted at the end of the exposure. These reductions will be used as a diagnostic to ensure that the instrument is performing correctly, allowing the observing staff to address problems quickly should they arise. Under normal operations all observing decisions are automated, while reserving the ability for operator override for testing and exceptional circumstances.

This quick-look code will be a simplified version of the full data reduction pipeline described in the following section, replacing the most computationally expensive steps with faster approximations so that results are available within two minutes of readout. Since it is based upon the full data reduction pipeline, the data group will provide the software for this analysis, which will be integrated into mountain operations software. The results of these quick-look reductions will be archived and distributed as a data product. Similarly, guide camera data, temperature measurements, and any other meteorological information used for making observing decisions will be archived.

7.2.4 Survey Simulations

Software simulations of the full survey will be used to model the order in which tiles are observed and under what conditions each exposure is acquired. Survey simulations will use the same data flow and algorithm code as DOS will use for managing the actual observations. Field centers, target classes associated with each field, hour angles, and long term strategy will all be input to the survey simulations. Weather and moon conditions will be simulated for each night of the year. The next field selector will be used by the simulator to select each field over the course of each night.

Survey simulations confirm the algorithms developed for the next field selector and exposure time calculator subsystems and also test the interface to DOS. These simulations will inform the survey coverage and uniformity of clustering in the end-to-end data challenge. The survey simulations will address the following specific questions regarding Survey Planning:

- What is the final algorithm for the next field selector?
- What is the possible variation in areal coverage due to weather? This will help assess how robust the next-field selector and long-term survey plan will be to seasonal bad weather.
- What is the algorithm for determining real-time exposure times? This would require estimates of seeing, atmospheric transparency, and sky background as part of the survey simulator. These will be used in combination with simulated spectra to test the algorithm for the exposure time calculator and the total exposure time required to complete each field.
- What is the area and target completeness we expect as a function of time? The clustering group will need semi-completed footprints to test issues like reconstruction, fiber collisions, and incomplete target samples.
- What is effect of varying sky background and atmospheric transparency as a function of time? These variations in combination with the simulated spectra will inform the science working groups what level of variation in redshift efficiency to expect over the sky.

7.2.5 Survey Quality Assurance Interface

The quicklook software described in Section 7.2.3 will be used to inform the observer on the quality of each image immediately following the completed exposure. However, the quicklook routines will not provide a high-level overview of survey progress or global data quality. The Survey Quality Assurance Interface will be an online tool accessible to observers and members of the collaboration to track the progress of the survey, planned observations, and data quality.

The quality assurance interface will record information from the operations database, the quicklook extractions, the full pipeline, and the catalogued output of the full data reductions pipeline. It will be used to ensure consistency between the survey progress recorded at the mountain and downstream in the analysis.

It will provide visualization tools to access this information. The tools will interface the Operations database and offline processing results. For example, the interface should display all of the fields in a map that is color-coded by completeness, with an option to show individual layers of fields. It should be able to display histograms of various metrics averaged over each exposure such as sky background and fiducial S/N. The interface should have the ability to show observation progress as a function of time, including projections for future observations. The quality assurance interface will require coordination with DOS.

7.2.6 Planning for Commissioning and Science Verification

DESI will conduct a phase of commissioning and science verification to establish general operational procedures, evaluate instrument performance, and validate selection algorithms applied to each class of target. The commissioning strategy is outlined in Section 9. Members of the Data team will participate in commissioning to ensure that requirements needs are met. The Data team must confirm that the data model is complete for downstream analysis. Likewise, the Data team must test the operations software and iterate with developers to ensure that it is well-documented and observations are easily performed by those who are not familiar with the full system.

Once calibration routines, operational procedures, and instrument performance are understood, time before the main survey should be dedicated to science observations to the extent possible. These science verification observations will broaden the main sample to inform the final target selection and analysis. The exact scope of each of these observations is not yet defined, but one should expect samples on the order of 1% of the final cosmology sample. In other words, each program will likely take one month to complete with a complete spectrograph and should produce hundreds of thousands of spectra. There is overlap between some of these programs, so they should be performed in parallel whenever possible.

Equally important, the observations conducted during science verification should produce samples that are intrinsically interesting and can lead to immediate analysis and results. There may be an early data release to facilitate dedicated analysis of the science verification program. A preliminary list of science verification programs listed in the order in which they will be observed is as follows:

- As discussed in Section 7.2.1.4, the selection of standard stars will require *grz* photometry to cover the entire DESI footprint. Dropping *u* and *i* photometry from the selection will extend the distribution of metallicity beyond the standard star selection that has been well-tested in BOSS. At the beginning of Science Verification, it is likely that the system will not be operating at 100% efficiency. Observations of all stellar classes as bright as 16th magnitude will allow us to explore the metallicity distribution of potential standard star selections and test the instrument performance. Those targets will be more robust against system inefficiencies

than faint targets and will inform operational procedures. Finally, these observations will test our fiber positioning and calibration against astrometry and spectrophotometry from GAIA.

- Validate the exposure times for the bright galaxies over a range of moon/cloud conditions. This and other bright-time tests need to be documented more fully in a document dedicated to the bright-time program. These targets will also be easier to observe in the beginning of Science Verification as they are bright and will allow us to calibrate the throughput more accurately on extended objects.
- Perform a survey using target selection at full density over a limited volume. It is expected that 1–2% of the DESI survey volume could be completed in one month of science verification
- Measure the properties of the objects at the boundaries of the color boxes for each target class. By taking observations of a number of objects over extended selection criteria, we can evaluate the variations of number density as a function of imaging conditions. Imaging conditions to explore include the source of the data (which telescope was used), seeing, $E(B-V)$, calibration errors, zeropoint errors, and other sources of potential systematic in selecting targets from photometric data. By measuring the $N(z)$ at the boundary of color selection, one can empirically measure the derivative of the number density as a function of varying image quality and use that information to model the galaxy samples in the final analysis.
- Measure the properties of the objects that fail to produce redshifts in the normally allotted exposure time. Observations of 3–10X the normal depth will help us to characterize the full sample of objects we are observing and help us to better understand potential variations in the spectroscopic efficiency that result from natural variations in conditions during the full five year program.
- Confirm the properties of the various target classes. This includes the ELG line flux function, the target success rates, and the $n(z)$. If possible, we want to do this in regions representing the various imaging data sets. These measurements should be attainable with the data collected in the two items mentioned directly above.
- Verify that suitable Lyman-alpha depth can be reached in the planned exposure times. This should also be possible with the aforementioned observations.
- We may want to obtain a flux-limited sample as well. A program to $r < 23.5$ would provide targets at a density of 30k targets per square degree, about ten times higher density than the main program. The advantage of such a sample would be to better characterize the overall environment of our matter tracers and to provide a final check on target selection. The disadvantage of such a sample is that the observations are time-consuming, will produce accurate redshifts at a much lower efficiency than the main targets, and will not be competitive with PFS for broader analysis of galaxy evolution.

7.3 Data Processing

7.3.1 Spectroscopic Data Reduction Pipeline

The DESI spectroscopic data reduction pipeline (DRP) is a software system that will calibrate and transform raw CCD data from the DESI spectrograph detectors into extracted spectra with classifications, redshifts, and appropriate error estimates and warning flags. The requirements for the subcomponents of this pipeline are derived entirely from the top-level requirements of redshift

success rate for survey-quality data. In order to produce redshift catalogs at the required level of accuracy and precision, the DRP will also generate high-quality instrument calibration files and one-dimensional target spectra.

The design of the DESI DRP is based on the mature and successful model of the SDSS and BOSS spectroscopic pipelines [29], with improvements and modifications as necessary to reflect technical and scientific differences between the DESI and SDSS/BOSS projects. The schematic processing flow of the DESI DRP design is illustrated in Figure 7.3. In the following subsections, we briefly describe the major steps in this pipeline, highlighting in particular the aspects that are new for DESI, as well as points at which multiple software solutions are still under consideration as a hedge against unanticipated developments in hardware design or survey operations.

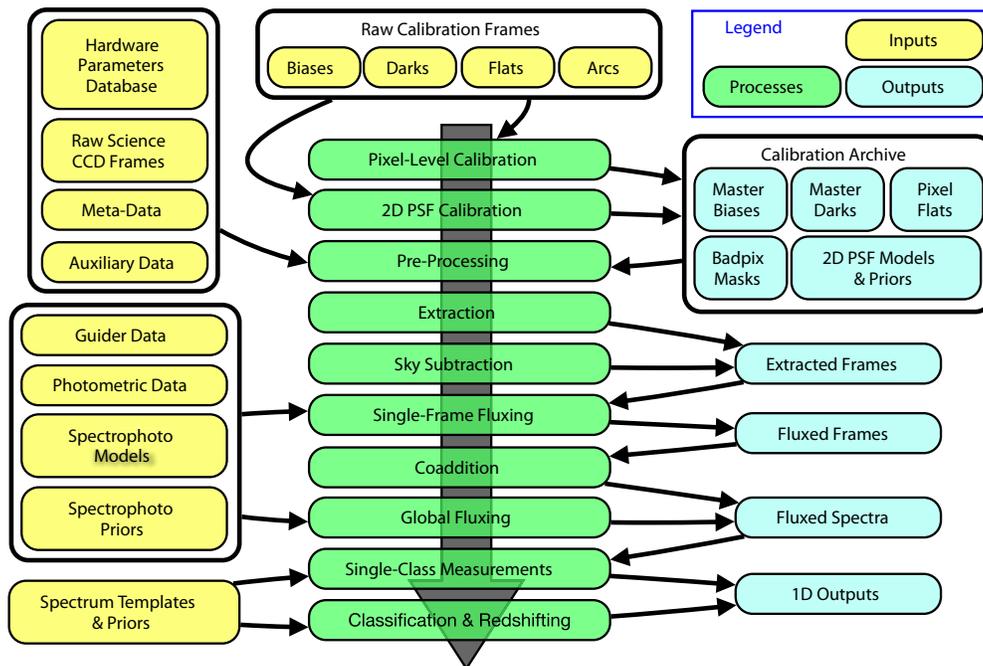


Figure 7.3: Schematic processing flow of the DESI DRP conceptual design. Successive steps receive data from previous steps either through intermediate data products or through direct API/function calls.

7.3.1.1 Pixel-level Calibration and Preprocessing

The first stage of the DESI DRP will derive and apply the necessary calibrations to the pixels of the DESI science CCD detectors. One suite of software tools and calibration data-taking procedures will be developed to enable estimation of the gains, dark currents, bias patterns, bad-pixel maps, pixel-to-pixel quantum-efficiency (QE) variations, nonlinearities, and electronic crosstalk signatures of all amplifiers on all DESI science detectors. These tools will be applied to the calibration frames, in order to develop a pixel-level calibration library that is updated with each lunation and also with every adjustment of the detector hardware itself. The details of coordination between hardware adjustment, calibration data-taking, and pixel-level calibration processing are a matter for the operations phase, but they can be greatly facilitated in the construction phase through the adoption of a calibration-product data model using a simple date-based file-naming scheme such as is currently used for BOSS.

A second set of routines will be developed to apply these bias, dark, gain, QE, crosstalk, and non-linearity corrections to individual frames, to estimate the read noise in each amplifier, to estimate inverse-variance images based on read noise and photon-count noise, and to flag bad pixels and cosmic-ray hits. The resulting corrected raw data images and their associated inverse-variance images will then be passed to the subsequent steps in the DRP. Sufficient algorithmic implementations of all aspects of pixel-level calibration are found within the BOSS pipeline, and thus the construction of this subcomponent of the DESI DRP will largely be a re-coding of existing software within a more modular Python framework. This preprocessing step is fast enough (< 1 sec) that it can always be applied directly to raw data and passed forward; it is not necessary to re-write the preprocessed data back to disk.

The lossy fiber system described in Section 5.2 will be used to measure the individual pixel response to generate “pixel flats” for raw data pre-calibration prior to spectral extraction. These calibration data and code for analyzing them are archived and distributed with the science data as part of the data management system, as described in Section 7.4.

7.3.1.2 2D PSF Calibration

The “2D PSF calibration” stage of the DRP will derive and record the calibration of the optical path between the telescope focal plane and the science CCD planes that is necessary to enable spectral extraction. This includes determination of the location of the traces of the spectra on the CCDs, the characterization of the shape of the two-dimensional PSFs of the spectrographs as they vary over their camera fields of view, the measurement of the throughput of fibers relative to one another (“flat-fielding”), and the determination of the shift of PSF centroid as a function of wavelength in each fiber. Taken together, these calibration aspects define a transfer matrix that maps input counts at the focal plane as a function of wavelength and fiber number into output illuminating counts on the plane of the DESI science CCDs, along with any charge-transfer inefficiency effects that further modify the effective PSF. The determination of these calibrations will be made on the basis of flat (incandescent) and arc (gas discharge) lamps uniformly illuminating the pupil and the focal plane of the telescope.

The spectrograph optics are very stable since they are mounted on unmoving optical benches in a temperature controlled room. These will be periodically calibrated using the continuum and arc lamp calibration system described in detail in Section 5.6. These exposures will measure the spectral trace positions, wavelength solution, and PSF shape as projected onto the CCDs.

Due to the anticipated stability of the DESI systems relative to the SDSS/BOSS systems, we plan to develop a library of 2D PSF calibration data to serve as a prior-knowledge source for routine re-calibration, and to identify the dominant modes of variation in the spectrograph transfer functions. We expect furthermore to verify and tune our 2D PSF calibrations against the optical design model of the DESI spectrographs. During the DRP construction development phase, we will implement multiple mathematical basis sets for the representation of 2D PSFs in order to have flexibility in choosing an implementation best suited to the data delivered by the as-built optical system.

A first empirical model of the 2D PSF has been developed and tested successfully against simulations of DESI arc lamp images. It uses a Gauss-Hermite basis to describe the core of the PSF, with a Lorentzian to describe its tails. The image simulations are based on a PSF model derived from the engineering design of the spectrograph, including optical aberrations, diffraction, the mean free path of NIR photons at large incidence angle, and charge diffusion in the CCD.

The 2D PSF calibration parameters determined in this stage are used to perform the extraction of science spectra from the DESI CCDs in the next stage of the DRP. We expect that our calibration

regime will determine these parameters with statistical errors that are small enough relative to noise levels in the science exposures that they can be neglected, but we will implement tracking of 2D PSF calibration-parameter noise if this proves necessary.

Pairs of Hartmann exposures on arc lamps will be used to monitor focus of the spectrographs, which is significantly more sensitive and precise than using the widths of the arc lines alone. Daily bias and dark exposures will also monitor the CCDs. These will be used by the daily spectral extraction pipeline and to monitor the overall stability and health of the spectrographs.

The primary moving part affecting DESI calibrations is the fiber system. Flexure in the fibers could affect the focal ratio degradation (FRD) losses or the near-field image at the fiber output, and thus the effective fiber throughput and PSF as projected onto the CCD. These in turn affect the PSF model and the flux calibration, and thus the ability to accurately model and subtract the sky from the science fibers. If necessary, these effects could be partially ameliorated in software by normalizing sky lines in science fibers according to the ratio of modeled flux in the model for sky background or by explicitly absorbing sky subtraction residuals with a PCA basis while fitting the galaxy and QSO templates. Alternately, if fiber flexure effects are reproducible, PSF and throughput calibrations could be performed each morning using the exact fiber positions of the exposures taken throughout the night. Ongoing lab tests and simulations seek to identify the scale of this issue and whether there are any impacts on Data Systems software.

7.3.1.3 Spectral Extraction and Sky Subtraction

This component of the DRP will extract one-dimensional background-subtracted spectra and associated noise vectors from individual preprocessed two-dimensional science CCD exposures and their associated 2D PSF calibration solutions. The spectra delivered will have units of flat-fielded counts.

The red channels of the DESI spectrographs are designed to operate at sufficiently high resolution that the free spectral range between night-sky lines is large enough to cover the necessary cosmological volume even if isolated wavelengths are compromised by sky-subtraction systematics. Realizing the fullest possible cosmological signal from the faint ELG targets of the DESI experiment nevertheless requires sky subtraction of uniformly high quality, and the DRP plan is therefore to implement spectral extraction using the “spectroperfectionism” (or 2D-PSF) algorithm of [30]. This algorithm offers the advantage of extracting the data using the actual 2D PSF of the spectrograph, avoiding the biases associated with non-separability of this PSF that can translate into sky-subtraction residuals when applying the row-by-row cross-section-based “optimal extraction” algorithm of [31]. The output spectra, noise vectors, and resolution estimates from the 2D-PSF extractions are furthermore desirable in that they deliver a closer approximation to lossless compression of the raw data [32], and can be tuned to a convenient and common wavelength baseline immediately upon extraction. Furthermore, the extracted flux samples from the 2D-PSF algorithm are free of covariance with one another.

In its most straightforward implementation, the 2D-PSF method is more computationally expensive than the row-by-row method. Work done during the R&D phase has demonstrated that 2D-PSF extraction can be implemented using an iterative extraction procedure that operates on sub-regions of the data, rendering the problem tractable at DESI scale even with today’s computing resources. For example, extraction of a single frame can be performed in about one minute on 120 nodes of a modern supercomputer, and can scale to many more nodes as needed. This implementation requires a periodic separation between adjacent fiber spectra on the detector (“bundle gaps”), and this requirement is satisfied by the spectrograph design (see Section 5.1.1).

Two implementations of the spectroperfectionism algorithm in Python and C++ using MPI

have been implemented and tested on pixel level simulations. Both provide the same output which is, for each fiber, an array of uncorrelated flux density, their variance, and a resolution matrix to convert any spectral model to the resolution of the spectrograph. Both codes allow the extraction on an arbitrary wavelength grid.

The resolution matrix is used for all subsequent reduction steps. For instance, when fitting for the average illumination spectrum for the fiber flat-fielding or when fitting for the sky spectrum, we consider a spectral model at infinite resolution, and degrade it to the resolution of each fiber individually. This is an important improvement over the existing SDSS/BOSS pipeline.

7.3.1.4 Flux Calibration and Coaddition

The DRP will perform flux calibration of the extracted and sky-subtracted DESI count spectra by matching physical stellar models to the count spectra of spectrophotometric standard stars observed during the same exposures as the primary survey targets. These matches will be used to derive the conversion vector from counts to specific flux units. Data on seeing and guiding from the guide camera may furthermore be used to correct for the differential effects of seeing and fiber sampling on extended galaxies as compared to point-like calibration stars. Flux-calibrated spectra from individual cameras and exposures will then be combined into single output spectra. The final coadded spectra will then be adjusted with low-order correction vectors to bring the synthetic photometry of standard stars and galaxies into agreement on average with available broadband photometry. This procedure is substantially similar to the methods used in BOSS currently to achieve the $\sim 5\text{--}10\%$ spectrophotometric accuracy that is sufficient to enable the application of flux-calibrated templates for classification and redshift measurement, as well as the measurement of clustering in the Ly- α forest when combined with additional quasar continuum-normalization techniques. More advanced approaches to spectrophotometric calibration for further optimization of the DESI Ly- α forest cosmology analysis will be pursued by the pipeline and Ly- α forest science working groups in collaboration during the operations phase.

A first version of the calibration and coaddition algorithms have been implemented and applied to simulated spectra of all DESI targets in 2015 (starting for CCD-level simulations). We were able to recover the input spectra at the expected statistical precision. More detailed simulations including CCD defects will be used to further test and improve the algorithms.

7.3.1.5 Classification and Redshift Measurement

The DRP will perform physical classification and redshift measurement of targets observed by DESI using the forward-modeling minimum- χ^2 template-fitting approach described in [29], with the redshift and classification reported for each object taken from the redshifted template that fits the data best from among all choices considered.

For DESI galaxy redshift measurement (both ELGs and LRGs), the DESI DRP will use a stellar population synthesis-based library of archetype spectra (possibly tuned against empirical libraries), along with emission-line components as necessary. This represents a transition from the basis of empirical PCA-derived “eigenspectra” used currently for redshift measurement in BOSS. The advantages of the archetype method over the PCA method are: a more restricted space of allowable models to disallow unphysical PCA solutions; a natural means to incorporate self-consistent photometric constraints to the spectroscopic redshift; a more fundamental wavelength zeropoint; and a clear mapping onto physical parameter measurement. The connection to physical parameter measurement will also allow us to derive self-consistent prior distributions of survey galaxies in redshift–parameter space, which can then be used to weight the likelihoods of multiple

contending χ^2 minima of classification and redshift relative to one another.

For DESI quasar redshift measurement, we also aim to generate a library of physical archetype spectra based on the combination of host galaxy light, quasar continuum, broad and narrow emission lines, blanketed iron emission lines, broad absorption lines, and a range of Ly- α forest decrements. However, since these physical components of quasar spectra are not fully understood, we will also build the DRP to support the continued use of empirical PCA-based eigenspectra, for which we will also enable the imposition of priors in PCA coefficient space to disallow unphysical linear combinations of eigenspectra. The choice of which method to implement for survey quasar redshift measurement can then be made during commissioning based on the comparison of redshift success metrics.

The DESI DRP will also need to identify stars automatically, in order to remove them from consideration within the galaxy and quasar target samples. This will require a comprehensive library of template stellar spectra. We anticipate that this library will be assembled as in [29], with an empirical set of stellar spectra supplemented by theoretical models to extend coverage across all necessary wavelengths. We will also enable the use of a library of fully theoretical stellar model spectra for testing against empirical libraries.

The galaxy, quasar, and star template libraries at the start of DESI commissioning will necessarily be based upon non-DESI sources. Over the course of commissioning, a large set of template targets will be observed in order to test and supplement these initial templates with additional spectra that span the range of all targets entering the DESI survey through any channel.

The redshift measurement and classification routines of the DESI DRP will also include methods for operating directly on collections of individual exposures rather than on coadded spectra. This approach can lead to increased redshift precision by replacing the separate nuisance-parameter sets of coaddition and redshift measurement with a single smaller set. The DRP will also include methods for identifying superposition spectra (e.g., star plus galaxy in one spectrum) that may have correct redshifts but that should be rejected from the large-scale structure analysis sample due to contaminated photometry.

Work is currently underway within the eBOSS project of SDSS-IV to implement all of the above classification and redshift measurement upgrades with a modular Python software framework that is being designed for adaptability to DESI and other future projects with minimal reconfiguration effort (“Redmonster” software: T. Hutchinson et al., in preparation). An initial version of this software has been successfully applied to simulated DESI data in 2015A. The results of this test have established the following priorities for the next phase of code development: (1) accommodating the higher (on average) and more variable spectral resolution and sampling of DESI as compared to BOSS/eBOSS, both in the processing of spectral templates and in their application to data; (2) provision for the preponderance of emission-line galaxies within DESI as compared to eBOSS, using both theoretical and empirical templates; and (3) ensuring that practical implementation within eBOSS does not compromise adaptability of the core algorithmic code to future projects such as DESI.

7.3.1.6 Progress and Quality Assurance Tracking

The DRP will automatically generate files summarizing the survey progress and quality metrics for each processed field. These will be available as plots, binary tables, and web pages for a quick assessment of the status.

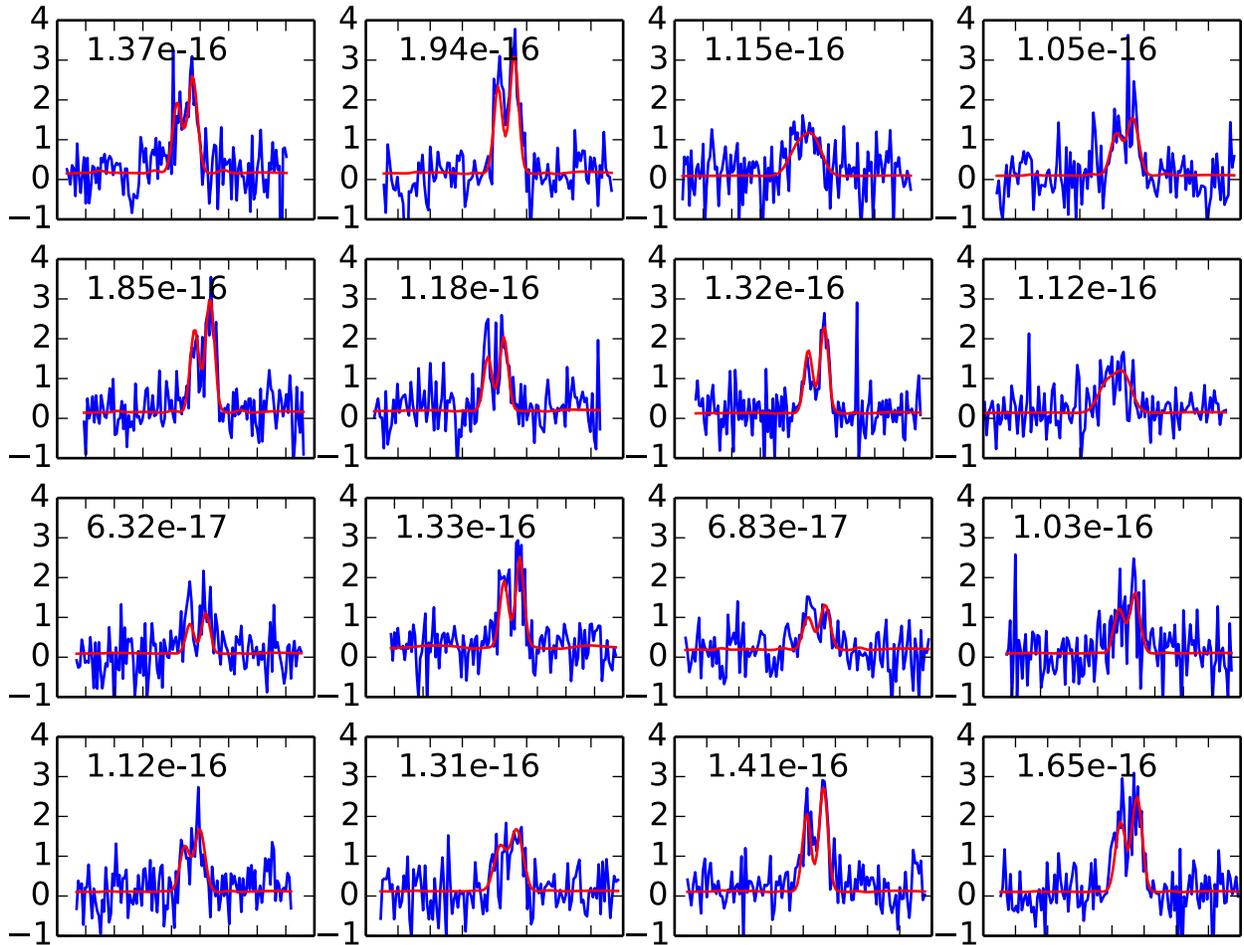


Figure 7.4: Example ELG spectra extracted by the DESI pipeline starting from pixel-level raw data simulations. The inset number is the [OII] flux in erg/s/cm^2 .

7.3.1.7 Prototype Spectroscopic Pipeline Results

Figure 7.4 shows example ELG spectra extracted and calibrated by the prototype DESI spectroscopic pipeline, starting from pixel-level raw data simulations (see Section 7.6.4.3) and proceeding through extraction, sky subtraction, flux calibration, and redshift fitting. The inset numbers are the [OII] flux; the nominal DESI flux limit is $8 \times 10^{-17} \text{ erg/s/cm}^2$ and a more typical case is $1.5 \times 10^{-16} \text{ erg/s/cm}^2$. Figure 7.5 shows results of fitting redshifts to these and additional ELG spectra. The left plot shows the fitted redshift z versus the true redshift. 1% are “catastrophic outliers” flagged with red \times symbols where the pipeline was wrong but raised no flags; this is well below the 5% requirement. The middle plot shows the redshift accuracy. The bias (10 km/s) and scatter (30 km/s) are well below the requirements (60 km/s bias and 150 km/s scatter). The right panel shows the redshift accuracy versus ELG [OII] line flux; the red vertical bar is the nominal DESI flux limit. Although these results are encouraging, we recognize that the current simulations are too clean and these metrics will get worse.

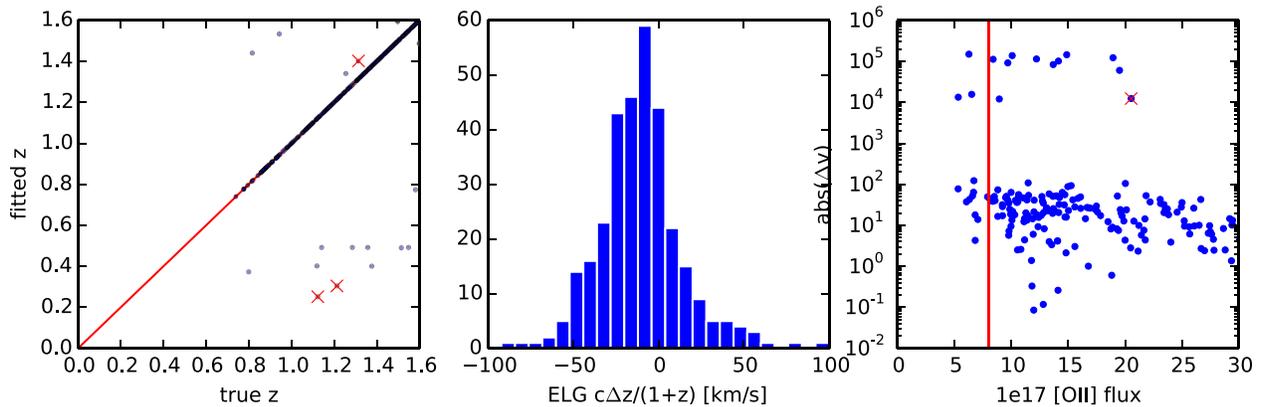


Figure 7.5: Redshift fitting results from pixel-level raw data simulations of ELGs processed with the prototype DESI spectroscopic pipeline.

7.3.2 Software Development

The DESI DRP will be a Python-based system, supplemented by calls to C/C++ code as appropriate for computationally intensive steps. Python is ideal because of its free and open-source nature, its wide and increasing adoption within physics and astronomy, the availability of mature and full-featured numerical libraries, its support for linking to compiled modules from lower-level languages, its ease of maintenance, and its facility for combining multiple coding styles (procedural, object-oriented, scripting) within a single flexible software system. All current DESI pipeline developers are already working in Python or Python/C/C++.

The primary mode of parallelization for the DESI DRP will be through an “embarrassingly parallel” mode where individual exposures or pointings are processed by individual computer cores independently of other data. Some pipeline steps are parallelized using OpenMP (C++) or multiprocessing (Python) to parallelize within a single node. The computationally intensive low-level extraction code is parallelized across multiple nodes using MPI.

The schedule for DESI DRP development, implementation, and testing consists of: an initial technical design specification phase, a core library development phase, a prototype system integration and testing phase, a full-scale testing and refinement phase, a commissioning phase coincident with DESI hardware commissioning, and an operations and maintenance phase during the course of routine survey operations. Throughout the pipeline construction process, the functioning of individual software components and integrated systems will be verified through unit and functional tests, including an automated nightly raw data through redshifts integration test for a few fibers. Higher level integration, functionality, and performance will be tested through periodic “data challenges” based on data from eBOSS, DESI simulations, and DESI spectrograph teststand data. Development and testing will be done on a range of small-scale (personal) and large-scale (e.g., NERSC) computing systems to ensure that the DRP scales and executes correctly across a range of architectures and operating systems.

All intermediate and final data products of the DESI DRP will be archived in FITS files with a documented data model. The intermediate files are anticipated to be of interest both for pipeline debugging and development, as well as for novel scientific analysis methods that need to access the data and calibrations at a lower level.

All software for DESI data processing will be managed in a version-controlled code repository. All collaborators will have access to this repository. Both internal and public data releases will be based upon tagged versions of the code, available at the same time as the data.

7.4 Data Transfer, Archive, and Distribution

7.4.1 Raw Data Transfer

Raw data will be transferred daily from KPNO via NOAO to the central data repository at NERSC. There it will be backed up to the HPSS tape storage system⁶. By retaining files at NOAO, we can maintain an additional, geographically remote copy of the raw data.

Before transfer, raw data will be compressed, and directories containing nightly data will be permission-locked so that no further data can be written. Checksum of files will be computed before transfer to insure data integrity at every stage of transfer and backup. As part of this process, the operations database will also be backed up, both in a flat file form and on a remote clone database.

Failures of the checksums at any point in this chain of steps will trigger human investigation of the problem, and recovery from the original files at KPNO.

The NOAO Data Transport System (DTS) [33, 34] is currently serving as the data transfer pipeline for the Dark Energy Survey, and we are planning to adapt it to DESI, which has much more modest transfer requirements. See Section 7.7.4 for further details of data bandwidth requirements.

7.4.2 Operational Data Archiving

In addition to the raw spectroscopic data, Data Systems will also archive operational data such as the Guide-Focus-Alignment camera output, temperature and pressure measurements, the history of commands sent to the fiber positioners, their recorded position, engineering monitoring data, and the images and analyzed data from the fiber view camera.

7.4.3 Processed Data Distribution

The DESI processing pipeline will deliver results as flat files that will be placed in a simple, transparent hierarchy. To the extent that databases are used for intermediate or final results, the database will be interchangeable with flat files, that is, one can be reconstructed from the other. Standard file types, such as FITS, will be used throughout. The directory hierarchy (which could, in principle, be spread across multiple file systems) will be visible to the collaboration through a variety of services including http, rsync and Globus Online⁷. These data access methods are already provided by NERSC.

Catalog data generated by the processing pipeline will be collected and placed into a catalog database. Catalog data will include, but will not be limited to, celestial coordinates, redshift, spectral classification (galaxy, QSO, etc.), spectral metadata (exposure date, fiber number, etc.) and targeting data. This database may also contain the full spectral data (flux versus wavelength) and associated metadata.

This database will be accessible to the collaboration through a web-based API. The specific details of this access method are still being developed. We would use the interfaces provided by the SDSS-III SAS⁸ and the SDSS-III API⁹ as a guide to developing a web-based data access method for DESI.

DESI plans to backup all reduced data to remote locations, potentially including NOAO as described above, in addition to HPSS tape storage at NERSC. We are developing tools that help

⁶<http://www.nersc.gov/systems/hpss-data-archive/>

⁷<https://www.globus.org/>

⁸<http://data.sdss3.org>

⁹<http://api.sdss3.org>

automate the HPSS backup process. The databases described above will be periodically dumped to files that can be backed up to HPSS tape storage.

Following the software development practices of SDSS/BOSS, all raw and reduced data files will have a data model that describes the content of the file. This documentation is the primary interface definition between different steps of the data processing. Automation will ensure that all raw and reduced data files conform to their data models and will also identify files that either fail to conform or that lack a data model. The data model will be both human and machine readable. SDSS currently uses HTML format; DESI is currently developing a data model based on reStructuredText¹⁰ which is more human-friendly than raw HTML but still easily processed by standard Python-based tools.

All code used for processing data will be documented using standard techniques such as Sphinx¹¹ (for Python code) or Doxygen¹² (for C/C++ code). Files will also contain metadata that points back to documentation relevant to the generation of that file, such as code name and version, the data model URL, etc. High-level documentation such as algorithm descriptions, user tutorials and technical term definitions will be managed with an off-the-shelf content management system to ensure that documenters do not get bogged down with formatting of their documentation.

7.4.4 Data Releases

Tagged versions of the processed data and associated code will be released to the DESI science collaboration approximately yearly. These will serve as the standard datasets for publications for consistency across analyses and future traceability. Additionally, the most recent reductions of the data will always be available to the entire collaboration as soon as they are processed, typically within 24 hours of observation.

After a proprietary period, these tagged data and software will also be publicly released, with the intention of producing high-quality science in a timely manner. Data releases will include software and additional documentation as needed. DESI's management policy for digital data is provided in the Project Execution Plan (DESI-0381).

Once vetted for internal (and eventually public) release, the tagged data will not be writable by the DESI collaboration. These data will be provided with checksums to verify the integrity of the data. Access to public data may involve the same methods described above, but with no password required and with access limited to public data only.

7.5 Large Scale Structure Catalog

The spectroscopic data reduction pipeline outputs classifications, redshifts, and uncertainties for each observed target. The likelihood of successfully measuring the redshift of desired targets will depend on the redshift and angular position of targets. These variations are induced by effects such as target selection under different photometric data conditions, efficiencies of the fiber assignment algorithm, and from the pipeline performance under different observation conditions. If not corrected, they will induce an artificial pattern in the distribution of observed targets and may significantly bias clustering measurements.

The Large Scale Structure Catalog code (LSScat) handles the bookkeeping for these efficiency measurements. It begins with a complete list of targets along with the results of the fiber assignment algorithm and redshift measurements. Its output is an estimate of the galaxy overdensity field as a

¹⁰<http://docutils.sourceforge.net/rst.html>

¹¹<http://sphinx-doc.org>

¹²<http://doxygen.org>

function of angular and redshift coordinates. The galaxy overdensity field is typically reported as a list of 3D galaxy positions and a set of weights assigned to each galaxy, as well as the *selection function* that quantifies the expected completeness of the survey as a function of both angular and radial coordinates, target class, and potentially other target properties. For most practical purposes, the selection function will be given as a set of “random” galaxies, where the relative density of “random” galaxies in different parts of the survey is proportional to the relative completeness of those regions.

Correlation functions or power spectra can then be straightforwardly computed through weighted pair counts of the galaxy and random catalogs. Below we detail three intermediate steps for developing the final weights, 3D selection function, and random galaxy catalogs.

7.5.1 Angular Selection Function and Angular Systematics

The angular selection function, or mask, specifies the expected number density of targets as a function of angular coordinates. This function describes the geometrical structure of the imaging and spectroscopic footprints, and requires knowledge of pertinent variations in, e.g., number of tilings, completeness, depth, and seeing across the survey. Large scale structure catalogs from many galaxy redshift surveys (including BOSS) have used the *mangle* software package¹³ for the geometrical description and related computations. *Mangle* divides the celestial sphere into regions in which conditions are relatively uniform. For instance, in BOSS these are regions within the imaging footprint covered by a unique set of spectroscopic tiles. Each region is defined by an arbitrary number of “edges” that must each be part of some circle on the sphere; see [35] for more details. In DESI (unlike BOSS) the fibers can not be put anywhere on a plate, which implies that the *mangle* regions will have to be defined at the level of fiber patrol radii. Given that DESI survey will consist of more than 50 million unique fiber locations, the number of *mangle* regions will be extremely large which makes this approach impractical.

Significant nonuniformity in the angular selection function will be present already in the targeting catalog. The nonuniformity will be generated by, e.g., variations in galactic extinction and/or stellar density, observing conditions when the imaging data was taken, or photometric calibration variations. These variations are expected to be smooth (compared to the fiber scale) and can be mitigated by a weighting function that will apply relative weights to objects in “random” catalog based on their angular positions.

Additional, purely angular, inefficiencies will be introduced at a later stage, e.g., a broken fiber or a bright star will result in an area that is effectively unobservable. These effects can be described by a veto mask that removes all targets and random galaxies in specific areas.

7.5.2 Radial Selection Function and Radial Systematics

For DESI targets, particularly ELGs, the probability of obtaining a successful redshift will depend on the observing conditions at the time the spectrum as taken (e.g., sky background), the [O II] flux of the target, and whether the redshift of the object puts the [O II] doublet inside a sky line. Redshift success rate may also be a function of location on the focal plane during observation. This information must be used to define at each point on the sky the *radial survey selection function*, which is the actual redshift distribution of the targets times the probability of obtaining a successful redshift as a function of e.g. target [O II] flux, line width, and profile, as well as the actual redshift.

¹³<http://space.mit.edu/~molly/mangle/>

7.5.3 Effects of Fiber Assignment

The fiber assignment algorithm will induce additional non-uniformity into the LSS catalogs. There are three main reasons behind this. The main source of non-uniformity is that the tiling scheme will unavoidably result in some areas of the footprint being covered by more plates than the others. The redshift measurement efficiency will be lower in the parts of the sky that are reachable by a lower number of fibers. This will induce spurious correlations on large scales (order of a DESI field). The next leading source of non-uniformity is related to DESI having multiple target types with different priority. QSOs and LRGs need multiple observations and are assigned higher priority compared to ELG targets. This implies that ELG targets are less likely to be observed in the vicinity of higher priority targets. The last source of non-uniformity is the variation in the density of targets. Since DESI fibers positions are restricted within a field, in regions with high target density some targets will not be assigned a fiber. All these sources of non-uniformity impact lower priority targets (ELGs) more than the higher priority objects (Ly- α QSOs, target QSOs, LRGs).

To mitigate the spurious signal induced by first two sources of non-uniformity we process “random” catalogs by the same fiber assignment pipeline as the target catalog. Below is a brief description of how this is done for ELG targets. We create a large number of “random” catalogs with the same average density of targets as in targeting catalog. Targets other than the ELGs are placed at exactly the same positions as in the targeting catalog. The ELGs themselves are put in such a way that they follow the observed $N(z)$ but are assigned random angular positions. These “random” catalogs are then “observed” using the same fiber assignment pipeline as for real targets. Successfully “observed” ELGs from all “random” catalogs are then concatenated into the final “random” catalog for ELG sample. This procedure naturally results in a “random” catalog in which the density of “observed” targets is higher in areas with higher density of fibers and lower in areas around higher priority targets. In the limit of large number of “random” input catalogs, this procedure is expected to completely remove non-uniformities generated by first two sources.

Figure 7.6 demonstrates how this procedure works on simulated target catalog. The blue lines show input correlation function of the simulations (first two angular multipoles). The red lines on the left panel show the correlation function computed without correcting for the fiber assignment effects. The induced spurious signal significantly distorts the signal on all scales. Red lines on the right panel show the correlation function computed after correcting for the fiber assignment effects as described above. After corrections most of the bias is removed and the measured correlation function is close to the input.

As successively more realistic models of tiling and fiber assignment are developed (see Section 7.2.1), these will be tested by running full analyses on the catalogs of “observed” galaxies generated by implementing the fiber assignment code on mock catalogs. We expect the success of this approach to be insensitive to the details of fiber assignment algorithm and tiling strategy.

A small bias remains in the correlation function even after using the “observed” randoms. This bias is likely to be coming from the fact that the efficiency of fiber assignment anti-correlates with the density of targets. This bias can be mitigated by weighting targets while calculating the correlation function, e.g. by taking all targets that haven’t been assigned fibers and up-weighting their nearest neighbors that were assigned fibers.

7.6 Simulations

Simulations are needed throughout the design, development, and operations of DESI. Some of these focus on individual aspects, e.g., to optimize a particular piece of the hardware design or to tune an individual algorithm. Other simulations provide mock data for the spectral extraction

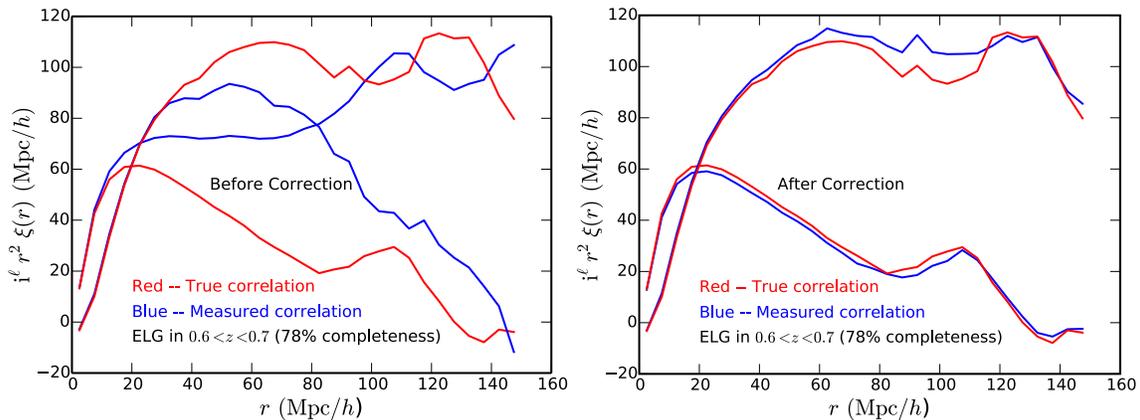


Figure 7.6: Red lines show the input correlation function (first two Legendre moments) of ELGs from N-body simulations. The blue lines on the left panel show the measured correlation function with no correction for the fiber assignment. The blue lines on the right panel show the measured correlation function after correcting for the fiber assignment as described in Sec. 7.5.3.

pipeline development prior to obtaining real data. End-to-end simulations will ensure system level integration and scaling of the software, while also validating the design performance as a whole. Cosmological simulations are needed as input for particular pieces that require realistic cosmology to test their performance. The following sections describe DESI simulations, tracing through the order of data flow.

7.6.1 Cosmological Simulations

Cosmological simulations are critical inputs for the development, testing and validation of the full DESI pipeline. In particular they are essential to

- understand the effect of the tiling and fiber assignment strategies
- model the radial selection function of the different targets for the development of the large scale structure catalog
- provide a realistically clustered mock input catalog for algorithm development
- serve as input for the end-to-end simulation pipeline for system level testing

The cosmological simulations needed to test the pipeline are a subset of the simulations needed for final science analysis, and thus the Data Systems team will coordinate with the Cosmological Simulations Working Group (and other science working groups) to obtain the simulations needed.

The cosmological simulations as needed by DESI are constructed with a multi-step procedure. First, given a cosmological model an N-body simulation is run using either baryons plus dark matter or solely dark matter. Second, galaxies and quasars are populated within this N-body simulation: Gas-hydrodynamical simulations need a way of identifying the objects, while solely dark matter simulations require a scheme such as a statistical halo occupation distribution (HOD) model or a physical semi-analytic galaxy formation model. The last step, which also depends upon how the N-body simulations are run, is the creation of a lightcone from the simulation outputs (unless created already on the fly).

The differing methods have various strengths and weaknesses. For example, HOD models can be tuned to real data distributions to accurately reproduce the clustering signal of a given population at a given cosmic epoch. On the other hand, the final DESI targeting data do not yet exist and

thus the data to tune against is not yet available. In the meantime, semi-analytic models can provide approximate predictions for samples that are either not yet defined or for which no data are available yet. Both approaches are needed for a project which aims to sample different galaxy populations at a fixed cosmic epoch.

A selection of requirements for the mocks are:

- a. the redshift space clustering of the main targets (LRGs, ELGs and QSOs) needs to be accurately recovered to enable detailed tests of the impact of the tiling and fiber assignment algorithms. In a first instance, the correct angular clustering is necessary, while the redshift space clustering as function of redshift will be important to understand any remaining biases.
- b. it will be necessary to create mocks with all three target classes covering the full redshift range of interest (i.e., $0.6 < z < 3.5$) to ensure any effects related to the tiling are properly understood, leading to a well defined angular selection function.
- c. the radial selection function of the mocks needs to match that of the targets, to ensure one can incorporate the instrumental limitations in recovering the correct redshift given the source redshift and flux.
- d. the mock galaxies need to have similar properties to the ones used to select the targets in the first place to ensure one can run the targeting selection algorithm on the mocks, like on the real data, ensuring that one can model its limitations and understand the impact photometric selections have on the sample definition and its associated clustering signal.

We envisage the need for deep spectroscopic data covering the parameter space used in the target selection to ensure we can properly model and constrain the properties of mock galaxies to be as similar as possible to the real DESI targets. The combination of galaxy formation mocks, which have a certain level of predictive power, and statistical mocks, requiring larger datasets to be trained on, is key in this process.

The final requirement on the size of the cosmological simulations is not yet set. Mass resolution of a few $10^9 M_\odot$ (and possibly as low as a few $10^8 M_\odot$) is necessary to model the LRGs, ELGs and QSOs within the same volume, while the mass resolution needed for the Ly- α forest QSO has to be several orders of magnitude higher. Creating a suite of mock catalogs of several hundred of square degrees each (i.e., much less than the full DESI footprint of $\sim 14,000 \text{ deg}^2$) ought to be sufficient to test the end-to-end simulation pipeline, including the tiling algorithm, the instrument simulations, and the target selection. Even though DESI targets are selected to be in the range $0.6 < z < 3.5$, it is imperative to have mock catalogs to $z = 0$ to ensure the target selection can be modeled in full.

Finally there is a need for a few full scale DESI specific simulations and mocks to be produced to properly test the whole pipeline, as only with the large amount of data this requires can one truly test the reliability of the end-to-end pipeline: any order of magnitude scaling cannot be assumed to work without being tested.

The cosmological simulations needed for the final science analyses will likely be of similar resolution as those described here, although of much greater size to fully cover the DESI footprint, and many more realizations will be needed to enable error estimates and cosmological parameter searches. In addition to N-body cosmological simulations focused on the galaxy broadband power spectrum, final analysis of the Ly- α forest broadband power will require large hydrodynamic simulations and quasar mock catalogs with astrophysical features such as complex quasar continua, high column density absorbers or metal absorption lines, and instrumental features such as noise, sky subtraction residuals, and errors in the spectrophotometric calibration. These final science analysis

simulations will be provided by the Cosmological Simulations Working Group in coordination with the other science working groups.

7.6.2 Operations Simulations

Section 7.2.4 describes an operations simulator for survey footprint and long term observation planning. The prototype version of this simulator currently guides survey design and will be further developed to connect input simulated targeting catalogs to simulated “as-observed” data for instrument and pipeline simulations.

7.6.3 Target Spectral Templates

Spectral templates are needed for two purposes: fitting models to the data to measure classifications and redshifts (see Section 7.3.1.5), and generating simulated data for the spectral extraction pipeline algorithm development and end-to-end tests of the DESI design.

We have developed a set of empirical ELG templates based on spectral synthesis models fitted to broad- and medium-band spectrophotometry of $\sim 20,000$ galaxies with $0.5 < z < 2$ and $r \lesssim 24$ in the COSMOS field. We have incorporated realistic variations in the emission-line ratios in the templates using spectroscopy of faint galaxies from the zCOSMOS survey. In particular, the model spectra account for the measured redshift evolution in the [O II] doublet ratio due to the differing physical conditions in the interstellar medium of intermediate-redshift galaxies. Using these 1D templates as a baseline, we are using measured rotation curves of emission-line galaxies at $z \sim 1$ observed by TKRS/DEEP2 to construct 3D spectral datacubes (2D sky position versus wavelength), in order to account for realistic variations in the emission-line center (due to galactic rotation) and line-width (i.e., velocity dispersion). With 3D datacubes in hand, we will simulate the effective 1D spectrum that each spectroscopic fiber will obtain based on the position of the target galaxy in the focal plane.

QSO templates have been developed from SDSS and BOSS observations, as well as LRG templates from BOSS ancillary data taken with DESI-like targeting requirements. These ELG, LRG, and QSO templates will be combined with the cosmological simulations described in the previous section to generate input datasets for DESI instrument and pipeline simulations.

Current studies use sky spectra measured with UVES [36]; future studies could add variations by calibrating the high-resolution UVES sky spectra to observed spectra from KPNO or alternately BOSS. Atmospheric extinction uses the widely available `knpoextinct.dat` curve from 3400 Å to 9000 Å, augmented with high resolution water absorption bands as measured at KPNO [37].

Arc and flat lamp spectra are based upon BOSS calibration lamps, deconvolved to model the arc lines as delta-functions. These allow simulation of DESI calibration data, e.g., for measuring the PSF shape and fiber-to-fiber throughput variations of simulated data.

7.6.4 Instrument Simulations

Instrument simulations guide the hardware design process and provide inputs for the spectral pipeline development. This is optimized both at the high-level to ensure that DESI meets the science requirements, and at the low-level for where the spectral extraction pipeline places requirements on the hardware design, e.g., for fiber-to-fiber cross talk and PSF stability between calibration and science exposures.

Data Systems is developing multiple levels of simulations for code development, testing, and verification; these are shown in Figure 7.7.

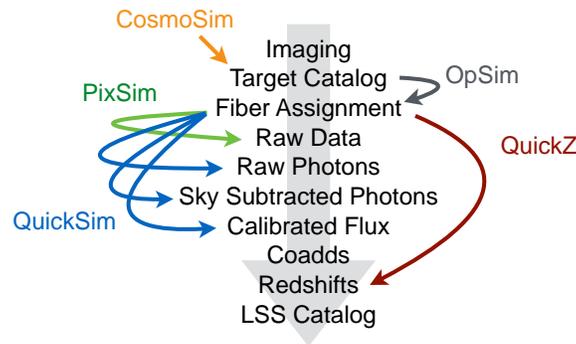


Figure 7.7: Diagram of different types of simulations under development for DESI.

- CosmoSim: input cosmology simulations to produce mock target catalogs. Exists.
- PixSim: pixel-level simulations of raw data to be used for spectroscopic pipeline development and study of detailed systematics. Exists.
- QuickSim: a fast spectral simulator that emulates the DESI spectroscopic resolution and throughput. It propagates signal, sky, and detector noise but bypasses the computationally expensive raw data pixel simulations and extractions. Exists.
- OpSim: a survey simulator that traces what tiles would be observed in what order based upon the real next field selector and a Monte Carlo realization of weather and observing conditions. Planned.
- QuickZ: an ultra fast simulator that applies DESI efficiencies to an input target catalog to generate an output redshift catalog. Planned in conjunction with the science collaboration using tools provided by Data Systems.

CosmoSim has been used for fiber assignment algorithm development. QuickSim was used for the majority of the performance studies in this report. PixSim has been used for spectroscopic pipeline development and Figures 7.4 and 7.5; we are in progress with calibrating/verifying QuickSim versus PixSim.

Hardware simulations are based upon a throughput budget provided by systems engineering and a spectrograph point-spread-function (PSF) model provided by the spectrograph engineering team. The PSF is simulated using Zemax ray traces of the input fiber illumination pattern at the slit, plus diffraction and CCD detector absorption effects. These are modeled on a grid of wavelengths and fiber slit positions and then interpolated to arbitrary wavelengths and fibers. Figure 7.8 show these spots on a log color scale for a 980 nm monochromatic illumination of fiber 0 on a 500 μm thick CCD, which is the worst case for PSF distortion. The various panels show different contributions to the PSF covering a size of 15×15 CCD pixels; the bottom right spot is the final spot used for simulations. Equivalent spots are generated for 10 other fiber positions and 32 other wavelengths¹⁴.

In addition to these simulations, the DESI algorithms are written in a modular fashion so that they can also be applied to real BOSS data. This provides a valuable cross check on the performance of these algorithms in the presence of data quality issues that arise in real data. That also guides areas where the DESI simulations need to improve to be more realistic.

¹⁴Finer grids are possible if needed.

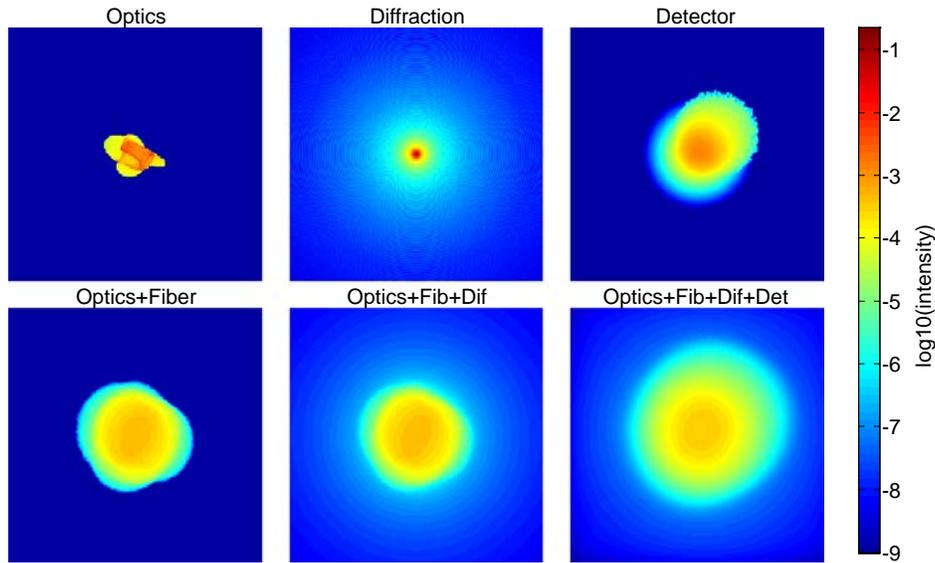


Figure 7.8: Simulated spectrograph PSF spots including various effects. Top row left to right: infinitesimally small fiber for optics only, diffraction only, detector only. Bottom row left to right: $107\ \mu\text{m}$ fiber for optics only, optics and diffraction, and optics and diffraction and detector. Each spot covers 15×15 CCD pixels. Note that these are on a log color scale.

7.6.4.1 desimodel

DESI hardware and operations parameters used by the simulations are stored in machine readable formats in the “desimodel” product of the DESI code repository. Tagged versions of desimodel provide unambiguous descriptions of each reference DESI design.

The hardware parameters include the throughput, PSF model, Mayall mirror geometric area, CCD dimensions, focal plane positioner layout, plate scale, and fiber size. These have documented traceability back to DocDB entries for details. In addition to hardware parameters (Section 1.4), desimodel includes survey parameters such as median seeing, sky emission and extinction spectra, default exposure time, reference spectra for each target class, and dn/dz distributions expected from targeting. All parameters necessary to simulate the reference DESI mission are contained in desimodel.

Ownership of each class of parameters is coordinated: systems engineering controls the hardware parameters; data systems controls the astrophysical quantities such as the impact of seeing, night sky brightness, and extinction; and the science collaboration provides reference spectra and targeting dn/dz distributions.

7.6.4.2 Quicksim

Quicksim code included in desimodel simulates the S/N properties of DESI spectra assuming error propagation of photon shot noise plus CCD readout noise. It goes directly from an input spectrum to a resolution-convolved output spectrum plus noise. It treats the PSF dispersion as Gaussian in the wavelength direction, and parameterizes the effective number of pixels affected by CCD readout noise using the true cross-dispersion shape of the PSF for fiber 100 (which is neither the best nor the worst PSF fiber). Quicksim is available in both IDL and Python versions for end-user flexibility.

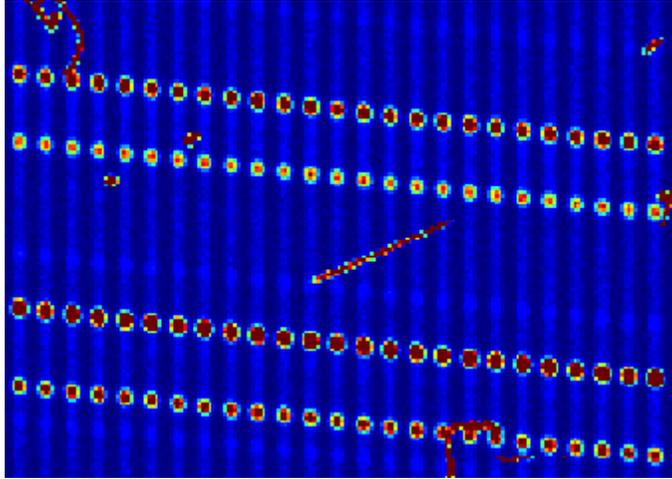


Figure 7.9: Example CCD pixel-level simulation of 25 sky spectra, including CCD readout noise and cosmic rays superimposed from real data. This is approximately 1/1500 of the data from a single DESI exposure.

7.6.4.3 Specter Pixel-Level Simulations

Detailed pixel-level simulations use the Specter toolkit¹⁵, with a DESI-specific wrapper in desisim¹⁶. It simulates all 500 fibers per CCD and generates raw data frames mimicking DESI raw data, including fiber-to-fiber cross talk, PSF distortions at the edges of the CCDs, and cosmic rays. A subset of a single simulated frame is shown in Figure 7.9. Specter provides inputs for spectral pipeline development and enables studies of systematics not addressed by QuickSim, e.g. fiber-to-fiber cross talk, PSF stability, multi-fiber sky subtraction, and calibration requirements. Specter will also be used to generate a full survey of simulated raw data to perform end-to-end data challenges. Since Specter is much slower than QuickSim, it will be used only for studies that require pixel-level detail.

7.6.5 DESI Oerformance Studies

7.6.5.1 ELG Signal-to-Noise

Figure 7.10 shows the quicksim output of a 1000 second exposure at zenith with 1.1 arcsec seeing and no galactic dust extinction. These conditions define a “reference” exposure S/N. Actual observations will be longer or shorter to achieve this same S/N given the current conditions (see Section 7.2.3). This ELG is at $z = 1.189$ where the [O II] doublet is between sky lines; The nearest sky line is a faint line at 8105 Å.

The top plot shows a limiting flux case of $F([\text{O II}]) = 0.8 \times 10^{-16} \text{ ergs s}^{-1} \text{ cm}^{-2}$ with a binning of 0.6 Å corresponding to the typical CCD pixel size in the NIR arm of the spectrograph. Although the spectrum is noisy, this is a 7σ detection, as defined by the significance of the [O II] doublet amplitude derived from an optimal fit using known line profiles and flux ratio. The bottom plot of Figure 7.10 shows the median flux case of $F([\text{O II}]) = 1.4 \times 10^{-16} \text{ ergs s}^{-1} \text{ cm}^{-2}$ with a 11.8 σ detection.

To accurately predict the fraction of targeted ELGs that will have high-confidence redshifts, we must understand the DESI redshift detection efficiency versus redshift and [O II] flux. Figure 7.11

¹⁵<https://github.com/desihub/specter/>

¹⁶<https://github.com/desihub/desisim/>

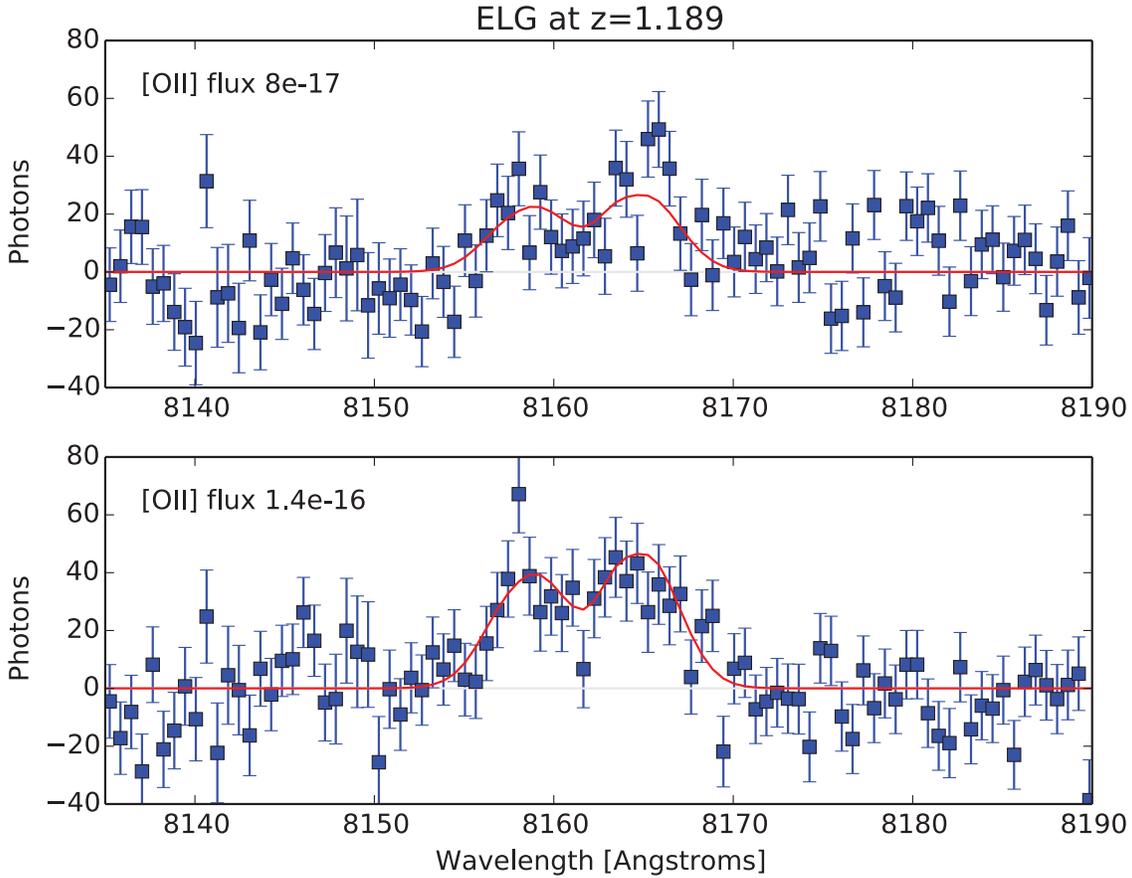


Figure 7.10: A quicksim simulation of the [O II] emission line doublet at a limiting flux of $F([\text{O II}])=0.8 \times 10^{-16}$ ergs $\text{s}^{-1} \text{cm}^{-2}$ (top) and the median case of $F([\text{O II}])=1.4 \times 10^{-16}$ ergs $\text{s}^{-1} \text{cm}^{-2}$ (bottom) for a reference 1000 second exposure. The simulated emission lines have a velocity width of 70 km/s and a ratio of 1 : 1.3. The red curves represent the input spectra at the resolution of the instrument (expected number of collected photons per pixel row), and the blue squares a random realization of the data with noise.

shows the emission line S/N for a 1000 second reference exposure of an $F([\text{O II}])=8 \times 10^{-17}$ ergs $\text{s}^{-1} \text{cm}^{-2}$ ELG template spectrum. This spectrum is redshifted in $\Delta z=0.001$ increments over the full DESI spectral range. The S/N for other [O II] fluxes is scaled from this example as described in the following section.

The template spectrum uses constant emission line flux ratios relative to $F([\text{O II}])$, with a velocity dispersion of 70 km s^{-1} . The template [O II] doublet line ratio is 1:1.37, and the other line ratios are $[\text{O II}]/\text{H}\beta=2.5$, $[\text{O III}] (5007 \text{ \AA})/\text{H}\beta=1.6$, $[\text{O III}] (5007 \text{ \AA})/[\text{O III}] (4959 \text{ \AA})=2.984$ and $\text{H}\alpha/\text{H}\beta=3$.

For $z < 0.5$, the combined S/N from all emission lines is strongly enhanced by the presence of $\text{H}\alpha$. Between $0.5 < z < 1.0$, $\text{H}\alpha$ is redshifted beyond $\lambda > 9800 \text{ \AA}$ and a redshift must be measured from a combination of $\text{H}\beta$, [O III], and [O II]. The [O II] doublet will be the only emission line available for redshift measurement beyond $z > 1$, therefore requiring that the doublet is resolved for an unambiguous two-line identification in this redshift range. $\text{S/N} > 7$, shown in the blue dashed line, ensures that the line is unambiguously detected as an [O II] doublet and not a mis-identified single line. Note that the change of sensitivity to the [O II] doublet with redshift for $z < 0.3$ is principally due to the change of the spectrograph throughput with wavelength below $\lambda < 5000 \text{ \AA}$,

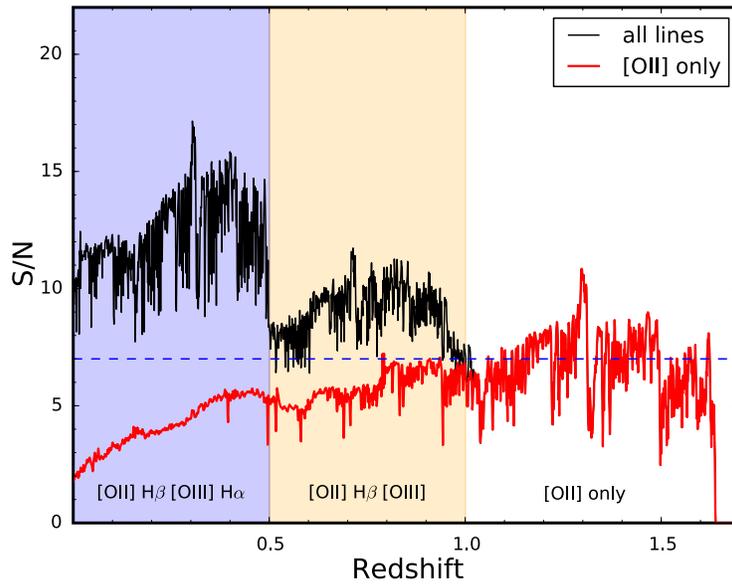


Figure 7.11: The emission line S/N assuming constant line ratios for $F([\text{O II}])=8 \times 10^{-17}$ ergs $\text{s}^{-1} \text{cm}^{-2}$ across the full DESI redshift range for a reference 1000 second exposure. The black line shows the combined S/N from all emission lines observable in the waveband, while the red line shows the S/N only from [O II]. The horizontal blue dashed line shows $S/N > 7$ where DESI achieves an unambiguous [O II] detection.

see Figure 5.15.

7.6.5.2 Redshift Success Rates

A robust estimate of the success rate versus redshift and [O II] flux can be derived from Figure 7.11 because the noise is largely dominated by the sky Poisson noise (with a small contribution of readout noise). Requiring $S/N > 7$ translates into a [O II] flux limit shown in Figure 7.12. For galaxies above this limit, we can safely assume a high redshift success rate of 95%. The conservative 5% inefficiency accounting for CCD defects and cosmic ray hits at the CCD location of the emission lines. This flux limit is used in Target Selection section of the Science TDR to derive a redshift efficiency given an input ELG target selection catalog, and is the basis of the dN/dz distributions used for the cosmology projections in the Science TDR.

7.6.5.3 Trade Studies

In developing a conceptual design for the DESI experiment, it is necessary to perform trade studies around the baseline instrument design and observation plan during the R&D phase. Ultimately, the scientific impact of these design decisions must be quantified in a useful metric such as the FoM described by the Dark Energy Task Force [1]. In the case of DESI ELGs, we can use the above simulations to evaluate the change of redshift success rate with S/N threshold, exposure time, sky brightness, the fraction of light from the target galaxy collected in the fiber, CCD readout noise and number of exposures (which increases the contribution of readout noise). The results are shown in Figure 7.13. This study is based on a distribution of ELG [O II] fluxes as a function of redshift consistent with the selection presented in the Target Selection section of the Science TDR. Assuming uncorrelated uncertainties of 10% on the system throughput (equivalent to a change of exposure time), the sky brightness, and the fraction of galaxy light collected in the fibers results in

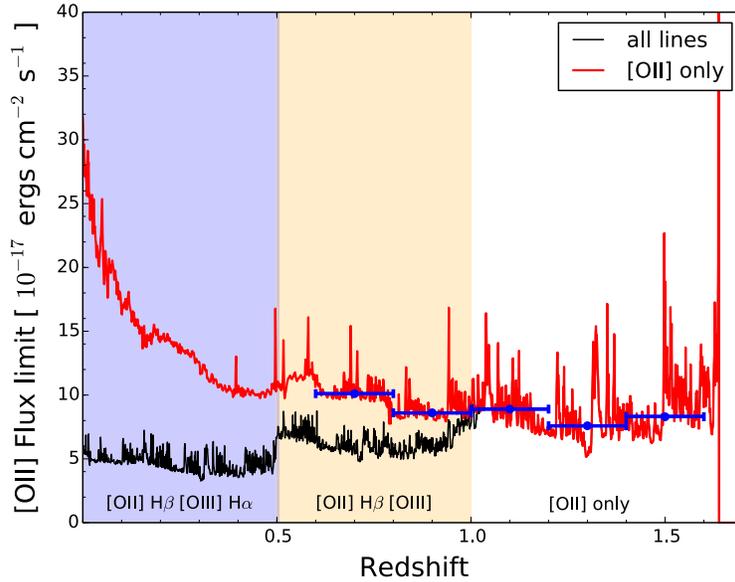


Figure 7.12: [OII] flux limit for a $S/N > 7$ detection of the [OII] doublet only (red curve) or a combination of emission lines (black curve) vs redshift for a reference 1000 second exposure (a single exposure), at zenith, without Milky Way dust extinction. We have assumed here a fixed line ratio between the [OII] doublet and the other lines. The blue points show the binned median of the red curve.

an uncertainty of only 4% on the redshift success rate for ELGs. This is a consequence of the fact that most targets are significantly brighter than the flux limit defined above.

7.6.6 DESI End-to-End Survey Simulations

End-to-end simulations provide a system-level integration test of the survey plan and data reduction software, as well as a method to test for system-level systematics [39, 40]. Examples of such systematics include coupling between tiling, fiber allocation, and source clustering; or between targeting color selection, photometric calibration, and final source populations. Simulating and testing these effects ahead of time enables optimization of the algorithms and verification of the science goals given the “as-designed” hardware and “as-built” software. End-to-end simulations have also been used by other cosmology experiments such as LSST [41] and CMB experiments.

We expect end-to-end simulations to be used throughout the life cycle of DESI. At early stages, they will be used to optimize the instrument and survey strategy. On intermediate time scales they will be used to demonstrate the feasibility of the baseline design, to shape the development of the DESI data management system, and to test its scaling performance prior to first light. During the operations phase, they will be important for the science exploitation of the data as a tool to control systematics.

Final end-to-end simulations will use the actual DESI data systems components, inserting simulated data as if they were real data. A cosmology simulation will provide a simulated targeting catalog, upon which the real fiber assignment code is run using the same file formats and interfaces as the final real data. The operations simulator will simulate observing conditions and select tiles using the real next field selector. We will use these to generate pixel-level raw data simulations that the data reduction pipeline will process without knowing that they are simulations. This tests both the scaling and integrity of the data flow, with the final BAO analysis testing the software

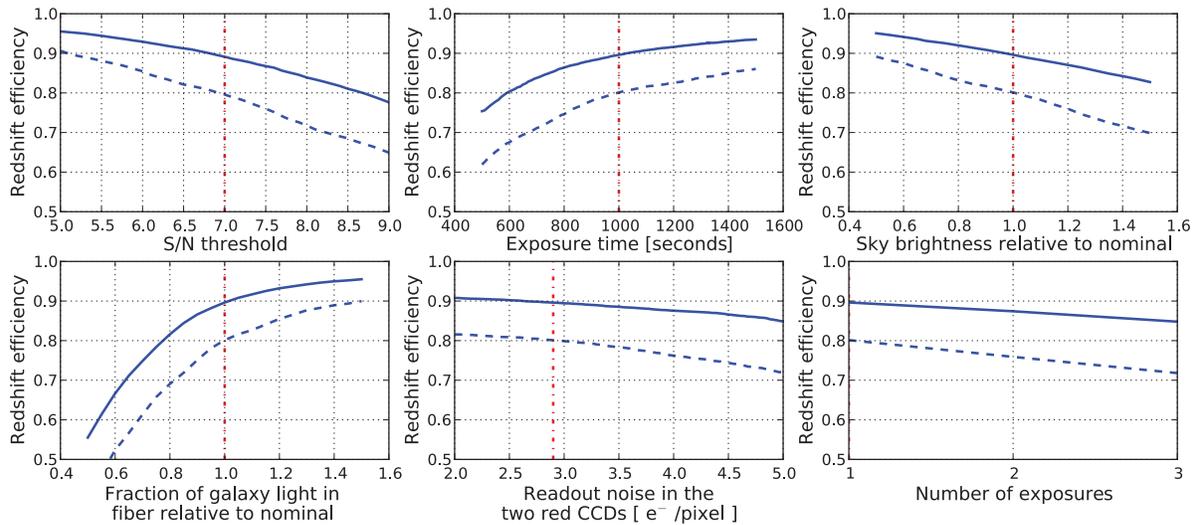


Figure 7.13: Redshift success rate for ELGs as a function of S/N threshold, exposure time, sky brightness, fraction of galaxy light collected in the fibers, readout noise and number of exposures. The distribution of ELGs as a function of redshift and [O II] flux follows that described in the Target Selection section of the Science TDR. The solid curve is the efficiency when all emission lines are used, and the dashed curve when only the [O II] doublet is considered. The vertical red dashed-dotted lines are the nominal values. In this plot, we do not include the 5% provisional inefficiency related to CCD defects and cosmic rays mentioned in the text.

“as-built” performance. A subset of these data will be used to test the data transfer system and its connection to automatically launching data processing as data arrive at NERSC.

A data challenge approximately a year before first light will focus on end-to-end integration. This provides time to address any integration issues that arise during the end-to-end tests.

7.7 Computing Requirements

There are several distinct activities within the DESI project that have substantial computing requirements, notably target selection in the near term, full survey simulations in the mid-term, and the data reduction pipeline during survey operations. Tables 7.3, 7.4, and 7.5 provide an overview of these by year, split by disk storage, data transfer, and computation requirements. These include computing requirements beyond the timescale of DESI construction since one requirement of DESI Data Systems is that it will be viable to run on available NERSC resources during the years of operation.

CPU usage for data processing will be provided through NERSC allocations, i.e., with no direct cost to the DESI project. Similarly, input simulations will use allocations at NERSC, other DOE leadership class facilities, or at computing centers provided by collaborating institutions. Disk space, however, will be purchased at NERSC to support these activities. The budget for this disk space is detailed in a spreadsheet in DocDB (DESI-0738).

Here we describe the requirements by activity. All processing requirements are described in circa 2012 CPU core hours. In the next 1–2 years, NERSC will transition to a many-core Intel architecture, with ≥ 60 cores per node. Although such systems will have an ever-increasing theoretical peak number of flops, actually leveraging those new architectures will require some work. Fortunately, processing of the full DESI dataset can be parallelized both at the task level (extracting the spectra from many exposures) and within a task (extracting smaller groups of fibers over a reduced

Table 7.3: Cumulative data volume in terabytes used by the DESI project by fiscal year. **Note:** these fiscal years assume current schedule predictions. All of this data is archived to tape (HPSS) and kept on disk. These numbers do not include science analyses.

Activity	FY15	FY16	FY17	FY18	FY19	FY20	FY21	FY22	FY23
Targeting – WISE	68	95	121	121	121	121	121	121	121
Targeting – DECam ¹	175	263	351	351	351	351	351	351	351
Targeting – Mosaic ¹	0	47	94	94	94	94	94	94	94
Targeting – Bok ¹	23	47	70	70	70	70	70	70	70
Targeting – ZTF ¹	0	0	47	47	47	47	47	47	47
Instrument Sims ²	0	15	150	150	150	150	150	150	150
Cosmology Sims ³	10	10	10	10	10	10	10	10	10
DESI Data ⁴	38	77	115	232	349	465	582	698	815
Science Collaboration ⁵	100	300	500	1000	2000	3000	4000	5000	5000
Total	414	854	1458	2075	3192	4308	5425	6541	6658

(1) Assumes reduced data is factor of 4 larger than raw data, and includes additional 1/6 of total for reprocessing workspace.

(2) 2017 is the full, 5-year survey simulation and processing.

(3) This is the space for one cosmology simulation needed for instrument simulations.

(4) This is raw data plus two copies of reduced data at any given time. Includes data from early spectrograph testing.

(5) Needed for science analysis, and budgeted separately.

Table 7.4: Data transfer requirements in terabytes for the DESI project by fiscal year. **Note:** these fiscal years assume current schedule predictions. These numbers are the total volume of data moved in each year. The instrument simulations and target catalogs will be generated at NERSC and do not need to be moved. The cosmology simulations may be generated at the DOE Leadership Class Facilities, and this is included below. The numbers for data processing represent the raw data transfer from KPNO. Data distribution from NERSC to the collaboration assumes one major data release per year and is based on network statistics from BOSS.

Activity	FY15	FY16	FY17	FY18	FY19	FY20	FY21	FY22	FY23
Targeting – WISE	80	0	0	0	0	0	0	0	0
Targeting – DECam	55	55	55	55	0	0	0	0	0
Targeting – Mosaic	0	8	8	0	0	0	0	0	0
Targeting – Bok	4	4	4	0	0	0	0	0	0
Targeting – ZTF	0	0	27	0	0	0	0	0	0
Cosmology Sims	30	30	30	30	30	30	30	30	30
DESI Data to NERSC	0	0	0	6	6	6	6	6	6
DESI Data serving	0	0	0	100	100	100	100	100	100
Total	169	97	124	191	136	136	136	136	136

wavelength range for a single exposure). In our development of software tools and algorithms we will strive to build this parallelism into our design, in order to use these systems effectively.

7.7.1 Target Selection

See the Target Selection section of the Science TDR for a discussion of the process of selecting targets for spectroscopy by DESI. In order to perform the target selection in the years leading up to the beginning of observations, we must transfer substantial amounts of data from other locations to NERSC. At NERSC, we use simultaneous astrometric and photometric measurements across multiple targeting datasets to identify and select objects. This analysis will dominate the

Table 7.5: Computational requirements of project activities by fiscal year, given in millions of 2012 CPU-hours. **Note: these fiscal years assume current schedule predictions.**

Activity	FY15	FY16	FY17	FY18	FY19	FY20	FY21	FY22	FY23
Targeting ¹	3.6	7.2	9.6	12	10	10	10	10	10
Instrument Sims ²	2.3	2.3	45	2.3	2.3	2.3	2.3	2.3	2.3
Cosmology Sims ³	2	2	2	4	4	4	4	4	4
Data Processing ⁴	0	0	0	18	36	54	72	90	108
Science Collaboration ⁵	5	5	5	10	20	20	30	40	50
Total	12.9	16.5	61.6	46.3	72.3	90.3	118.3	146	174

(1) Assumes running Tractor on all targetting data 4 times per year until survey start, and then performing Monte Carlo analyses on the target selection.

(2) In 2017 we simulate and analyze a full 5 year survey.

(3) This is only the cosmology simulation to support the project needs, not science analysis. One per year until survey start, then two per year.

(4) Assumes 3 reprocessings per year.

(5) Needed for science analysis.

disk space usage prior to the start of the survey, and will use moderate levels of CPU time as detailed below.

The primary instruments that will be used for DESI target selection are the Wide-field Infrared Survey Explorer (WISE), the Dark Energy Camera (DECam) on the Blanco telescope, and the Bok telescope and Mosaic imager on Kitt Peak. In addition, data from other facilities such as SDSS, the Canada France Hawaii Telescope (CFHT), and the Zwicky Transient Factory (ZTF) may be used to supplement target selection. Network transfers of the raw data from these instruments to NERSC is well within current capabilities. In addition to the uncompressed raw data, we must also compute and store derived products (reduced images, image stacks, catalogs, etc) needed for target selection. We store the raw and reduced data on disk as well as archiving it to tape storage. We additionally use a small amount of disk space for testing the data reduction techniques. Detailed yearly totals for both network use and disk space are given in Tables 7.3 and 7.4.

The dominant computational cost of target selection is the process of extracting catalogs from combined datasets (see the Tractor section of the Science TDR). We estimate that a full target selection run (using all data) will be performed four times a year as part of the development for the data releases 1–2 times per year. Based on production Tractor runs with imaging data covering 12% of the DESI footprint, we can extrapolate the future CPU usage in Table 7.5.

7.7.2 Cosmological Simulations

N-body and hydrodynamical simulations are needed as inputs for developing the algorithms for tiling, fiber assignment, and large scale structure catalog generation since each of these steps impacts the systematics of the measured cosmology. The numbers given below are for a single realization of the simulated sky; many tests could be performed with a much smaller simulated area. Final science analyses will require many such realizations, but that is under the purview of the science collaborations and is not scoped here.

For both N-body and hydrodynamic simulations, the low-level (“level-1”) data outputs are stored on the computer where they were generated (for example, the DOE Leadership Class Facilities or the machine-specific scratch disk at NERSC). We do not transfer the level-1 data, and instead produce “level-2” data products which can be transferred to the NERSC global filesystem for further work. This level-2 data consists of the mock DESI galaxies and approximately 40 snap-

shots of halo data needed to construct those mocks. The total size of these items is approximately 10 TB. Performing one N-body simulation and constructing the mocks is estimated to require 2M CPU hours. We anticipate creating the first such simulation early in the project, to enable rapid use for pipeline development. The CPU requirements in Table 7.5 reflect the likely need to generate one such simulation per year (to incorporate new features or fix bugs) in the years leading up to the full survey data challenge. Only one such simulation is required to be stored on project disk at any given time; previous simulations may be staged from tape to scratch disk as needed.

7.7.3 Instrument Simulations

Pixel level instrument simulations are used to develop the hardware design and generate simulated data for the spectroscopic data reduction pipeline; see Sections 7.6.4 through 7.6.6. Current full CCD pixel-level simulations require 450 CPU hours per DESI exposure to generate 30 CCD frames with 5,000 spectra. Generating a full exposure requires constructing a PSF from a realization of the instrument model (using a nominal model plus fluctuations within the design tolerance), using that PSF to project a set of simulated spectra onto the CCD, and adding realistic noise and other artifacts. If we chose a fixed PSF across many exposures, we could reduce the computational cost of the simulation in exchange for less realism. In addition to the full survey data challenge (see below), we anticipate needing a couple million (circa 2012) CPU hours per year for smaller testing campaigns of specific features of the simulation and extraction tools. This estimate is based on current experiences testing these tools on BOSS and simulated DESI data. These test campaigns will generate 10–50 TB of data. Because instrument simulations are generated and analyzed on the machines at NERSC (which all share a common filesystem), no data transfers are needed for this activity.

A full survey data challenge in late 2017 will verify the full Data Systems chain and guide the development work for the final year before first light. This data challenge will begin with mock targeting catalogs and proceed through simulations of the observing strategy, field selection, and fiber assignment. These will be used to generate a full survey of simulated pixel-level data that will flow through the data transfer and archive system and be analyzed by the data reduction pipeline as if it were real data. A large scale structure catalog will be produced from these simulations and the power spectrum / correlation function will be analyzed, thus ensuring the complete bookkeeping chain from targeting through science analysis.

Since this is a full-sized dataset, processing it will require the computational resources outlined in Section 7.7.4, as well as the resources required to simulate images from the input catalogs and fiber allocation methods.

7.7.4 Spectroscopic Data Processing

Raw data are transferred daily from KPNO to NERSC via NOAO in Tucson. Copies of the raw data will be archived at both NOAO and NERSC to provide geographically separate backups. At NERSC the data is preprocessed, calibrated and made available to software which performs spectral extraction and redshift determination. The output data products are hosted and served to the science collaboration through the NERSC science gateways.

When estimating the size of the Raw data, there are several possible ways of computing the data volume per year. Three such calculations can be found in the spreadsheet documenting computing resources by year (DESI-0738). The final estimate we use is based on the scaling of compressed BOSS raw data volumes (by 30 versus 4 CCD frames per exposure), plus a margin to allow for uncertainty in the number of daily calibration images and the data compression factor. This gives

us 10 TB/year of raw data, plus an additional 0.6 TB/year of auxiliary data from acquisition and guiding.

BOSS spectral extractions result in 2.5 times more extracted data than raw data volume. DESI spectra will be similar, with the addition of the “resolution matrix” to encode the spectral resolution. A naive encoding of this matrix would be quite large, but we anticipate that a sufficiently accurate parameterization will result in extracted data being 5 times larger than raw data, i.e., 50 TB per year. While modestly large by current standards, this will be a trivial amount of disk space by the start of the DESI survey.

The network link from KPNO is large enough to enable data transfers in real time as soon as the data are taken. The computing systems at KPNO will have sufficient disk storage to cache at least one week of raw data in the case of significant network outages or delays in data transfer. After processing, calibrated images and spectral domain products are served from NERSC to the rest of the collaboration. This processed data is also backed up to NOAO. Based on experience serving BOSS reduced data, we anticipate serving $\mathcal{O}(100 \text{ TB})$ of data per year to the DESI science collaboration.

Constructing the PSF from calibration images will require about two CPU-hours per CCD frame. Assuming three re-calibrations per day, this amounts to less than 100,000 CPU-hours per year total. Our baseline spectral extraction software splits the spectra by independent “bundles” of fibers on the CCD and overlapping wavelength regions which are then reassembled to avoid edge effects when extracting sub-regions. Current development code for spectral extraction can extract a single DESI frame with about 15 (circa 2012) CPU hours. If we assume that we have 20 minute exposures and that we have 221 nights of observing with an average of 10 hours per night, this gives us about 6630 exposures per year. At 30 frames per exposure, this is approximately 200,000 frames per year of science data. We assume an additional factor of two for calibration images, which gives us 400,000 frames and a total of six million CPU hours per year of survey data to do the extractions. Based upon BOSS redshift fitting code, we expect classifications and redshifts to take less than 100k CPU-hours per year of DESI data.

Allowing for 3 full reprocessings of all data per year, we obtain the CPU hour estimates summarized in Table 7.5. While fairly large by current computing standards, these should be quite manageable by the start of DESI.

7.7.5 Science Analysis for Cosmology

The DESI science collaboration will coordinate a broad research program in Cosmology and this is described in detail in Part 1 of the Technical Design Report. This effort will require substantial computing resources in the form of CPU hours and disk space. The CPU hours will be provided by standard NERSC allocations, and the disk space is budgeted separately from the DESI project costs. We include these required resources in tables 7.3 and 7.5 in order to give a more complete picture of our requirements.

The needed disk and computing resources are dominated by the generation, storage, and analysis of mock catalogs and their parent simulations, more so than the actual DESI data. These mock catalogs are critical for the control of systematic errors at the level of DESI precision, and analyses such as for neutrino masses and modified gravity require connection to the underlying dark matter and gas distributions. Typically, one uses hundreds to thousands of mock catalogs, for dozens of choices of control parameters, and then repeated several times through the life of the survey. While the underlying cosmological simulations will be run with other computing allocations, storing suitable data products and then analyzing them is the responsibility of the DESI collaboration. Even retaining simplified and subsampled data products for hundreds to thousands of simulations

adds up to PBs of data.

7.7.6 Computing Requirements Summary

Data transfer volume is well within the current capabilities of ESNET and is not expected to be a problem. CPU requirements are large but not intractable, dominated by processing the full survey data challenge in 2017 and the final reprocessings of the entire dataset at the end of the survey. Disk space requirements for targeting data will likely be the most expensive piece of hardware computing since it is both large and needed prior to commencing the survey. Thus overall, the computing requirements are large but entirely manageable. The tables below are a summary of the spreadsheet in DESI-0738.

7.8 Collaboration Tools

We have developed an Integrated Collaboration Environment system based on Trac¹⁷ software. Trac provides a wiki, source code browser, bug tracking system, timeline and milestone tracking, and basic search facilities. We have further integrated Trac with a set of mailing lists, based on GNU Mailman¹⁸. This integration allows mailing lists to be searched from within the Trac environment.

The DESI version-controlled code repositories are based on Subversion¹⁹. Membership in the DESI Trac also grants access to our Subversion repositories. This feature allows DESI collaborators to immediately access DESI code without additional sign-ups or requests. In addition, we are developing open-source software in the `desihub` group on GitHub²⁰.

Document Control is based on DocDB²¹, which we have already begun to integrate with Trac. Because Trac is highly extensible through plugins, we expect to make further developments in DocDB-Trac integration. Similar to how we have integrated Trac and Subversion access, DocDB access is also connected to a Trac account.

The Integrated Collaboration Environment is backed up daily to a server at the University of Utah. This backup can be activated quickly in the case of a temporary or catastrophic loss of the primary site.

We are developing a public website for DESI based on WordPress²². This can serve as the basis for public outreach and documentation of our public data releases (see also Section 7.4).

We will provide a system for announcing projects and publications similar to a system used by SDSS-III. This allows the entire collaboration to be informed of projects and working groups that may be of interest. The announcement of publications facilitates collaboration-wide review of papers written using DESI data.

¹⁷<http://trac.edgewall.org>

¹⁸<http://www.gnu.org/software/mailman/>

¹⁹<http://subversion.apache.org/>

²⁰<https://github.com/desihub>

²¹<http://docdb.fnal.gov/doc/>

²²<http://wordpress.org>

8 Integration and Test

The DESI instrument will consist of numerous separate elements supplied by distinct and distant collaborators, all finally coming together at the Mayall Telescope. Comprehensive planning and management of integration and testing activities, of interfaces between elements, and of preparation of the Mayall Telescope for the installation of DESI will be crucial to project success. The Level 2 Integration and Test Managers are primarily responsible for these activities. In addition, the DESI Project Engineer will be engaged in integration and test planning and strategy.

Periodic workshops dedicated to integration and test planning will be held with the collaborating institutions to involve them in the planning and execution of the integration, interfacing, and testing tasks they will be party to. The first of these workshops was the initial meeting of the Installation and Commissioning Task Force (ICTF) during April 2014 at Kitt Peak and NOAO Headquarters in Tucson. That meeting raised previously unidentified issues and yielded a number of Action Items (all identified, tracked and responses referenced in DESI-0781), each of which addresses an integration question or issue. An ICTF Report (DESI-0776), referencing those issues and actions, has been published.

This section describes Integration and Test all the way through installation and functional verification of DESI on the Mayall telescope. Commissioning of DESI is described in the next section.

8.1 Instrument Integration and Test

The DESI Instrument consists of a Corrector, Telescope Fixed Top End Structure, Hexapod, Corrector Alignment System, Focal Plane Assembly, Fiber System, Spectrograph System, Fiber View Camera, and Instrument Control System, as shown in Figure 1.1. Each of these major elements is the responsibility of distinct collaborators or groups of collaborators. Most of these elements will first be brought together at the Mayall Telescope during the Installation Campaign. To ensure successful integration of these elements, a comprehensive Integration and Test plan is required, along with rigorous Interface Control.

An Integration and Test Flow has been developed (DESI-0377). Figure 8.1 illustrates a high-level synopsis of this Integration and Test Flow. To minimize problems due to faulty elements, components and subsystems are to be verified before integration into higher level of assemblies. Depending on the component or subsystem, verification may be as simple as a visual inspection or as complex as a complete functional test under environmental extremes. System-level integration and test steps are the ultimate responsibility of and require approval by the Level 2 I&T Managers.

This subsection describes system-level I&T activities up until the major DESI instrument elements are handed off to NOAO on-site. These activities include bringing major subsystems together prior to shipment to NOAO, along with post-delivery verification at NOAO. Integration of DESI to the Mayall will primarily be performed by NOAO and their contractors, with help from DESI personnel.

Post-delivery verification will be carried out primarily by the instrument team responsible for the system level I&T with support from DESI and NOAO personnel. The DESI components will be delivered to NOAO in various stages of integration. Upon receipt, the shipping crates will be inspected for visible signs of damage, and any environmental monitors used to track relevant conditions during transit (including dynamic loading, temperature, humidity, and air pressure) will be checked. After unpacking, the hardware will be inspected visually and tested to verify functionality. Depending on the environmental and testing requirements, this verification will take place in the NOAO-Tucson high-bay facility, the Instrument Handling Facility on Kitt Peak (which

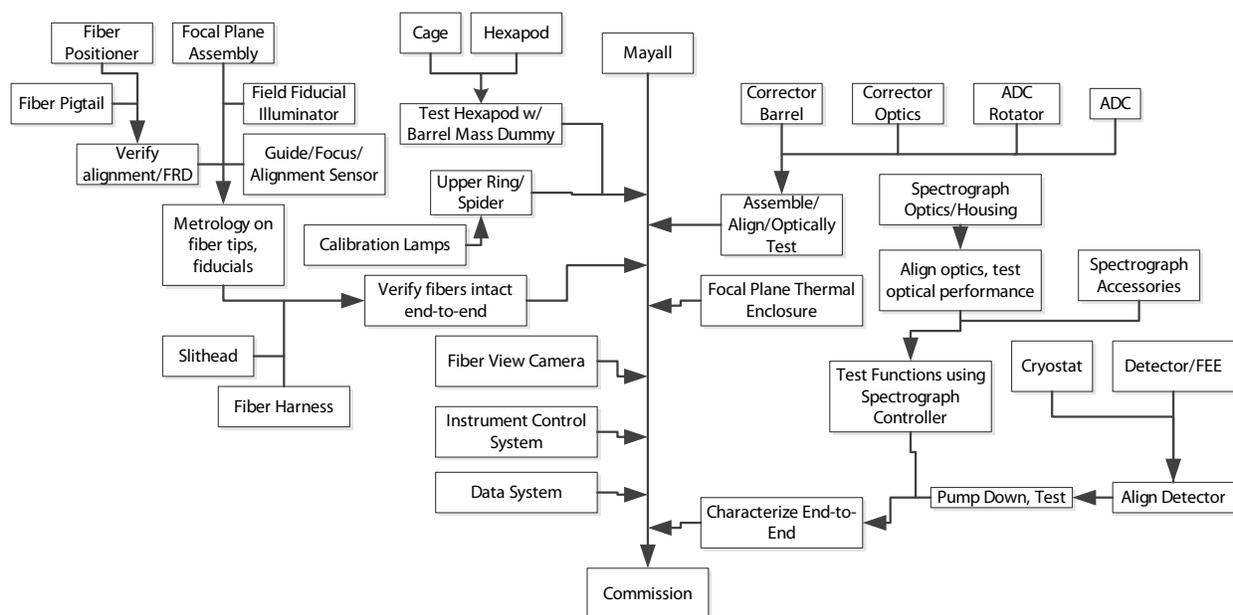


Figure 8.1: High-level DESI Integration and Test flow

includes a class-10000 clean room), or the Mayall Telescope building on Kitt Peak.

After passing these post-shipping tests, elements will be handed over to NOAO, who will execute the integration with the Mayall Telescope as described in Section 8.3.

8.1.1 Corrector Barrel/Corrector Optics/ADC Rotators

Integration, alignment, and test of the Corrector Assembly prior to delivery to NOAO is described in Section 2.2.3.

The three segments of the Corrector assembly will be shipped to NOAO in three individual shock-isolated crates. Unpacking, verification, and integration of the Corrector will occur in a tented area on the ground floor of the Mayall building. This area will be outfitted with a portable gantry crane, along with the UCL turntable/pencil beam setup. Reassembling in the Mayall building will limit transportation loads on the fully assembled corrector.

The ADC rotators will be run post-delivery at least one full revolution in each direction. Motor current will be monitored and verified to be within specification.

Post-delivery to NOAO, laser pencil beam/rotary table testing (as described in Section 2.2.3), will be done after the three segments are integrated together. This mainly verifies that the lenses have not shifted significantly since pre-ship testing.

8.1.2 Telescope Fixed Top End Structure/Hexapod

The hexapod assembly will be delivered to the supplier of the Cage, Spider, and DESI Upper Ring. The cage and hexapod will be integrated together, and a corrector/focal plane mass dummy will be integrated to the hexapod. Functional testing of the hexapod will include running hexapod algorithms and measuring associated motions of the corrector/focal plane mass dummy. In addition, range of motion, power consumption, and temperatures of the hexapod motors will be measured.

Following hexapod verification, the mass dummy, hexapod assembly, and cage all will be separated from each other. The hexapod will be shipped to NOAO in the crate it arrived in. The

spider vanes will be shipped together in a crate. The cage will be shipped in a crate by itself.

The upper ring will be a monolithic weldment 5.4 m in diameter. It will necessarily be an oversize load for on-highway transportation. It will be plastic-wrapped and mounted on a flat-bed truck for shipping to NOAO.

After delivery to NOAO, the hexapod system will be run on the bench through a test sequence of motions. The direction of the hexapod motions will also be measured. Motor current will be monitored and verified to be within specification.

Post-delivery verification of the elements of the telescope fixed top end structure include unpacking and visual inspection. In addition, prior to integrating the spider vanes and cage to the new upper ring, the new upper ring will be test fit to the Mayall Serrurier trusses as described in Section 8.3.2.1.

8.1.3 Focal Plane/Fiber System

8.1.3.1 Pre-Shipment

The Focal Plane Assembly and Fiber System are closely interwoven. Each fiber positioner will be integrated with its fiber ferrule and associated positioner fiber assembly with a cleaved end. Then each of the ten focal plate segments will be populated with 500 fiber positioners with their fiber pigtailed and electrical wires routed through the focal plane fiber management system to that segment's fiber junction box, containing 500 fiber ends. As groups of twelve positioners are integrated, those twelve positioners and fibers will be tested to verify basic mechanical, electronic, and optical operation. This is an opportunity to address issues without having to de-integrate positioners after they are fully surrounded by neighbors. Once the segment is fully populated, basic operation of all of the fiber positioners, GFA modules, and field fiducial illuminators will be verified using a test sequence driven by a PC. Integration and test of the focal plane segments to this point (including field fiducial illuminators and GFA modules) will have been the responsibility of the focal plane integrator.

Each petal assembly will be surveyed using a coordinate measuring machine (CMM) with a touch probe to map the relative locations of each field fiducial illuminator, the GFA fiducial illuminators, and the reference tooling balls installed in the focal plate. With this set of known relations, fiber view camera measurements of the illuminated field fiducials, GFA fiducials, and back-illuminated science fibers can map accurately to physical locations, establishing the focal plate scale and the relation of the fiber tips to the guide sensor pixels.

In parallel with the assembly of the focal plane, ten ~ 35 m 500-fiber cable assemblies from slithead to cleaved fiber ends will be built and tested as described in Section 4.6. Each of these fiber cable assemblies will be integrated to its respective focal plane segment assembly by threading the fiber ends into the cable side of the fiber junction box, strain-relieving the mechanical cable end to the fiber junction box, fusion bonding the cable fiber ends to the positioner fiber pigtail ends by extending them out from the junction box to a fusion splicer, dressing the now-continuous fiber loops into the fiber junction box, then installing covers on the junction box. Fiber integrity will be tested by illuminating the slit block and looking for dark fiber tips at the positioners. Diagnosis and repair of discontinuous fibers will take place at this stage. Basic operational tests of the positioners, GFA modules, and field fiducials will be performed.

Once integrated with its fiber cable, each focal plate segment will be integrated one at a time with the focal plate interface ring/focal plate adapter assembly. Once all ten segments are integrated and the center connection plates installed, a CMM with a touch probe will be used to verify alignment of the petals to each other and the integration ring. Fiber integrity and basic operational

tests of the positioners, GFA modules, and field fiducials will be repeated.

The complete focal plane assembly with integrated fiber cables will be crated together and shipped to NOAO as a single unit. The Focal Plane rear closeout and thermal management system will be crated and shipped separately.

8.1.3.2 Post-Delivery

To avoid contamination, unpacking, inspection, and testing of the Focal Plane/Fiber System assembly will be done in a clean tent.

The integrity of the fibers will be verified by illuminating each slithead one at a time and observing light from each fiber tip of the corresponding focal plane segment. A record of this test will be a digital photograph of each segment with lighted fiber tips.

The liquid cooling loops in the heat exchangers will be plumbed and leak-checked.

The cooling fans will be run and current monitored and verified to be within specification.

The field fiducial illuminators will be powered and visually confirmed to function.

The GFA sensors will be turned on and tested for functionality, sensitivity, and contrast.

A fiber positioner drive computer will be connected to the fiber communication system, and all 5000 fiber positioners will be operated without using a fiber view camera. The positioners may be operated individually or in groups. This test is designed only to verify the operation of the positioners, not their accuracy.

To avoid the need for collision avoidance, the positioners will be commanded to move only within the 10.4 mm envelope that avoids any contact with neighbors. Operation will be verified visually and recorded on video to aid in identifying and diagnosing problem positioners.

8.1.4 Spectrographs/Cryostats

CCDs and their front end electronics will be installed and aligned in the cryostats by the cryostat supplier. Non-contact metrology will be used to accurately locate and orient the active area of the detector relative to precision interfacing features on the cryostat. The CCD location will be verified cold, under vacuum through a dummy Field Lens Assembly with a flat window. This will ensure that the Field Lens Assembly is correctly located in relation to the CCD, and that each cryostat is interchangeable with every other cryostat of the same channel.

The Field Lens Assembly will be supplied by the spectrograph camera supplier. Because it also acts as the vacuum and contamination barrier to the cryostat vacuum vessel, it will be integrated to the cryostat by the cryostat supplier after the dummy Field Lens Assembly is removed. The integrated and sealed cryostats will be shipped to the spectrograph integrator under vacuum. One complete, tested spare cryostat for each channel (three spare cryostats in total) will be shipped to NOAO to minimize downtime in the event of a cryostat failure in-service.

As described in Section 5, the spectrograph integrator will assemble and align the spectrograph without the cryostats but with optics, gratings, shutters, illuminators. Testing of throughput and PSF will be done at that integration level.

The cryostats with integrated detectors and field lens assemblies will then be integrated to each spectrograph assembly by the spectrograph integrator. A test slithead will be used to do complete calibration, resolution, and stray light testing. Each tested and characterized spectrograph will be shipped to NOAO as an assembly including its three cryostats.

Post-delivery verification of the spectrographs will include operation of essentially all functions, but not verification of optical performance (e.g., no PSF or throughput measurements).

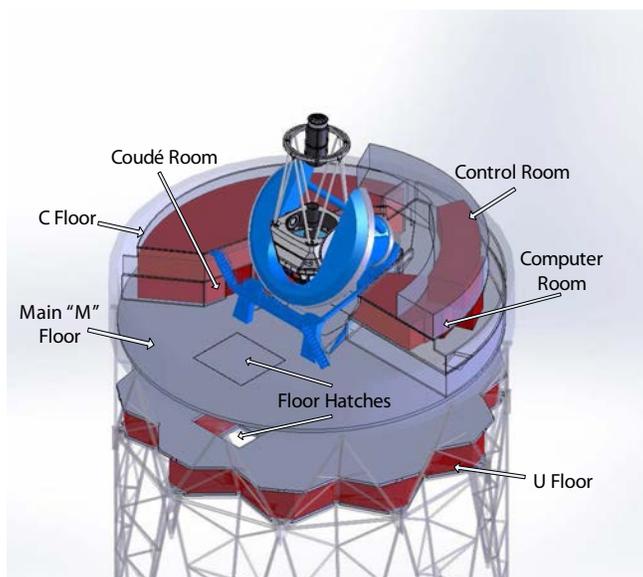


Figure 8.2: Iso view of the Mayall telescope at zenith pointing, showing the general layout of the major supporting facilities referred to throughout the text. The old FTS lab is on the same floor level as the Coudé room, below and behind the Computer Room from this viewing angle.

After external and internal inspection, the spectrograph purge will be connected, the cryostats will be plumbed to cooling water and leak-checked, the vacuum in the vacuum vessel will be regenerated as needed, and detector cool down using the LPTs will be started and allowed to stabilize overnight.

A test slithead with illuminator will be installed.

The exposure shutter and NIR shutter will be verified by opening and closing individually.

The Hartmann shutters will be verified by opening and closing one half at a time.

The fiber back-illuminator will be operated.

CCD/FEE operation will be verified using the test slithead illuminator.

8.1.5 Instrument Control System

Integration and test of the Instrument Control System is described in Section 6.9.

8.1.5.1 Fiber View Camera

After arrival at the Mayall, the fiber view camera will be connected to a computer and its function verified by imaging a test pattern.

8.2 Mayall Preparation

This subsection describes the work needed to prepare for the installation of the DESI instrument on the Mayall telescope. Much of this work will begin while the telescope is still in use for regular scientific observing with its existing instruments. Figure 8.2 illustrates the general layout of the telescope and the surrounding rooms and facilities that will be mentioned frequently throughout this subsection and the next.

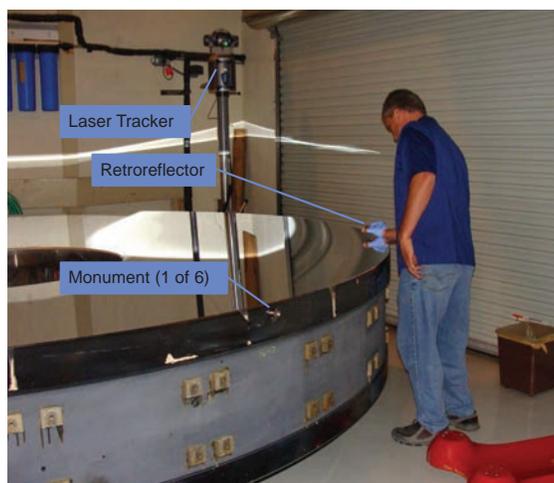


Figure 8.3: Laser tracker surveying of the Mayall primary mirror in July 2014. Just before re-aluminization, the mirror was washed and its optical surface, outer diameter, and inner hole diameter were surveyed relative to the six permanent monuments on the mirror outer diameter. This survey yielded the relation between the mirror optical axis and the fixed monuments, to help align DESI to the primary mirror.

8.2.1 Measurements

Measurements of the Mayall M1 surface and environmental monitoring of key locations at the Mayall will be used to help define requirements and guide the development of the DESI instrument.

8.2.1.1 Laser Tracker Measurement of M1 Surface

Just prior to re-aluminizing the Mayall primary mirror in July 2014, its front surface, inner hole diameter, and outer surface diameter were surveyed using a laser tracker. These measurements were made relative to six magnetic laser tracker retro-reflector monuments that were permanently bonded to the outer diameter of the mirror in 2013. Figure 8.3 shows the mirror being surveyed on the ground floor of the Mayall building.

The aspheric profile of the mirror surface was fitted to a solid model of the mirror to identify the location and orientation of the mirror optical axis relative to the fixed monuments. The survey was done with the laser tracker located in three different azimuthal positions around the mirror, and the results of the three surveys bundled to give a best-fit relation of the surfaces to the monuments. These measurements will be used to align the DESI cage and corrector barrel to the Mayall primary mirror, using a laser tracker and tracker monuments on the DESI hardware.

The individual measurements of the monument locations relative to the mirror axis deviate from the bundled values by an average of 25 microns, and the locations of the centroids of the six monuments deviate from survey to survey by 13 microns. The inferred orientations of the optical axis (the Y-axis in the model) vary by less than 4 arcseconds from survey to survey. The mirror optical axis was found to be offset 9 mm from the mirror hole and outer diameter, indicating that those cylindrical surfaces are not good references for optical alignment.

8.2.1.2 Environmental Monitoring

Data on the thermal and vibrational environment of the telescope and immediately associated facilities are needed for the detailed design. The most critical parameters are the thermal and

vibration environment at prime focus and in the Coudé Room. Work has already begun in several areas.

Accelerometers were installed temporarily and used in measurement campaigns in the prime focus cage and in the large Coudé room. Accelerometers in the prime focus cage were used to measure the background vibration spectrum during normal operation and to assess the additional vibration from different types of cooling fans. These data will provide critical input to the design of any cooling system needed for the DESI prime focus hardware. Accelerometers on the floor of the Coudé room were used to measure the spectra of vibrations transmitted through the floor from different pieces of telescope and facility equipment that are currently used during normal observing. Similar measurements with the accelerometers on the cart of a large instrument stored nearby were used to assess the vibration mitigation provided by the wire-rope shock isolators in the cart. These data will be used in modeling the mechanical structures of the spectrographs and their racks, and for incorporating any needed damping devices into the racks and their mountings.

Temperature monitoring in the originally planned DESI spectrograph location (the old Fourier Transform Spectrograph or FTS lab, on the main dome floor West of the telescope mount) has been done with a combination of the existing building monitoring system and portable USB temperature loggers. Similar monitoring has begun for the Coudé room (East of the telescope mount on the same floor) using monitors connected to the building environmental control system. The Coudé room is the preferred location for the spectrographs versus the FTS Lab as it allows a shorter fiber run and it offers quite a bit more space for a thermally controlled enclosure and other support equipment. The Coudé room monitoring program found that the room temperature follows longer-term temperature changes in the dome and outside, but with a time lag of 24–36 hours, and roughly a factor of 2 dampening in response amplitude. The Coudé room also experiences seasonal variations in temperature, typically ranging between 10 °C and 20 °C, with recorded extremes during the monitoring period of 0 and 25 °C. These data will help define the requirements for the thermally controlled spectrograph enclosure. Parallel monitoring of temperatures in the dome is helping to define the operating range required of the prime focus components. The interior of the dome saw temperature variations typically between 0 and 25 °C, with recorded extremes of during the recording period of -10 and 28 °C. An extreme low temperature of -18.1 °C was recorded in the dome in February 2011.

8.2.2 Observatory Facility Modifications

8.2.2.1 Cooling System Modifications

Heat removal from equipment and temperature control of the telescope chamber and support equipment is currently provided by the Mayall facility chillers. Currently the Mayall facility has two chillers. One, the “new chiller” is routinely used. The other, the “old chiller” is routinely not used but is currently available as an in-place spare. The new chiller, a Carrier Aqua Snap Model 30RAN045, was installed in 2009 and has a nominal cooling capacity of 45 tons at sea level. It can deliver about 43 tons of cooling after de-rating for the working altitude of 6875 feet. Under the typical load conditions currently encountered, the Mayall facility uses no more than 50% of the capacity of the new chiller. Thus there is about 20 tons (72 kW) of cooling capacity available presently. In addition, during DESI operations there will be no need to cool the two He compressors currently used on the NEWFIRM cryogenic system; these compressors impose about 5 kW of heat load each during NEWFIRM operations. In the DESI era, this 10 kW of heat removal will also be available for DESI equipment, making a total of about 82 kW of heat removal available for DESI equipment, solely from the new chiller. The old chiller, a Trane unit (model number unknown),

Table 8.1: DESI heat sources and locations (Estimated average power during science operations, reference document DESI-0484).

Subsystem	DESI Document	Location	Mean Heat Load (W)
Focal Plane	389	Prime Focus	466
Hexapod	621	Cassegrain Cage	130
Fiber View Camera	388	Cassegrain Cage	50
Spectrograph Shack	470	Coudé Room	2,500
Spectrograph Equipment	470	Coudé Room	1,400
Computer Equipment	473	Computer Room	23,500
Total			28,046

was built in 1992 and has a nominal capacity of 40 tons, or about 38 tons (130 kW) after de-rating for the working altitude. This chiller is plumbed into the system and can be run, but it is normally not run because the new chiller is more than adequate to meet existing demand.

Detailed heat budgets for the DESI equipment are under development, but drafts are contained in DESI-0389 for the Focal Plate Assembly, DESI-0621 (Hexapod) and DESI-0388 (Fiber View Camera) for the Cassegrain cage, DESI-0470 for the Coudé room, and DESI-0473 for the computer room. Summaries of these loads are reflected in Table 8.1.

At the telescope top end, heat will be actively removed from the elements inside the thermal shroud: fiber positioners with electronics, Guide-Focus-Alignment sensors (GFAs) with electronics, focal plane cooling fans, field fiducial illuminators, and power supplies. The fiber positioners are by far the largest peak heat load, but are operated only intermittently. The relatively high thermal time constant of the focal plane system allows the cooling system to be sized for mean heat load rather than peak. Heat will be removed from the top end by means of a liquid loop running from a liquid-air heat exchanger located outdoors on the telescope catwalk, powered by a pump to account for the height gain to the telescope top end. The requirement is to maintain the temperature within the focal plate thermal shroud at ambient or slightly above. It is important not to cool the focal plate assembly below ambient in order to prevent condensation from forming within the shroud under humid conditions. Therefore this system will simply extract the modest average heat load from the ambient air within the shroud and deposit it outside; it will return ambient-temperature coolant to the heat exchangers in the shroud. Within the thermal shroud, the cooling liquid will be plumbed through heat sinks in direct contact with heat sources other than the positioners, and through one or more air-liquid heat exchangers in a gentle forced-convection air loop with the fiber positioners. The hexapod and ADC motors are expected to operate with such low duty cycle and power levels they will produce negligible effects on image quality if they are allowed to cool by conduction to the structure and by natural convection to the air. The calibration lamps on the top ring will not operate during observations and will not have active heat removal.

In the Coudé room, there will be a chiller to supply cooling water to the thirty Linear Pulse Tube (LPT) cryocoolers that cool the science CCDs. This chiller and the spectrograph shack environmental control system will reject their waste heat into the building glycol system. The Coudé room is not currently served by the building glycol system, but the facility preparations will include extending the glycol system to the Coudé room and providing glycol distribution where needed within the Coudé room. A contract has been let to a consulting engineering firm to design the additional glycol distribution needed to serve the Coudé room, and the design was received in May 2015. There are multiple locations close to the Coudé room where the present system can be tapped; a final connection point will be determined based on required flow rate and ease

Table 8.2: Estimated DESI equipment peak electrical loads and locations (reference DESI-0483).

Subsystem	DESI Document	Location	Peak Power (W)
Focal Plate	389	Prime Focus	9,022
ADC Rotator	n/a	Prime Focus	100
Calibration Lamps	470	Top Ring	200
Hexapod	621	Cassegrain Cage	1,300
Fiber View Camera	388	Cassegrain Cage	50
Spectrograph Shack	470	Coudé Room	3,500
Spectrograph Equipment	470	Coudé Room	18,930
Computer Equipment	473	Computer Room	23,500
Control room annex	TBD	U-Floor	5,000
Total			61,602

of implementation. Other DESI equipment in the Coudé room, the cryostat control electronics and possibly an air dryer (if the Mayall facility air dryer is deemed insufficient), will vent their modest heat production into the room air. It is not expected that active cooling of the Coudé room will be necessary; if this changes, the room air can easily be kept near dome-ambient by a small air-handling unit (AHU) that includes a heat exchanger for chilling the air using building glycol.

In the Cassegrain cage, the DESI heat sources will be the fiber view camera system and the hexapod power supplies and drive electronics. Their small heat output will be satisfactorily removed by convection into the ambient air and by conduction into their mounting hardware.

DESI will use two full-height racks of computer and network equipment, to be located in the computer room. There is now the rough equivalent of one-and-one-half such racks of computers serving the current science instruments. These computers will no longer be used in the DESI era and will be removed prior to or at the start of DESI equipment installation. The net increase in space consumption and heat loading resulting from DESI installation will therefore be quite modest. The air conditioning unit in the computer room is currently loaded fairly lightly, and it has more than adequate capacity to extract the additional heat load. The U-Floor area that will be converted to a control room annex will house a few additional computers and network equipment for the telescope operator and DESI observers. The existing climate control system for that area is more than capable of handling these modest heat loads.

8.2.2.2 Electrical System Modifications

DESI will be locating a great deal of new equipment distributed among various locations at the Mayall telescope, including prime focus; the Cassegrain cage; the spectrograph room (large Coudé room); the Mayall computer room; and the Mayall control room annex. Table 8.2 shows predicted DESI electrical power loads at their respective locations at the Mayall.

Table 8.2 and Table 8.1 are not directly comparable. The electrical service must be sized to handle the maximum peak load possible, plus a suitable margin, so peak loads are shown in Table 8.2. However, during DESI operations only average heat loads must be extracted, so average loads are shown in Table 8.1. Also, the peak electrical loads in Table 8.2 include some equipment that will not be running at all except during installation or major maintenance periods; examples of this include the turbo-molecular vacuum pump and the optional clean tent for the Coudé room. The electrical service must be sized to provide for these loads, but they will add no heat to the room during operations.

There are currently one clean 15 amp 110 VAC circuit and one dirty 15 amp 110 VAC circuit

running to prime focus. It will not be possible to run new electrical wiring all the way there before DESI installation, because DESI installation will involve replacing the entire top ring and top end assembly of the telescope. However it will be practical to run the new service drops through the existing cable ways and up the telescope truss to the top ring at any time. It is currently planned to begin this work during the summer shutdown of 2015, and to continue as necessary in the 2016 summer shutdown.

It is clear that some expansion of electrical services will be required to and within the Coudé room. The current service to that room is quite minimal, and the new loads there will be large. The computer room and the control room annex may require some additional power capacity or outlets, although likely quite minor and available without expanding the capacity of the electrical panels serving those areas. NOAO has supplied the anticipated DESI loads to its consulting engineering firm and let a contract for design of the system expansions needed, including design of sufficient modern UPS capacity for the expected clean power loads. The contract calls for delivery of the design by the end of May 2015. NOAO will begin work on implementing the expansions following a separately funded overhaul of the main utility connection at the Mayall during August, 2015.

It is assumed that equipment supplied by international collaborators will be specified to run on U.S.-standard AC frequency and voltages.

8.2.2.3 Telescope Modifications

Aside from the upper ring and spider, DESI requires two mechanical changes to the existing hardware on the telescope. The first is at the baffle extending up from the center hole in the primary mirror. The upper portion of the baffle, which is a lightweight metal tube extending above the heavy weldment designed to hold an M3 mirror for the Coudé light path, vignettes the wide DESI field of view. It will be removed during the process of DESI installation, but removal is not necessary until then. This upper baffle also provides the contact point for the petals of the primary mirror cover. With the upper baffle gone, the cover petals will require extensions to cover the circular area left open by removal of the existing baffle. NOAO currently plans to design and fabricate new cover petals that are long enough to cover the entire primary mirror including the central hole (formerly filled by the upper baffle). These new cover petals will be installed during the DESI installation process, but they will require design and fabrication before DESI installation begins.

DESI also requires a new mechanical subsystem on the telescope, the e-chain cable wraps for carrying the DESI optical fibers. One set of e-chains goes around the outside of the East Declination bearing, at a large enough radius to put it completely outside of the Declination hard-stop blocks mounted on the East side of the center section. The other set of e-chains goes in front of the South bearing journal to accommodate motion about the Hour Angle axis. NOAO will design and fabricate the hardware for attaching these e-chains to the telescope structure along with the other supports or sliding surfaces that will be needed, beginning in October 2015. Fixed support brackets for the optical fibers will be designed to support the fiber cables along the upper truss en route to the Declination cable wrap. Fixed brackets will also be designed and built for the run along the wide elliptical tube between the “horseshoe” and the South bearing journal to support the cables en route to the Hour Angle cable wrap. All of the cable wraps and support hardware are planned for installation immediately following the protoDESI testing campaign. Installing these cable wraps about a year prior to the full DESI installation will allow plenty of time for testing and adjusting the wraps to enable smooth operation of the telescope with these new mechanical loads,

In addition to the mechanical changes, the Mayall Telescope Control System (TCS) software will require an interface to the comprehensive DESI Instrument Control System (ICS) that will control the DESI hardware and sequence the many complex operations required during observing.

An Interface Control Document (ICD) defining this interface has been drafted and approved by both NOAO and OSU, which is responsible for writing the ICS software. This ICD, DESI-0473, defines the protocols that will be used for passing commands and queried from the ICS, and for the responses from the TCS. It also includes examples of the commands and queries, with properly formatted responses. NOAO's preparations for DESI will include coding the TCS modules required to implement this interface, and testing them with simulation packages that represent the ICS. This TCS interface development will in fact be required for the operation of the ProtoDESI test hardware, so the software work will need to be completed and tested prior to the arrival of ProtoDESI, currently expected in the second half of 2016.

8.2.2.4 Spectrograph Room Modifications

The large Coudé room will require substantial modifications to turn it into a space suitable for the DESI hardware. Figure 5.21 shows the approximate location of the spectrograph enclosure (“shack”) in the Coudé room.

First and most obviously, an environmental enclosure (the spectrograph shack) will have to be built to enclose the spectrograph stacks. This enclosure must maintain the spectrographs at $20 \pm 2^\circ\text{C}$ in the presence of much larger diurnal and seasonal swings in the Coudé room as a whole. In addition, there will be requirements on humidity, both within the spectrographs and (probably) inside the environmental enclosure. The environmental system will need to address both of these. It will also have to provide some level of filtering for maintaining cleanliness, although the exact requirement has not been set yet. It must be large enough to enclose the spectrograph stacks in their racks as well as the fiber cables and junction boxes after they come through the wall, and all the wiring, data cables, gas piping and cold liquid distribution needed for the cryostats. Either around or inside the spectrograph shack, the working space must be large enough for a work platform, scissor lift, or other means for the personnel to access and (when necessary) remove and install a spectrograph or cryostat from any location in the stack. Access to the shack will be via doors or removable panels on the shack.

The spectrographs may also need to be isolated from building vibrations caused by fans, pumps, and movements of people. A requirement for this has not yet been determined, though data on the present vibration spectrum in the room has been taken and analyzed. Any needs for vibration damping must also be taken into account in the design of the spectrograph shack.

Finally, the large Coudé room will also be the best place to locate any other operational equipment that must be near the spectrographs, the telescope or the dome chamber, but not out in the dome environment directly. This category includes power supplies for the cryostat electronics, and the power supplies and controls for any moving components on the spectrographs (e.g., shutters, Hartmann doors, deployable sources for back-illuminating the fibers). In addition, there will be considerable support equipment – including one or more vacuum pumps, an optional clean tent, a laminar flow bench, work benches, lifting equipment, electronic test equipment, and computers – that will be used in the Coudé room during spectrograph installation and maintenance periods. All this operational and support equipment will need adequate electric power and network connections, and the operational equipment will also require cooling; these services must be planned carefully into the early stages of the process of upgrading the Coudé room.

8.2.2.5 Mayall Control Room Annex

The present Mayall control room cannot accommodate more than 5 people comfortably. Given the complexity of DESI and its numerous interactions with the telescope and dome environment, some

multiple of that number of people will be needed at the telescope during the commissioning and science verification phases. Even after regular operations commence, periodic engineering nights will be needed, which again will likely require a larger number of people than can work comfortably in the existing space. Also, provision needs to be made for participation by remote collaborators throughout the commissioning, science verification, and operations phases. This means providing for convenient videoconferencing capability into the control room space, with screens, cameras, and microphones positioned so that remote collaborators can be fully engaged in the control room work. The layout of the present control room does not permit placement of these items in locations where easy communication with everyone is practical.

The best option for providing additional working space is the conversion of a little-used lounge area on the U Floor, four floors below the control room. If properly arranged and equipped, this room can easily provide working space for 15 or more people, as well as remote participants via dedicated video (e.g., skype) screens and cameras. It is already within the climate-controlled part of the building, and it is also not far from the computer room, so providing the necessary network access would be straightforward. It would require only repainting, provision of adequate electrical and network services, modernized lighting, and appropriate furniture and computer equipment. During the detailed design phase, options for laying out the room will be considered with an eye toward making the space suitable for as many night workers as possible, as well as collaborators at remote locations. The lounge area furnishings can easily be relocated to another part of the building.

The existing control room will not be taken completely out of service, but during the DESI era it will no longer be used for nighttime operations. Having the telescope operator co-located with the DESI commissioning and science teams will be ideal for efficient nighttime work, encouraging rapid and efficient communication. The TCS software and guide cameras will all be operated over Ethernet, so other than provision of an emergency stop switch there will be no hard-wired connections required between the telescope systems and the U Floor area. The old control panel with its mechanical Selsyn dials will remain in place on the C Floor and continue to be used for movement of the telescope required by daytime engineering activities.

8.2.2.6 Calibration System

DESI will require systems for calibrating detector response (i.e., flat fielding), wavelength mapping, and line spread function determination. These systems will require light sources of significant power, projection systems inside the dome, and reflecting screens for uniformly scattering the projected light into the telescope beam. Dome-mounted equipment must be robust enough to withstand wind buffeting, making installation correspondingly complex and time-consuming. As with DECAM, the projectors per se must be mounted on the telescope top ring, so those items will be installed as part of the overall DESI installation. The current design of the calibration system calls for the light sources to be co-located on the top ring with the projection optics. The existing reflecting screen mounted on the inside of the Mayall dome is not large enough to cover the DESI field of view. However, the frame (see Figure 8.4) is large enough. NOAO will add an additional ring of panels, similar to those seen in the outer ring in Figure 8.4, to provide sufficient area. Installation of these panels will be require specialized equipment (e.g., a rented boomlift) and while underway will prevent all other work on the telescope or use of the dome cranes.



Figure 8.4: Installing the existing reflection screen used for daytime flat fielding. The screen is being mounted to the inside of the dome, between the arch girders and just below the attachment point for the dome crane rails. Note the use of a long-reach boomlift. For safety reasons, the telescope drives must be locked out and tagged out during the entire operation.

8.2.2.7 Computer Room

DESI will come with a large number of computer systems for instrument control, observation planning, image processing, and data buffering (among other uses). A careful survey of the Mayall's current computer room will be made during the detailed design phase. Some of the computers currently there (the equivalent of 1.5 full-height racks) can be retired and removed, if they support instruments or systems that will not be used during the DESI era; such removal of course cannot begin until the telescope shuts down for DESI installation. Those computers will be identified, and plans drawn up for laying out the computer room and installing the DESI hardware. The survey will also consider the electric power and cooling needs of the DESI computers, and compare that to what is currently available. As noted above, substantial changes to the electric power system will not be needed, but some additional outlets may be required. Again, preparation of the room should be done before DESI installation begins to ensure a smooth installation and commissioning process, even if the removal of old computers and installation of new ones awaits the start of DESI installation.

8.2.2.8 Ground Floor Garage

A protected space needs to be prepared within the high-bay area of the Mayall garage for re-assembling the DESI corrector, checking its alignment, and assembling the corrector and hexapod into the new Prime Focus cage frame. This space requires a clean tent with about 20 square meters of floor area and about 5 meters of working height and the tent must be slightly positively pressurized to keep out dust. Also, the garage door will be locked out of operation and sealed against dust infiltration during the period of corrector assembly. This tent will be constructed in place, much like a similar facility at the Blanco telescope used to re-assemble the DECam corrector. The working space also requires a crane with a hook height of at least 6 meters and a working capacity of at least 7 metric tons. This crane may be an A-frame crane purchased commercially, or it may be provided by the smaller of KPNO's two mobile cranes. This mobile crane is routinely used within the Mayall garage area and has more than the required load capacity and hook height. For use

in this application, provisions will need to be made for providing outside air to the crane engine and venting its exhaust to the outside of the building. Such “breathing” can easily be provided by flexible metal ductwork running through temporary penetrations in the outside wall. Both crane options will be thoroughly evaluated and costed during the detailed design phase.

8.2.3 Installation Planning

Detailed planning of tasks must be carried out before DESI installation begins. Tasks need to be in the proper order and carefully coordinated to avoid conflicts over personnel resources, physical resources such as cranes, and working space. All resources required for each task need to be clearly identified and their availability confirmed. Work should not begin until this plan has been completed and thoroughly reviewed.

The first draft of such a plan has been done, although it is still very clearly a preliminary draft. First, there is a widely varying level of detail possible at this stage of the DESI project. While there is reasonable detail on steps that Mayall personnel are familiar with (e.g., removing the primary mirror), there is considerably less detail on other steps where designs of DESI equipment are less advanced. In a few cases, no design exists yet for some specific features such as the mounting of the Declination and Hour Angle cable wraps to the telescope structure. Of necessity, time requirements and resource needs are still purely notional for installing things that have not been designed. This plan will therefore evolve throughout the design and fabrication phases of the DESI project, in order to keep up with the developing project design details.

At the same time, it will be mandatory to develop safety plans for the entire installation process. These will include procedures for every task identified in the plan; every procedure will be accompanied by a Job Hazard Analysis (JHA). These procedures and the associated JHAs will develop along with the plan, seeing revisions as needed to keep them current with the state of the DESI equipment designs. Safety planning will also encompass identification of all critical lifts to be carried out during installation, and writing of Critical Lift Plans for every critical lift. Finally, the safety planning will cover the training required for all personnel, ranging from training in general KPNO conditions and policies to specific training required for individual tasks. Like the installation plan itself, the basic safety documents have been drafted, but they are expected to be revised throughout the DESI design and construction period. Task-specific safety documents and lift plans will continue to be written and revised up to the point of readiness to begin installation.

NOAO intends to call a formal installation readiness review prior to the shutdown of the telescope. This external review will cover the final detailed installation plan and the safety plans, as well as the status of the preparation work described above.

8.2.4 Installation Equipment Preparation

In connection with the installation planning, NOAO is also designing and will construct three items of specialized equipment needed during DESI installation. The first item is the set of work platforms needed for the removal of the existing top and flip rings and the installation of the new DESI top end. These platforms will allow safe work spaces for personnel while the telescope is locked in a zenith-pointing orientation. Their design is based on that for the similar platforms used at CTIO during DECam installation, although some changes are planned such as allowing access via a combination of stairs and a ladder (see Figure 8.5). The second item is a set of braces for securing the upper Serrurier truss members in position prior to removal of the existing top end. These braces (also depicted in Figure 8.5) must be secure enough to hold these truss members in position with nothing attached to the truss tops, and yet must be easy enough to install and remove



Figure 8.5: Extract from preliminary design for the lower of two Zenith work platforms, showing the stairs-plus-ladder access arrangement. Also shown, above the lower platform, are the braces for securing the upper Serrurier truss members when the top ring system is removed.

that those steps can be carried out by personnel working either on the zenith work platforms or in a mobile boomlift. The completed preliminary design incorporates these braces into the upper Zenith work platform, using the braces as part of the support for the upper work platform. Figure 8.6 shows the complete design with all features visible. The third item is a set of work platforms to allow personnel the required access along the East side of the upper truss and the horseshoe while the telescope is tipped over to the Southeast Annex, in order to install the DESI fiber cables. These cables will arrive attached to the DESI Focal Plate Assembly, which will be installed at the Southeast Annex. The cables will then need to be attached to the DESI top ring, the East side of the upper truss, and the Declination cable wrap. These work platforms will be needed to allow personnel access to those areas while the telescope is oriented to the Southeast Annex. Design of these platforms is underway as of the time of this writing.

8.3 Installation

DESI Installation will require that the telescope be inoperable for almost a year. Obviously, once this process begins, the telescope will no longer be usable for nighttime observing. The launch of this phase thus represents a major milestone for the project, as well as a major change in the scientific capabilities available to the US astronomical community. The schedule and sign-off procedures for beginning the DESI installation will be worked out by the funding agencies. The next subsections describe the current understanding of the DESI installation steps. These will be further developed during the detailed design phase of the project.

Throughout this discussion, it is important to remember some of the physical parameters of the dome and the dome working environment that will drive much of the installation process. First, the 5-ton and 50-ton dome cranes have a limited reach from the dome center. Figure 8.7 shows the range of motion of those cranes; the outer edge of the orange circle represents the limit of reach for the 5-ton crane, and the inner edge represents the limit of reach for the 50-ton crane.

Second, the dome cranes travel radially within the circle shown in Figure 8.7 along their rails,



Figure 8.6: Preliminary design for both upper and lower top end platforms, showing access ladder and stairs, and showing upper platform supported by upper truss braces.

but they are moved azimuthally only by rotating the dome itself. The dome rotation drive system has no brakes, depending rather on rolling resistance and mass to bring the dome to a stop. It can be positioned reliably to within about a foot by an experienced operator, but the dome cranes cannot be relied upon for precise horizontal positioning of loads. The lack of brakes also means that the dome, along with the cranes and any loads suspended from them, can be moved by the wind under strong wind conditions. It will thus be necessary to specify and observe wind speed limits in planning and carrying out all critical lifts involving the dome cranes.

Third, the dome hatch (the gray square North of the telescope in Figure 8.7) has a cover that is divided roughly in thirds. The center hatch section can be removed without disturbing the outer two sections, but removing either of the outer sections requires first removing the center section. All three sections are heavy steel-and-concrete constructions designed to support the weight of the primary mirror and its cell. Removing or replacing them requires use of the 50-ton dome crane itself, and so the hatch sections must be stored within crane range, usually adjacent to the hatch on one side, whenever hatch opening is required.

8.3.1 Removal of Existing Telescope Hardware

Just prior to the start of DESI installation, any instruments not currently mounted on the telescope, along with their handling carts or other support equipment, will be removed from the Mayall building and stored elsewhere on Kitt Peak or in Tucson. As soon as the telescope is taken out of service, all computers that will not be needed during DESI operations will be shut down and removed from the computer room. The computer removal does not interfere in any way with the telescope mechanical work underway in the dome, so it can proceed independently.

8.3.1.1 Preparation of Top End for Removal

DESI requires the complete removal and replacement of the existing telescope top end, including the upper ring, flip ring, spider vanes, and prime focus assembly. In preparation for this removal,

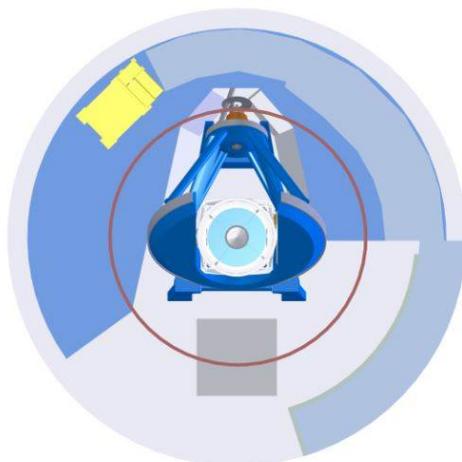


Figure 8.7: Plan view of telescope and dome with the crane limits marked (orange circle). North is down in this view.

first the telescope will be positioned at the South limit. The Mosaic-1.1 prime focus imager will be taken off, boxed, and removed from the building for storage. The Mosaic-1.1 counterweight will be installed in its place. The telescope will then be moved to the Southeast Annex and physically restrained. The $f/8$ M2 will be removed, placed in a protective crate, and then removed from the building to external storage. The M2 covers will be removed, and the M2 counterweight installed to maintain telescope balance (Figure 8.8). All existing service connections – power, data, air, vacuum, etc. – will be removed from the prime focus cage and stripped back to points below the top rings. Temporary platforms will be installed on the truss to enable personnel access to the top ring at zenith. Bracing will be installed between the upper trusses to support them in the absence of the upper ring. Finally, the inner and outer top rings will be secured together with welded plates.

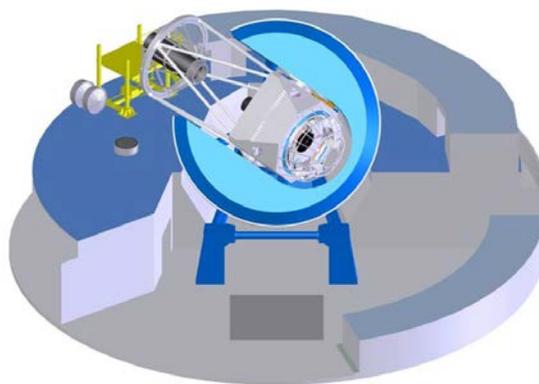


Figure 8.8: Telescope positioned at the Southeast Annex. The secondary mirror and its covers have just been removed and are laid off to the side.

8.3.1.2 Bottom End Disassembly

The telescope will be rebalanced and returned to the zenith-pointing position, locked out and tagged out, and physically restrained. All needed handling equipment will be staged and prepared for M1 removal. The currently mounted Cassegrain instrument will be removed, placed in its handling cart, and removed from the building for long-term storage on Kitt Peak or in Tucson. The Cassegrain equipment cage and lower shell will all be removed from the telescope bottom end. The existing central baffle assembly will be removed and lifted off the telescope. All removed items will be staged on the main dome floor (the M floor) or the console room level (the C floor). Next the M1 and its cell will be removed from the telescope, and the M1 removed from the cell. The M1 will be lowered to the ground floor and stored in the aluminizing chamber for cleanliness and safety. The M1 cell, the lower shell and the Cassegrain cage will then be re-installed on the telescope to make space in the dome for DESI installation. The central baffle assembly will be removed from the building along with any other items still remaining. Figure 8.9 shows the telescope with the bottom end completely disassembled and all components staged for removal from the dome. The primary mirror is on the C floor, above the Coude room. The central baffle assembly is on the C floor above the old FTS lab. The mirror cell is on the hatch. Staging these items in these locations is part of the normal process used for primary mirror re-aluminizations throughout the service life of the Mayall.

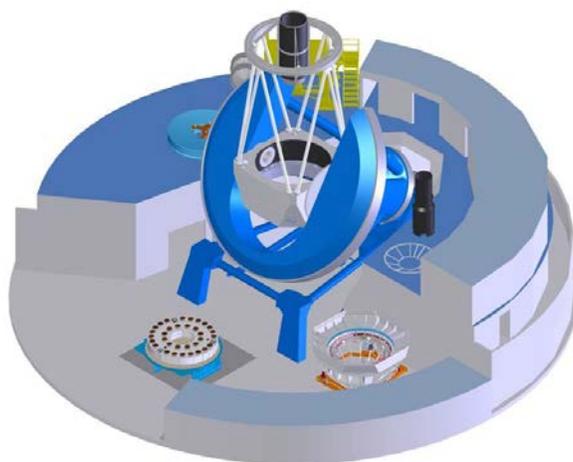


Figure 8.9: The Mayall telescope with the bottom end fully disassembled and the components staged for removal from the dome.

8.3.1.3 Top End Removal

Equipment needed for disassembling the top end will be brought up to the M floor and placed in position (Figure 8.10). The 50-ton dome crane will be rigged to the inside of the Prime Focus cage which has been exposed by the removal of the M2 mirror assembly. The bound top rings will then be unbolted from the top ends of the upper truss members. Once free, the top end assembly will be lifted off the upper truss members as a unit, just enough for the lower spider vanes to pass between the North and West truss leg-pairs (Figure 8.11).

This is a tight fit, but careful examination and manipulation of the solid models demonstrates that there is sufficient clearance with margin (Figure 8.12). When it is fully clear of the telescope the top end assembly will be lowered to existing workstands in place on the M floor. The top end

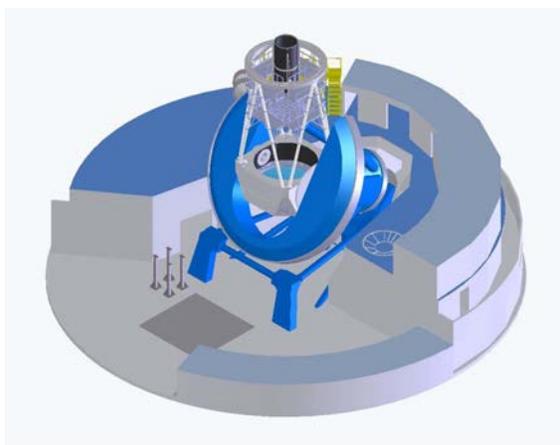


Figure 8.10: Bracing and work platforms in place for removal of top end.

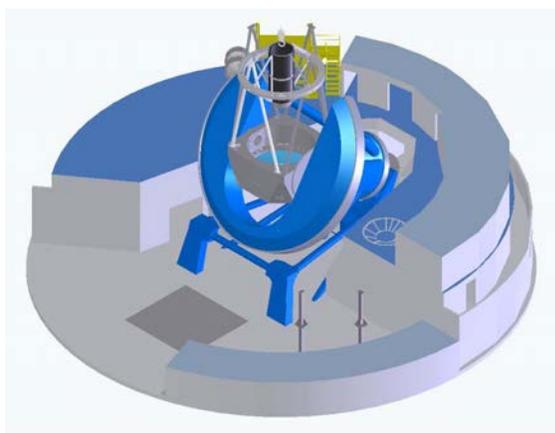


Figure 8.11: Top end lifted off upper truss members.

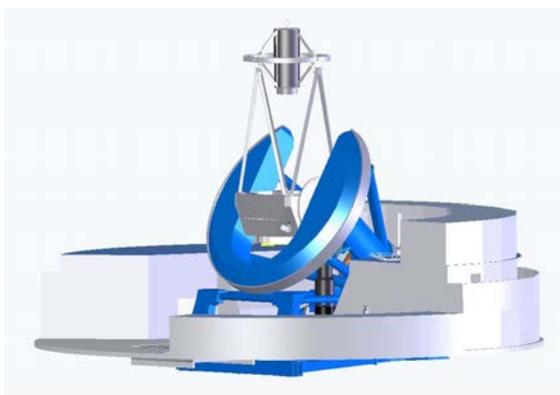


Figure 8.12: Side view showing clearance for removal of top end.

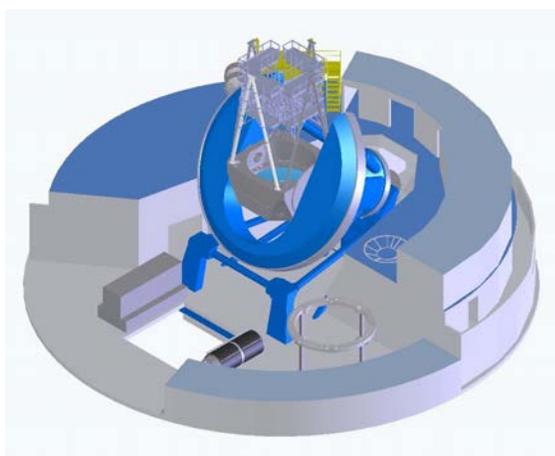


Figure 8.13: Disassembly of old top end on M floor. Hatch cover sections stacked to left of open hatch. Top end bracing and platforms installed.

will be disassembled into its major components: the bound rings, the spider vanes, and the Prime Focus cage (Figure 8.13). The cage will be wrapped for protection, lowered to the ground floor and removed from the building for storage elsewhere. The spider vanes and bound rings will be lowered piecemeal to the ground floor, coated with a protectant seal, and stored in the outdoor storage yard on the mountain. The telescope is now ready for DESI installation.

8.3.2 Installation of DESI Hardware

The task of installing DESI includes work both on and off the telescope. One of the major off-telescope tasks (assembly of the prime focus cage with its major components) must be scheduled critically to be ready in time for installation on the telescope. Other off-telescope tasks, such as installation of the spectrographs, may (depending on the readiness dates of the spectrographs) be paced by the on-telescope work in that there are very limited opportunities to bring spectrographs into the building while the on-telescope work is going on. Completing the installation as quickly

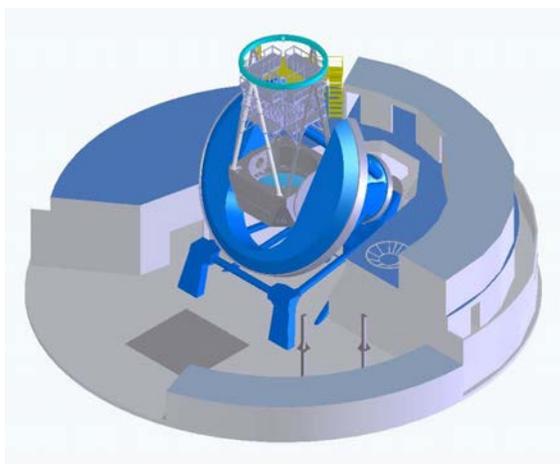


Figure 8.14: Test fit of the DESI top ring to the truss.

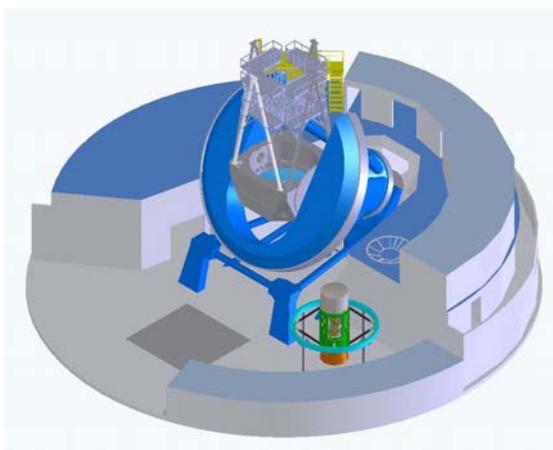


Figure 8.15: DESI prime focus cage installed in top ring on dome floor.

as practical will require very careful scheduling and detailed work coordination to ensure safety, efficiency, and quality of work.

8.3.2.1 Initial Assembly and Installation of New Telescope Top End

First, prior to any on-telescope assembly work, the DESI prime focus cage assembly, consisting of the cage structure, the corrector barrel, the hexapod and a dummy weight in place of the focal plate adapter, the focal plate and the fiber bundle, will be assembled in the garage high-bay on the ground floor of the Mayall building. Assembling the cage inside the Mayall building will avoid the need for truck transport of the assembly, but the assembly work there will interfere with the ability to remove old Mayall components from the building or bring DESI components into the building. Ingress or egress for components too large to fit in the personnel elevators will have to be scheduled around the cage assembly work.

Inside the dome, the new DESI top ring will be lifted to the top of the telescope truss and test-fit to the truss members (Figure 8.14). After a satisfactory mechanical alignment of the ring to the upper truss is obtained, the ring will be punch-marked in place, for later drilling and tapping of the screw and pin holes for attaching the ring to the upper truss. Then, the empty top ring will be lowered back to the M floor and placed on work stands near but not on top of the main hatch in the floor. The ring will then be drilled for the bolts and pins needed for truss attachment, and the bolt holes will be tapped.

The prime focus cage assembly will then be lifted into the dome and placed in position at the center of the top ring, and the spider vanes will be installed to connect the two (Figure 8.15). Then, the cables and other connections for the hexapod and ADC will be extended from the cage to the top ring and dressed in place for later connection. The lamps and projection optics for the calibration system will also be installed at this time, and their wiring dressed in place to the ring for later connection. Finally, the completed top end assembly will be lifted to the top of the telescope truss and bolted in place atop the truss members (Figure 8.16). All connections for the hexapod, the ADC, and the calibration lamps will then be completed between the unterminated service lines at the top of the truss and the dressed connections from the hardware on the top end assembly. Basic “on-off” tests will be performed at this point to verify operability of both the ADC and calibration lamps. The hexapod cannot be tested until its power supplies are installed (next

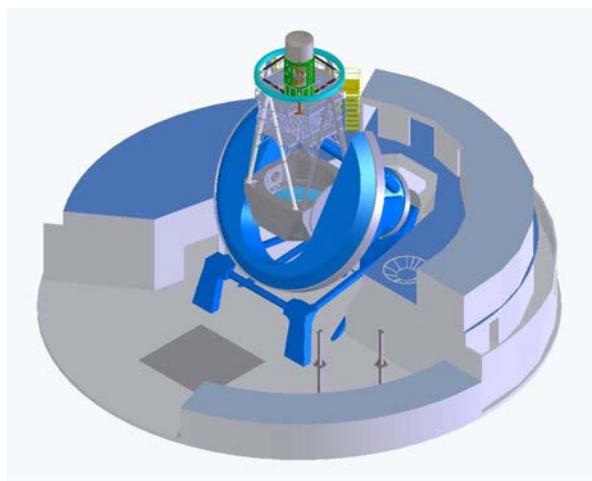


Figure 8.16: DESI top end assembly installed on telescope.

section). The top end assembly fixtures will be removed from the main floor to make room for the telescope bottom end re-assembly.

8.3.2.2 Re-Assembly of Telescope Bottom End

Fine alignment of the Prime Focus cage requires the laser tracker monuments (retro-reflector target mounts) that are permanently bonded to the edge of the primary mirror. Re-installation of the primary mirror must therefore take place before fine alignment.

With the upper portion of the central baffle assembly removed, the primary mirror cover petals will be replaced with revised versions that extend to the center, fully covering the entire mirror and Fiber View Camera. The next steps are to recoat the primary mirror with aluminum, remove the lower shell and mirror cell, lift the mirror up to the M floor, re-assemble the mirror in its cell, and re-install the cell and lower shell on the telescope. Then the Cassegrain equipment cage will be re-installed along with the mirror support control equipment it contains. The hexapod power supplies will be installed in the Cassegrain cage, and the power cables from the supplies to the hexapod will be dressed along the outside of the center section and up one of the upper truss members along the West side of the truss where they will be out of the way of the optical fiber installation later. The hexapod can now be tested for operability; the hexapod specialists (from FNAL) can carry out these tests in parallel with the following steps in the Cassegrain cage. Following that, the Fiber View Camera will be installed at the back of the mirror cell in place of the now-removed Cassegrain rotator, connected and tested, and aligned with visible targets on the corrector barrel or prime focus cage. Finally, any other DESI equipment to be installed in the Cassegrain cage, such as power supplies for the focal plate (TBD), will be installed. The counterweights on the bottom end of the telescope will be adjusted as necessary to provide a proper balance with the weight of the new DESI top end. The new DESI top end is required to weigh no more than the weight of the existing top end that is being removed. However, the bottom end of the telescope will be substantially lighter (more equipment is being removed from the bottom end than is being added) so additional counterweights will be required at Cassegrain. This stage ends with a coarsely balanced telescope that is ready to be moved but still physically restrained for safety.

8.3.2.3 Top End Mechanical Alignment

Next, with the hexapod adjusted so the barrel is at the midpoint of its range of motion relative to the cage, detailed measurements will be taken of the position the Prime Focus corrector barrel relative to the laser tracker target monuments on M1. These monuments were previously used to locate the optical axis of M1 relative to its outer circumference. Using a laser tracker mounted on a temporary fixture above the center section, it will be possible to survey simultaneously four of the six M1 retro-reflector locations and four retro-reflectors fixed to the corrector barrel. These measurements will be used to adjust the tension on the spider vanes, if necessary, to position the new cage assembly so as to align the corrector barrel as closely as possible to the M1 optical axis with the hexapod at the middle of its travel range.

8.3.2.4 DESI Fiber Cable and Cooling Hose Installation

After the bottom end equipment is re-installed, the physical restraints on the telescope will be removed, and the lock-outs and tag-outs removed from the telescope drive equipment. The telescope will then be moved over to position the top end above the Southeast Annex work platform. See Figure 8.17. The telescope will be locked-out and tagged-out in this position, and the routine physical restraints applied to prevent movement. The dummy weight representing the focal plate assembly will be removed from the top of the corrector barrel, and the real focal plate installed in its place. Doing this work at the Southeast Annex allows the roughly 38-m long fiber cables attached to the focal plate to be laid out in an orderly fashion along the floor while the focal plate is installed. It also enables installation of the delicate focal plate at a location where use of a custom built cart-plus-alignment jig becomes possible, and it provides straightforward access for the personnel carrying out the task.

Appropriate work platforms (to be designed during the Mayall preparation phase) will be installed along the East (down) side of the telescope truss, for access to the fiber mounting brackets and cable wraps. First, the hoses for carrying coolant liquid to the DESI focal plate system will be installed using the same mounting brackets and cable wraps. These hoses are required to share the cable management system with the fiber cables, as the electrical code does not permit hoses carrying liquids to be in the same trays or wraps as any cables carrying an electrical voltage. Im-

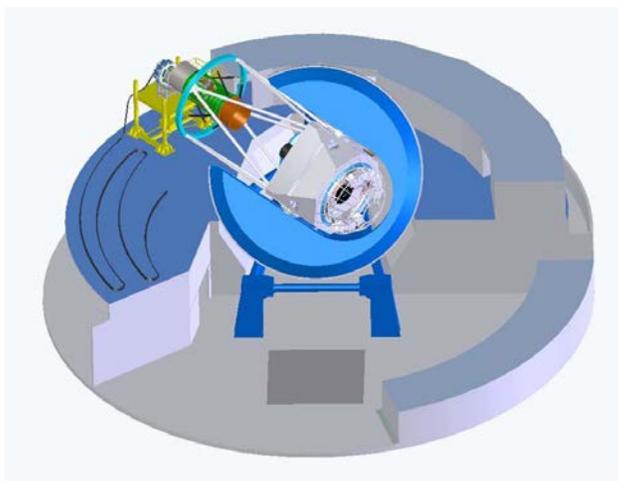


Figure 8.17: Installing the DESI focal plate assembly at the Southeast Annex. Note fiber cables laid out on C floor to North of SE Annex platform.

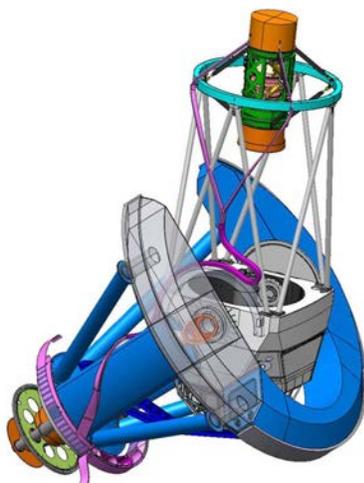


Figure 8.18: Fiber routing on telescope, illustrating locations and space requirements for the Dec and HA cable wraps.

mediately after installation, these hoses will be pressure-tested with air for leaks. Any leaks found will be corrected at once, before installation of the fiber cables.

The optical fiber cables will be mounted along the spider vanes to the top ring and down the truss from the top ring to the East side Declination axis using the mounting hardware previously installed.

Fiber cables will be laid into the Declination axis cable wrap one at a time, then down along the polar axis structure using the previously installed brackets to the cable wrap at the base of that axis. Fiber cables will then be laid into that system one at a time and routed through the adjacent wall separating the telescope chamber from the Coudé room. Figure 8.18 shows the routing of the fiber cables on the telescope with the telescope pointing roughly to zenith for ease of illustration. Figure 8.19 shows the routing through the wall of the Coudé room.

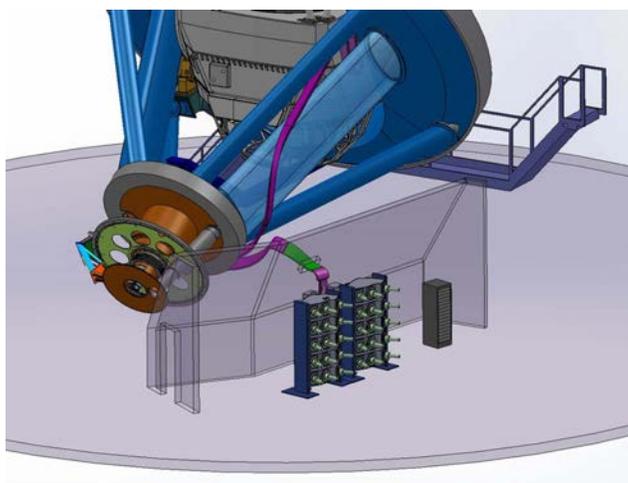


Figure 8.19: Fiber routing through wall of Coudé room to spectrographs. Note that spectrographs may be arranged in three stacks instead of two.

The electrical and data services for the DESI top end cannot follow the same routing, as the electrical code requires that they not share space or mounting hardware with the liquid cooling

hoses. Also, it has not yet been determined whether the power supplies for the focal plate will be located within the focal plate enclosure (orange cylinder at the top of Figure 8.18) or in the Cassegrain cage. If they are located within the focal plate enclosure, then these lines will be dressed down the upper Serrurier truss from the top end and through the West Declination bearing to off-telescope terminations. If in the Cassegrain cage, they will be installed along with the hexapod power supplies (see above) and the Ethernet and DC power cables dressed from the Cassegrain cage along the outside of the center section and upper Serrurier truss (most likely the North side). In either case, that work will be completed before the final steps of removing the physical restraints and lock-out/tag-out protections to re-enable telescope motion.

8.3.2.5 Telescope Motion Tests and Final Alignment Check

With the telescope ready to move, the telescope balance will be checked and bottom-end counterweights changed as needed, but it is expected that only small adjustments will be needed at this point. The telescope will then be put through a series of motion tests to confirm that the new loads in the cable wraps can be handled within nominal drive current limits. The telescope motion servo systems will be re-tuned to optimize performance with the new weight, mechanical moments, and cable wrap loads on the telescope. If there are any problems with meeting slew and settle time requirements, they will be resolved before proceeding further. After that, there will be a final alignment check performed with the laser tracker system at zenith and various other orientations to ensure that movement of the top end position with changing position is within the expected limits. This data may also be used to build a preliminary look-up table for positioning the hexapod following telescope slews.

8.3.2.6 Spectrographs

The ten DESI spectrographs will be installed on their racks in an environmentally controlled chamber (the “spectrograph shack”) in the Coudé room. The work of installing and testing the spectrographs thus does not directly interfere with the flow of work in the main dome. However, to get into the Coudé room, the spectrographs may have to be lifted up from the ground floor through the M floor hatch using the 5-ton dome crane, and then rolled from the telescope dome into the Coudé room. If so, the work in the telescope dome must pause for about one day each time a batch of spectrographs is to be delivered so that these lifts can proceed safely. It is possible that the spectrograph components may fit within the personnel elevators, obviating the need for use of the dome crane but requiring more extensive re-assembly in the Coudé room. If so, this will reduce the conflict with in-dome work. Once the spectrographs are in the Coudé room, the rest of the work on them can proceed without interfering with the work on the telescope, provided that sufficient personnel are available for both tasks, and provided that both groups observe safety restrictions on access to the others’ work areas.

Once the spectrographs are in the Coudé room, they must be verified to assure they survived shipping (a process that will likely require opening the spectrograph housings), partially re-assembled as needed, installed in the racks, and connected to power, cooling, and data services. The slit heads will arrive attached to the 38-m fiber cables, so they will be available only after the fiber cables are installed on the telescope and through the cable wraps, but initial testing can be done with a test slit head prior to fiber installation. Once the slit heads have reached the spectrograph rack, they can be installed on as many spectrographs as are ready to receive them at the time. The remaining slit heads will be secured temporarily for their protection to keep them out of the way while the rest of the spectrographs are installed and connected.

Timing of the spectrograph installation process will largely depend on when the spectrographs are completed and delivered from the integrator to Kitt Peak. Any units that arrive before work starts on the telescope could be installed immediately as long as their environmental enclosure is ready, as work in the Coudé room will not interfere with night-time science observing prior to the telescope shutdown. Similarly, spectrographs delivered after the in-dome work is complete can be installed immediately as well. Timing of spectrograph receipt is not critical to the installation schedule, as on-sky testing can begin with less than all spectrographs (one is sufficient for initial testing).

8.3.2.7 Computer Equipment

The Mayall computer room is located on the mezzanine level one floor above the M floor. The computer room has its own elevator access, and work in that room can proceed independently of the on-telescope installation. The computer racks and equipment can be brought up in the elevators without tying up the dome crane or main floor hatch, further separating the computer installation from the main installation. The only requirement on this work is that it be fully completed in time to support the initial testing of other hardware as the other hardware is installed. This of course assumes that any clearing of unneeded equipment, rearrangement of the room and expansion of the power or cooling services are all finished before the first DESI computers arrive.

8.3.2.8 Support to Other DESI Subsystem Tests

After installation is complete, NOAO staff will be needed to support functional checkout of DESI subsystems. First, the mechanisms in the prime focus cage – the ADC drives and hexapods – will need to be tested, their performance measured, and any required adjustments or repairs carried out. In the case of the hexapod, the confirming measurements will require use of the laser tracker system mounted temporarily above the top surface of the telescope center section. Next, the focal plate system will require testing to make sure that the connections to the cooling fluid system are leakproof, to verify that the movable fibers and fixed fiducials illuminate properly and can be imaged with the Fiber View Camera, and finally that the movable fibers can be positioned accurately. The GFA sensors will also need to be tested at this time to verify that they are sensitive to light and communicating properly with the control software. Third, the slit heads will need to be connected to the spectrographs. Finally, the fiber system and spectrographs will need testing together, both by back-illuminating the fibers from the spectrographs and by taking flat and arc-line calibration images using the dome screen.

8.3.2.9 Telescope Re-Verification

As soon as the motion tests following fiber cable installation are complete, the telescope will be ready for re-verification through night-time observations. These will consist primarily of gathering pointing data to update the telescope pointing model, checking the slew and settle times on-sky to verify the performance of the motion control servo loops, verifying pointing, measuring open-loop tracking performance, verifying guiding under TCS control, and gathering data on top end movement due to flexure to build any look-up tables for control of the DESI hexapod. Tests will also be conducted to verify the proper performance of the interaction between the telescope, the DESI hexapod and the DESI guide-focus-alignment (GFA) sensors. All these on-sky tests require use of the DESI GFA sensors for finding stars, centering stars, and making low-order measurements of the incoming wavefronts to improve image quality within the limited degrees of freedom available.

Some of these checks constitute verification that performance under TCS control post-installation matches pre-installation. A coarse grid of positions that spans the (HA, Dec) range of DESI Survey operations will be used. Slew and settle times will be verified for large (30 degree) and small (5 degree) slews. Pointing, open-loop tracking, and guiding will be checked using stars, and either the small on-axis camera or one of the GFA sensors. The same tests can be performed using the same combination of sensors with ProtoDESI to establish pre-installation performance. Pointing accuracy around the sky shall be verified after the pointing model is updated. Open loop tracking will be checked for random jitter and cumulative errors over a 5 minute interval, using (i) sequences of short exposures and (ii) single long exposures with small nonsidereal drift rates to produce star trails in the axis normal to that under check. Guiding performance will be characterized by image growth of stellar PSFs for 1-20 minute exposures (the longest time matching the average Survey exposure time), and by the power spectrum of guider correction signals to capture small random jitter. Image quality around the sky will be checked with the on-axis camera, measuring stellar PSFs on a night of good seeing. This will be done without using the hexapod for tip-tilt correction, in accordance with the pre-installation test condition.

Once these steps are complete, the telescope is ready for system-level testing on-sky with the rest of the DESI instrument.

8.4 Safety

This safety description focuses on personnel and equipment safety throughout the installation, commissioning and operational phases of the Dark Energy Spectroscopic Instrument (DESI) project. The Plan addresses working conditions and procedures at the Kitt Peak site, as well as the management structure that positively impacts safety.

The DESI project is centrally managed but executed by several teams in various locations and with different funding sponsors. The DESI Installation and Commissioning Safety Plan covers these project phases while recognizing and relying on existing Environmental, Health and Safety Policies at Kitt Peak.

This section provides the plan description and references other project documents for additional details.

8.4.1 Environmental, Health and Safety Plans

The detailed guidelines for safe working conditions are found in site specific Environmental, Health and Safety (EHS) Plans. Each DESI collaborating organization and contractor has established Safety Plans that will govern the specific activities at their own location. The draft safety plan for the Kitt Peak site can be found under DESI-1004. NOAO expects and indeed requires that all staff, permanent to the location or visiting, will follow these local requirements during all work at Kitt Peak.

8.4.1.1 Compliance with Regulations, Codes and Standards

NOAO EHS plans comply with all applicable EHS regulations and requirements in Title 29 of U.S. Code of Federal Regulations (CFR). This includes part 1910, “OSHA Safety and Health Standards for General Industry”, and part 1926, “Safety and Health Regulations for Construction”, 49 CFR Federal Motor Carrier Safety Administration, and 40 CFR Protection of Environment and others that may apply. NOAO considers the above CFRs as a minimum standards.

8.4.1.2 Environmental, Health and Safety Plan Responsibilities

Work conducted on NOAO sites, by participating organizations, shall follow NOAO Safety Plans. These plans include identification of the local Safety Manager/Coordinator and lines of authority to which all personnel working on NOAO activities at that location shall adhere. NOAO Safety plans take the precedence over home institution regulations.

8.4.1.3 EHS Plan Expectations

NOAO has a set of guidelines, expected to be followed, from the local EHS plans while working at Kitt Peak or other NOAO sites. The Kitt Peak Safety Manager and the project management will work with the collaborating institutions to insure that local plans meet Project expectations. The Kitt Peak Safety Manager is responsible for the review of the local plans to see that expectations are met, that all elements (documentation) are available to the staff, and that issues of nomenclature and document titles are reconciled where the differences are identified. The following topics are expected to be addressed in local EHS plans:

- Safety Manager/Coordinator
- Visitors and Access Policy
- Personal Protection Equipment
- Hazardous Material Management
- Emergency Contacts and Procedures-Kitt Peak Emergency Manual
- Utility Use and Servicing
- Lock-out Processes
- Housekeeping
- Reporting and Records

8.4.1.4 Contractor Safety and Health Plans

All NOAO Contractors are required to develop, submit, and implement a project and site-specific safety and health management plan. The plan must be extended to its own employees, project employees, other workers, and members of the public. The contractor is also required to ensure compliance with the plan. The details of the contractor requirements are subject to specific policies from NOAO. Contractor requirements are expected to address the same information as described in section 4.3 above.

For work contracted at NOAO specific locations the contractor's safety record and ongoing Safety Plan will be an important element in the selection criteria. All contractors are required to complete a "Safety and Health Questionnaire for Contractors" that will be used to evaluate potential contract employers. All general contractors shall require subcontractors to comply with the Contractors Safety and Health Specification. The Safety and Health Questionnaire for contractors will be provided to potential Contractors during the proposal documents to be completed. The questionnaire will be used by NOAO to assess contractor's safety performance and Plans and will be used during the selection process.

8.4.1.5 EHS Plan Availability to Personnel

NOAO will maintain a Safety Plan Website that will include links to all applicable NOAO EHS plans and policies to facilitate convenient access to the information to everyone working on NOAO tasks. This is particularly important for visiting staff who work at other institutions where access to the information is not routine.

8.4.2 Safety Reviews and Hazard Analysis

NOAO will conduct periodic design and procedure reviews focused on compliance with safety regulations, this Plan and good practices. The frequency of the reviews will be commensurate with the stage of the project as defined in the Project Management Plan. Reviews will be conducted by safety professionals, the Project Management team and front line supervisors and will focus on specific subsystems of the observatory, the observatory as a whole, and the Safety Plan itself. Included in the safety reviews will be a periodic Hazard Assessment and Hazard Analysis of each subsystem.

8.4.2.1 Safety Reviews

NOAO will conduct periodic design and procedure reviews focused on compliance to the Safety Plan and applicable standards. The frequency of the reviews will correspond with the stage of the project as defined in the Project Management Plan. The Kitt Peak Safety Manager with the support of other safety professionals and project leaders will lead the reviews. Reviews will focus on specific subsystems of the observatory, contracted efforts, the observatory as a whole, and the Safety Plan itself. Included in the reviews will be the periodic Hazard Assessment and Hazard Analysis of each subsystem. The Contractor's hazard analysis will also be reviewed to confirm that the deliverables established in the contract documents are consistent. The Project Manager(s) and the Kitt Peak Safety Manager will determine other safety reviews and their scope during the project period.

8.4.2.2 Job Hazard Analysis

NOAO will utilize a formal job hazard analysis to identify, analyze, and determine the solution for the hazards throughout the project work being done at NOAO. This hazard resolution method for NOAO consists of the series of analytic steps summarized below:

- Define the physical and functional characteristics of the proposed project by employing the information available, and relating the interaction between people, procedures, equipment and the environment.
- Identify known hazards related to all aspects of the DESI project work being done and determine their causes.
- Assess the hazards to determine the severity and probability, and to recommend means for their elimination or control.
- Implement corrective measures to eliminate or control the individual hazards, or accept the corresponding hazards.
- Conduct follow-up analysis to determine the effectiveness of preventive measures, address new or unexpected hazards, and issue additional recommendations if necessary.

8.4.3 Safety Management

The NOAO Project Management team is responsible and held accountable for incorporating the Safety Plan policies, standards, rules, and principles into the project work. To emphasize the commitment to safety, a single NOAO-Kitt Peak Safety Manager will be named to manage, execute, and verify compliance to the Safety Plan. This safety professional reports directly to NOAO-Kitt Peak Director and is accountable for the implementation of the plan. Other team members from NOAO collaborating institutions and outside affiliations will assist the Safety Manager. For appropriate phases of the DESI installation and commissioning, Safety advisors/Project leads will be employed to provide front line review of work in progress. NOAO will also maintain a safety web site to communicate with the large distributed NOAO team and facilitate the dissemination of key information.

8.4.3.1 Kitt Peak Safety Manager

The Kitt Peak Safety Manager is responsible for the NOAO/Kitt Peak Safety Plan, and its implementation, and helps management ensure compliance. The Safety Manager reports directly to the Kitt Peak Director and works closely with NOAO subsystems managers, systems engineers and the safety managers/coordinators at each participating organization responsible for the implementation of local EHS Plans. The Safety Manager has the authority and responsibility to report EHS issues and to make recommendations to the Project Managers. The Kitt Peak Safety Manager encourages the project team to value safety and manage all hazards in their area of responsibility.

The Safety Manager, working with the institutional Safety Managers/Coordinators, will be actively involved in many of the aspects of the project. This group is responsible for

- Preparing the Safety Plan deliverable documents;
- Supporting the Plan level interface with NOAO and others;
- Developing and establishing safety design criteria and safety design requirements as needed;
- Participating in hazardous testing if required;
- Evaluating design changes for their impact to the safety, health or the environment;
- Coordinate and verify adequate emergency response systems and procedures that will be used during the project execution;
- Coordinate EHS activities needed during the project.

8.4.3.2 NOAO Associate Director for Kitt Peak

The Kitt Peak Director has the overall responsibility for ensuring that EHS Management practices are incorporated into the DESI project. The Kitt Peak director and NOAO-DESI project manager will implement the NOAO Installation and Commissioning Safety Plan and EHS objectives by:

- Confirming that the Safety Plan is established and integrated throughout NOAO.
- Confirming that known hazards are identified, eliminated, or controlled within established Plan hazard acceptability parameters.
- Reinforcing that NOAO operations are performed in accordance with applicable project safety requirements, and applicable governmental safety regulations.

8.4.3.3 NOAO DESI Project Manager

The NOAO DESI Project Manager has the day-to-day responsibility for ensuring that EHS Management practices are incorporated into local activities of the DESI Project. The NOAO DESI Project Manager will implement the NOAO Installation and Commissioning Safety Plan in close coordination with the Kitt Peak Safety Manager to ensure all subsystem managers to keep EHS issues a priority in all aspects of the project. Specifically the project manager and subsystem manager will:

- Make EHS considerations a part of all planning processes by identifying known hazards, determining what standards apply, implementing control, determining the competencies required to do the work safely, and finally assuring that each of these elements are in place before work is authorized to proceed.
- Focus on safe accomplishment of the operation, understanding assignments and carrying out the core safety management functions correctly and efficiently. These principles are dependent upon both management commitment and employees/individual involvement and accountability.
- Ensure the Safety Plan is established and integrated throughout the DESI project.
- Ensure that known hazards are identified, eliminated or controlled within established Plan hazard acceptability parameters.
- Review and approve safety analysis and Safety Plan documents.
- Ensuring that necessary documents are submitted to agencies that require them.

8.4.3.4 NOAO Safety Team

A NOAO project safety team will be established and will consist of representatives from each of the project groups and critical subsystems as determined by the Project Manager(s). The purpose of this team is to consult on EHS issues, provide policy advice, evaluate Plan effectiveness, and make recommendations to the project team. The project safety team will meet at appropriate intervals as required and determined by the team and safety manager.

8.4.3.5 Team Members

All members of NOAO team as well as DESI team members working at Kitt Peak are responsible for integrating safety into their work and supporting the EHS plan as established for the work location. NOAO and DESI staff are encouraged and empowered to understand the work environment and identify the signs, procedures and conditions that they consider unsafe, whether specifically addressed in EHS plans or otherwise occurring. Every team member working at Kitt Peak, regardless of who employs them, can stop work and seek technical assistance from the safety manager for guidance, resolution of safety issues or disputes involving the project.

8.4.4 Design for Safe Installation and Operation

NOAO will follow the best installation and commissioning practices and comply with the appropriate laws and standards in all aspects of the DESI project. The NOAO team, the safety manager,

project managers and engineers will work closely to apply the correct safety standard to the different elements. In all cases, they will be consistent with applicable standards from US Federal Government and other institutions, including:

- U.S. Occupational Safety and Health Administration (OSHA)
- Environmental Protection Agency (EPA)
- National Fire Protection Association (NFPA)
- National Optical Astronomy Observatory
- Department of Energy National Laboratories

Cooperation between the Safety Manager, Engineering staff and the safety team will be required to keep everyone involved with the review and hazard analysis processes described in this Plan and the project hazard management processes. As operating procedures are developed, the job hazard analysis will be included to protect people, equipment, and processes from known hazards.

As discussed in the preliminary safety plan and hazard analysis documents (DESI-1004), the major hazards during the Kitt Peak work include (but are not limited to) working at height, and overhead lifts of heavy, high-value equipment. The procedure for every task involving such hazards will be accompanied by Job Hazard Analyses and Critical Lift Plans which will cover all the hazard mitigations required for the task. As an example, in the case of at-height work, mitigations will include: designing the at-height work platforms to allow two means of ingress and egress; ensuring that all personnel have appropriate Personal Protective Equipment (PPE) for the job – fall restraint harnesses with attachment gear, hard hats, etc – and are fully trained in how to use it; and ensuring that an adequate number of personnel fully trained in at-height rescue are available at all times.

9 Commissioning

9.1 Overview

This section describes the plan for commissioning of the DESI instrument. A comprehensive commissioning plan is being developed and is available in DESI-0973. As we gain experience with the DESI components and ProtoDESI we will update the commissioning plan. To provide context this section also briefly describes the tests that will occur before the commissioning begins (Functional Verification) and the period of Science Verification that occurs after commissioning but prior to the start of the 5 year survey.

The purposes of Commissioning and Science Verification are to test and optimize the full DESI system and to ensure that it meets the requirements. Commissioning begins at the completion of functional tests of the telescope and DESI systems following installation of the focal plane/fiber positioner system in the prime focus cage on the Mayall telescope. Commissioning is currently scheduled to take place from January to June 2019. Completion of commissioning marks the completion of the DESI DOE construction project and the readiness for DESI for CD-4. A Science Verification period follows commissioning, and at its conclusion DESI should be ready for the 5 year DESI survey to begin. Technical support of DESI will be reduced, but will not end with the completion of the project. An operations budget will provide funding for the effort needed for operation of the survey after completion of the construction project.

Commissioning is largely a science-driven activity; by contrast, the phases of installation and functional verification are primarily engineering activities. Commissioning starts with on-sky testing. The activities to be carried out are systems tests to evaluate the performance and to identify causes where performance specifications are not met. The ability to respond to the unexpected with fast decisions is important, such as being able to adjust the observing schedule in near real-time depending on weather and other circumstances, while still trying to keep within the bounds of the time provided. The DESI project key performance parameters, KPPs, (see DESI Project Execution Plan) require that the DESI system has at least 6 spectrographs and that it has demonstrated the ability to obtain simultaneous spectra of hundreds of galaxies prior to completion of the commissioning period and the DOE construction project.

9.2 Functional Verification

Functional Verification of all the DESI systems will happen after each have been installed. Nearly all of them require the use of the DESI Online System (DOS). To define the state of the DESI systems at the start of commissioning we include a list of some of these tests here.

- Laser tracker: measure primary mirror to PF cage flexure using the laser tracker, build information for the hexapod look up table. The laser tracker will be removed from the telescope after that use.
- Spectrograph system: Operate spectrograph climate control system, pump down and operate cryostats and LPTs, dark exposures with spectrograph CCDs (involves data system also), operate spectrograph accessories
- Focal Plane System: Leak check FP cooling services, check cooling system aliveness (fans, temperature sensors), move positioners one petal at a time, look at them through porthole, turn on and read out Fiber View Camera (FVC), turn on and read out Guide and Focus Arrays (GFAs) (darks), illuminate field fiducials and image with FVC.

- Barrel: Rotate Atmospheric Dispersion Correctors (ADCs), visually monitor and or monitor encoder, operate Hexapod, visually monitor and/or measure barrel/cage relative motion directly.
- Telescope (and fiber wraps): Use ICS/TCS connection to point telescope with dome closed. Operate at slew and tracking speeds. Observe fiber wraps and telescope drive motor torques.
- Spectrograph/fiber system: Point at dome screen, do spectrograph exposures with each of the various calibration lamps (involves data system also).
- Fiber/FP: Back-illuminate fibers with GSE back-illuminator, take and readout FVC image, move all positioners 1 mm, repeat FVC.
- Spectrograph/fiber: Back-illuminate fibers with spectrograph back-illuminator, take and readout FVC image.
- The DESI Data Transport System (DDTS) is a DESI project deliverable The DDTS will have data paths set up and be thoroughly tested prior to commissioning. We will exercise it during commissioning by relying on it as the primary data transport mechanism.
- Quicklook pipelines on the Mt. debugged and tested.
- Full data reduction pipeline at LBNL run and tested on calibration frames (flats and arcs)
- Confirm that appropriate metadata is recorded in fits files and observation database for each exposure

9.3 Commissioning

Commissioning is when these separate sub-systems are operated as a system and on-sky tests begin. Broadly, commissioning includes:

- Tests that are designed to prove the correct functioning of the DESI system.
 - Verify that installation on the telescope has not degraded any performance characteristics (overlaps with functional verification tests).
 - Evaluate the optical performance, end-to-end.
 - Test and calibrate telescope-camera systems such as the fiber view camera, the automatic focus system, the guide system, the mirror support system (air pads), and the alignment system.
 - Test the ability of the telescope to point and track such that fibers stay located on targets for the required exposure times.
 - Collect astronomical and calibration data that will allow testing of the Pipelines.
 - Test the robustness (fault-tolerance), as a system.
 - Determine initial operational efficiency (will be optimized later).
- The science pipelines will be used during the commissioning period to provide feedback to the commissioning team. They will be optimized during the science verification period. Quicklook pipelines will be needed on the Mt. We will determine at a later date if the full set of pipelines will need to run on the Mt. as well as at LBNL (NERSC).

Commissioning will require broad participation from the collaboration. Some activities will happen on Kitt Peak but many require attention from people off-site. Excellent connectivity is essential. Activities on Kitt Peak include:

- Calibration, characterization of CCDs and spectrograph response using lamps (the dome has been demonstrated to be dark enough to do this).
- Monitor spectrograph shack climate controls
- Operating positioners and imaging backlit fibers using Fiber View Camera (may require a special filter for daytime testing).
- Operations training
- Final safety signoff

Examples of offsite activities include:

- Exercise the reduction pipelines, with real data.
- Evaluate the data quality
- Monitor the data transport system (DTS) performance and reliability.
- These groups will provide quick feedback to the on-site commissioning team.

Formally the Commissioning period can be declared complete when the DESI system has demonstrated that it can routinely obtain simultaneous spectra of hundreds of galaxies.

9.4 Science Verification

Science Verification continues the transition to a system capable of executing the DESI survey. It will be led by the scientific team but will likely need periodic technical support from the commissioning team. SV tests the end-to-end system by demonstrating that a substantive sample of data collected with the DESI protocols can be reduced and meets the science requirements. It begins the process of measuring and improving operational efficiency. DESI-0943 contains the detailed planning.

At the end of commissioning and science verification DESI will not be finished, in the sense that optimization of the active optics control system, provision of better calibrations and characteristics, tweaking and bug-fixing of software, etc. are all activities that are expected to continue for some time. Given successful commissioning, all these activities can take place while DESI is being used for science, normally with updates being implemented and tested during scheduled telescope maintenance periods and engineering runs.

9.5 Commissioning Strategy

It is expected that all 10 spectrographs will be available at the start of the commissioning. Even if not, the DESI online system will be able to deal with different numbers of spectrographs and petals. In addition we will construct a back illumination system for the fibers that are not in a spectrograph so that they may be included in the tests of the fiber view camera and fiber positioning tests. We note that project Key Performance Parameters can be met with as few as 6 spectrographs.

The Commissioning plan (DESI-0973) contains a summary of the expected weather data during the February to July time period, based on a study of historical weather patterns (DESI-0993).

Averages and extremes of usable hours per month and useful nights are tabulated using data from 2005-2014. The bottom line is that for average weather we can expect the commissioning period to have roughly 50% clear nights and about 75% of nights of useful data taking.

The commissioning plan details the commissioning tasks and divides them into four levels of increasing complexity (see Chapter 4 of DESI-0973), gradually approaching readiness for science verification. Tuning and improvement of performance and reliability will continue after commissioning is complete.

9.6 Commissioning Roles

Scientists and engineers from the DESI Collaboration and NOAO will participate in the commissioning activities. They will be organized as a day crew, a night crew, and a remote crew. The night crew will run the nighttime tests. The day crew will respond to nighttime problems and run scheduled daytime tests. The night crew in particular will likely be populated as teams, working approximately on a weekly schedule. Sub-system experts will be made available, many remotely, depending on the schedule. The remote crew will be geographically dispersed (Tucson, LBL and other DESI institutions) and will generally be monitoring pipeline outputs and conducting more deep analyses of data, where appropriate using codes developed for DESI. A daily “1pm meeting” will be used to communicate progress and problems between the daytime and nighttime crews. This model was used in the successful commissioning of DECam.

Specific Roles are listed below:

1. The DESI Project Scientists head the commissioning of the DESI System. Responsibilities include preparing the day-to-day plan, assigning staff, seeing that the plan is executed, monitoring progress, signing off on planning changes, reporting to senior management.
2. NOAO Telescope Scientist - The scientist present at the telescope who is the expert on telescope operations and performance. This may be staffed by NOAO.
3. On-duty scientists and staff - Other scientists and technical staff present at Kitt Peak during commissioning. This will be a mixture of NOAO staff and DESI collaboration members. These may work day shift, night shift, or swing shift. One will be the NOAO Telescope Scientist. Some may work directly on executing the commissioning programs, others on analysis, troubleshooting, etc. There will be one person specifically assigned to be responsible for maintaining a Punch List.

9.7 Summary

In many ways the DESI system is similar to the DECam system that was installed on the Blanco telescope in 2012. In particular re-commissioning of the telescope control system, tracking, pointing and commissioning of the communications between the TCS and the DESI guide and focus systems will follow similar steps. An initial version of the commissioning plan has been prepared. It builds on the experience of DECam and will continue to be developed over the course of the project as we gain experience with the DESI specific systems. Experience with ProtoDESI will provide critical input into the commissioning plans and will inform future updates to the commissioning plan.

A Acronyms

1D	One-Dimensional
3D	Three-Dimensional
A&G	Acquisition and Guiding
A/R	AntiReflection
AAO	Australian Astronomical Observatory
AAT	Anglo-Australian Telescope
ABL	AirBorne Laser Aircraft
ACT	Atacama Cosmology Telescope
ADC	Atmospheric Dispersion Compensator
ADC	Analog to Digital Converter
ADR	Atmospheric Differential Refraction
AGN	Active Galactic Nucleus
AI&T	Assembly, Integration and Test
AOS	Active Optics System
AP	Alcott-Pachinko [sic]
API	Application Programming Interface
APO	Apache Point Observatory
APOGEE	The APO Galactic Evolution Experiment
AR	Antireflection
ASTM	American Society for Testing and Materials
AURA	Association of Universities for Research in Astronomy
BAO	Baryonic Acoustic Oscillations
BCAM	Brandeis CCD Angle Monitor
BOSS	Baryon Oscillation Spectroscopic Survey
BTGS	Bright Time Galaxy Survey
CABT	Centrale d'Aquisition Basses Température (Low Temperature Data Controller)
CAD	Computer-Aided Design
CAN	Controller Area Network
CCD	Charge Coupled Device
CDE	Cooler Drive Electronics
CDM	Cold Dark Matter
CDR	Critical Design Review; Conceptual Design Report
CEA	Commissariat à l'Énergie Atomique
CFHT	Canada-France-Hawaii Telescope
CFHTLS	CFHT Legacy Survey
CM	Configuration Management
CMASS	BOSS Constant Mass Sample
CMB	Cosmic Microwave Background
CMM	Coordinate Measurement Machine
CNC	Computer Numerical Control
CoDR	Concept Design Review/Report
CPU	Central Processing Unit
CSS	Cascading Style Sheets
CTE	Coefficient of Thermal Expansion

CTE	Charge Transfer Efficiency (CCD)
CTIO	Cerro Tololo Inter-American Observatory
DAQ	Data AcQuisition
DE	Dark Energy
DEC	Declination
DECam	Dark Energy Camera
DEEP2	Deep Extragalactic Evolutionary Probe 2
DEIMOS	DEep Imaging Multi-Object Spectrograph
DES	Dark Energy Survey
DESI	Dark Energy Spectroscopic Instrument
DETF	Dark Energy Task Force
DGP	DvaliGabadadzePorrati
DIMM	Differential Image Motion Monitor
DOE	Department of Energy
DOF	Degrees of Freedom
DRP	Data reduction pipeline
DR9	SDSS-III/BOSS Data Release 9
DR11	SDSS-III/BOSS Data Release 11
DTS	Data Transport System
EE50	50% Encircled Energy
EE95	95% Encircled Energy
EE99	99% Encircled Energy
EGSE	Electrical Ground Support Equipment
ELG	Emission Line Galaxy
EPA	Environmental Protection Agency
ESNET	Energy Sciences Network
FEA	Finite Element Analysis
FEE	Front-End Electronics
FITS	Flexible Image Transport System
FLA	Field Lens Assembly
FNAL	Fermi National Accelerator Laboratory
FoM	Figure of Merit
FOV	Field of View
FPA	Focal Plane Assembly
FPD	Focal Plate Adapter
FPGA	Field Programmable Gate Array
FPS	Focal Plane System
FRD	Focal Ratio Degradation
FTS	Fourier Transform Spectrograph
FVC	Fiber View Camera
FWHM	Full Width at Half Maximum
GAMA	Galaxy And Mass Assembly Survey
GFA	Guide, Focus, and Alignment
GNU	GNU's Not Unix!
GUI	Graphical User Interface
HPSS	High Performance Storage Systems
HTML	HyperText Markup Language
HVAC	Heating, Ventilation, and Air Conditioning

I&T	Integration and Test
IAA	Instituto de Astrofísica de Andalucía
IAC	Instituto de Astrofísica de Canarias
ICD	Interface Control Document
ICS	Instrument Control System
IDD	Interface Definition Drawing/Document
IDL	Interactive Data Language
IGM	Intergalactic Medium
IP	Internet Protocol
IPAC	Infrared Processing and Analysis Center
iPTF	Intermediate Palomar Transient Factory
IR	InfraRed
KPNO	Kitt Peak National Observatory
L1	Level 1 requirements
L2	Level 2 requirements
L3	Level 3 requirements
LAM	Laboratoire d'Astrophysique de Marseille
LBNL	Lawrence Berkeley National Laboratory
LBT	Large Binocular Telescope
LED	Light Emitting Diode
LHC	Large Hadron Collider
LOWZ	BOSS Low Redshift Galaxy Sample
LPT	Linear Pulse Tube
LRG	Luminous Red Galaxy
LSS	Large Scale Structure
LSST	Large Synoptic Survey Telescope
M2	Existing secondary mirror at Mayall 4m telescope
MAST	Mikulski Archive for Space Telescopes
MB	Megabyte
MDLF	Mikulski Archive for Space Telescopes
MG	Modified Gravity
MMT	Multiple Mirror Telescope
MOS	Multi-Object Spectrograph
MOU	Memorandum of Understanding
MPC	Multi-Point Constraint
MTBF	Mean Time Between Failures
MVC	Model-View-Controller
NA	Not Applicable
NASA	National Aeronautics and Space Administration
NCSA	National Center for Supercomputing Applications
NERSC	National Energy Research Scientific Computing Center
NFPA	National Fire Protection Association
NGC	Northern Galactic Cap
NIR	Near-Infrared
NOAO	National Optical Astronomy Observatory
NOAONVO	NOAO National Virtual Observatory
NOMAD	Naval Observatory Merged Astrometric Dataset
NSF	National Science Foundation

NVO	National Virtual Observatory
OCS	Observation Control System
ODI	One Degree Imager
OPD	Optical Path Difference
OPO	Optical Parametric Oscillator
OSHA	Occupational Safety and Health Administration
OSS	Observatory System Specification
PAH	Polycyclic Aromatic Hydrocarbon
Pan-STARRS	The Panoramic Survey Telescope and Rapid Response System
PC	Personal Computer
PCA	Principal Component Analysis
PDR	Preliminary Design Review
PF	Prime Focus
PFA	Positioner Fiber Assembly
PFC	Prime Focus Corrector
PFI	Prime Focus Instrument
PFU	Prime Focus Unit
PI	Principal Investigator
PLC	Programmable Logic Controller
PM	Project Manager/Management
PML	Physical Markup Language
POS	Fiber Positioner
PPM	Parts Per Million
PSF	Point Spread Function
PSM	Point Source Microscope
PTF	Palomar Transient Factory
PTL	Focal Plate Petal
PVC	PolyVinyl Chloride
PYRO	Python Remote Objects
QA	Quality Assurance
QC	Quality Control
QE	Quantum Efficiency
QSO	Quasi-Stellar Object
R&D	Research and Development
RA	Right Ascension
RFP	Request for Proposal
RGB	Red Giant Branch
RMI	Remote Method Invocation
rms	Root Mean Square
ROC	Radius of Curvature
ROI	Region of Interest
ROM	Rough Order of Magnitude
RSD	Redshift Space Distortions
RSS	Root Sum Squared
RTD	Resistance Temperature Detector
RTV	Room Temperature Vulcanizing silicone
S/N	Signal to Noise
SCUSS	The South Galactic Cap U-band Sky Survey

SDF	Spectral Density Function
SDSS	Sloan Digital Sky Survey
SE	Systems Engineering
SED	Spectral Energy Distributions
SEGUE	The Sloan Extension for Galactic Understanding and Exploration
SEP	Systems Engineering Plan
SEQUELS	Sloan Extended QUasar, ELG and LRG Survey
SET	Systems Engineering Team
SGC	Southern Galactic Cap
SHE	Safety, Health and Environmental
SIDE	Super Ifu Deployable Experiment
SMBH	SuperMassive Black Hole
SN	SuperNova
SNR	Signal-to-Noise Ratio
SOW	Statement of Work
SPT	South Pole Telescope
SQL	Structured Query Language
SRD	Science Requirements Document
SRR	System Requirements Review
SRS	Software Requirements Specification
SVE	Shared Variable Engine
TB	TerraBytes
TBA	To Be Announced
TBC	To Be Confirmed
TBD	To Be Defined/Decided/Determined
TBR	To Be Reviewed/Revised/Resolved
TCP	Transmission Control Protocol
TCS	Telescope Control System
TES	Top-End Structure
TKRS	The Team Keck Treasury Redshift Survey
TTL	Transistor-Transistor Logic
UCL	University College London
UK	United Kingdom
UPS	Uninterruptible Power Supply
URL	Uniform Resource Locator
USA	United States of America
USB	Universal Serial Bus
USTC	University of Science and Technology China
UV	Ultraviolet
UVES	Ultraviolet and Visual Echelle Spectrograph
VAC	Volts AC
VIMOS	Visible MultiObject Spectrograph
VIPERS	VIMOS Public Extragalactic Redshift Survey
VISTA	Visible and Infrared Survey Telescope for Astronomy
VLT	Very Large Telescope
VPH	Volume Phase Holographic
VVDS	VIMOS VLT Deep Survey
WBS	Work Breakdown Structure

WFC	Wide Field Corrector
WFIRST	The Wide-Field Infrared Survey Telescope
WFOS	Wide-Field Multi-Object Spectrograph
WGL	Weak Gravitational Lensing
WIRO	University of Wyoming's 2.3 m telescope
WISE	Wide-field Infrared Survey Explorer
WIYN	Wisconsin, Indiana, Yale, NOAO Telescope
WMAP	Wilkinson Microwave Anisotropy Probe
WP	Wilkinson Microwave Anisotropy Probe
ZTF	Zwicky Transient Facility

References

- [1] A. Albrecht et al. “Report of the Dark Energy Task Force”. In: *ArXiv Astrophysics e-prints* (Sept. 2006). eprint: [astro-ph/0609591](https://arxiv.org/abs/astro-ph/0609591).
- [2] DESI. *DESI Level 1 through Level 3 Requirements, Science Objectives, Survey Data Set, Instrument Technical Requirements*. DESI-doc-318. Nov. 2013.
- [3] R. W. Hanuschik. “A flux-calibrated, high-resolution atlas of optical sky emission from UVES”. In: *Astron. Astrophys.* 407 (Sept. 2003), pp. 1157–1164.
- [4] R. G. Fata, V. Kradinov, and D. Fabricant. “Mounting large lenses for the MMT’s f/5 wide-field corrector: lessons learned”. In: *Society of Photo-Optical Instrumentation Engineers (SPIE) Conference Series*. Ed. by A. F. M. Moorwood and M. Iye. Vol. 5492. Society of Photo-Optical Instrumentation Engineers (SPIE) Conference Series. Sept. 2004, pp. 553–563.
- [5] K. B. Doyle, G. J. Michels, and V. L. Genberg. “Athermal design of nearly incompressible bonds”. In: *Optomechanical Design and Engineering 2002*. Ed. by A. E. Hatheway. Vol. 4771. Society of Photo-Optical Instrumentation Engineers (SPIE) Conference Series. Sept. 2002, pp. 296–303.
- [6] Ingrid Fang et al. *Conceptual design of the DESI corrector barrel for the ECHO22 optics*. DESI-doc-xxx. 2014.
- [7] A. Roodman. “Focus and alignment of the Dark Energy Camera using out-of-focus stars”. In: *Proc. SPIE* 8446 (2012), p. 60.
- [8] J. R. Fienup. “Phase-retrieval algorithms for a complicated optical system”. In: *Applied Optics (ISSN 0003-6935)* 32 (Apr. 1993), p. 1737.
- [9] F. James and M. Roos. “Minuit - a system for function minimization and analysis of the parameter errors and correlations”. In: *Computer Physics Communications* 10 (1975), p. 343.
- [10] Zacharias et al. “The Naval Observatory Merged Astrometric Dataset (NOMAD)”. In: *San Diego AAS Meeting* 48.15 (Jan. 2005).
- [11] J. N. Bahcall and R. M. Soneira. “Star counts as an indicator of galactic structure and quasar evolution”. In: *Astrophys. J. Lett.* 238 (May 1980), pp. L17–L20.
- [12] J. N. Bahcall and R. M. Soneira. “Comparisons of a standard galaxy model with stellar observations in five fields”. In: *Astrophys. J. Supp.* 55 (May 1984), pp. 67–99.
- [13] K. Reil et al. “Guide, focus/alignment system for BigBOSS”. In: *Proc. SPIE* 8450 (2012), pp. 845037–845037–9.
- [14] J. Allington-Smith et al. “End effects in optical fibres”. In: *Mon. Not. R. Astron. Soc.* 436 (Dec. 2013), pp. 3492–3499. arXiv: 1309.6569 [astro-ph.IM].
- [15] J. Zhou, J. Shannon, and J. Clarkin. *FBP Broad Spectrum Optical Fiber for Astronomy and Spectroscopy*. 2008. URL: http://www.molex.com/mx/_upload/superfamily/polymicro/pdfs/FBP_Broad_Spectrum_Optical_Fiber_for_Astronomy_and_Spectroscopy_Jun_2008.pdf.
- [16] S. A. Smee et al. “The Multi-object, Fiber-fed Spectrographs for the Sloan Digital Sky Survey and the Baryon Oscillation Spectroscopic Survey”. In: *Astron. J.* 146, 32 (Aug. 2013), p. 32. arXiv: 1208.2233 [astro-ph.IM].

- [17] E. B. Burgh et al. “Recombination Ghosts in Littrow Configuration: Implications for Spectrographs Using Volume Phase Holographic Gratings”. In: *Proc. Astron. Soc. Pacific* 119 (Sept. 2007), pp. 1069–1082. arXiv: 0708.0402.
- [18] T. P. O’Brien et al. “Design of the KOSMOS oil-coupled spectrograph camera lenses”. In: *Society of Photo-Optical Instrumentation Engineers (SPIE) Conference Series*. Vol. 9151. Society of Photo-Optical Instrumentation Engineers (SPIE) Conference Series. July 2014, p. 41. arXiv: 1407.4542 [astro-ph.IM].
- [19] D. Kubik et al. “Automated characterization of CCD detectors for DECam”. In: *Society of Photo-Optical Instrumentation Engineers (SPIE) Conference Series*. Vol. 7735. Society of Photo-Optical Instrumentation Engineers (SPIE) Conference Series. July 2010.
- [20] H. T. Diehl et al. “Testing the Dark Energy Camera on a telescope simulator”. In: *Society of Photo-Optical Instrumentation Engineers (SPIE) Conference Series*. Vol. 7735. Society of Photo-Optical Instrumentation Engineers (SPIE) Conference Series. July 2010.
- [21] B. Flaugher, T. Diehl, Honscheid K., et al. “The Dark Energy Camera”. In: *Astron. J.* (2015). arXiv: 1504.02900 [astro-ph.IM].
- [22] K. Honscheid et al. “The readout and control system of the Dark Energy Camera”. In: *Proc. SPIE* 8451 (Sept. 2012). Ed. by Nicole M. Radziwill and Gianluca Chiozzi, p. 845112. URL: <http://dx.doi.org/10.1117/12.925717>.
- [23] K. Honscheid et al. “The DECam DAQ System: lessons learned after one year of operations”. In: *Proc. SPIE* 9152 (July 2014). Ed. by Gianluca Chiozzi and Nicole M. Radziwill, 91520G. URL: <http://dx.doi.org/10.1117/12.2057073>.
- [24] M. J. Fitzpatrick. “DTS: the NOAO Data Transport System”. In: *Proc. SPIE* 7737 (July 2010). Ed. by David R. Silva, Alison B. Peck, and B. Thomas Soifer, 77371T. URL: <http://dx.doi.org/10.1117/12.857329>.
- [25] A. Roodman. “Focus and alignment using out-of-focus stellar images at the Dark Energy Camera”. In: *Proc. SPIE* 7735 (July 2010). Ed. by Ian S. McLean, Suzanne K. Ramsay, and Hideki Takami, 77353T. URL: <http://dx.doi.org/10.1117/12.857680>.
- [26] A. Roodman. “Focus and alignment of the Dark Energy Camera using out-of-focus stars”. In: *Proc. SPIE* 8446 (Sept. 2012). Ed. by Ian S. McLean, Suzanne K. Ramsay, and Hideki Takami, 84466O. URL: <http://dx.doi.org/10.1117/12.926671>.
- [27] A. Roodman, K. Reil, and C. Davis. “Wavefront sensing and the active optics system of the dark energy camera”. In: *Proc. SPIE* 9145 (July 2014). Ed. by Larry M. Stepp, Roberto Gilmozzi, and Helen J. Hall, p. 914516. URL: <http://dx.doi.org/10.1117/12.2056904>.
- [28] S. Kposov and O. Bartunov. “Q3C, Quad Tree Cube – The new Sky-indexing Concept for Huge Astronomical Catalogues and its Realization for Main Astronomical Queries (Cone Search and Xmatch) in Open Source Database PostgreSQL”. In: *Astronomical Data Analysis Software and Systems XV*. Ed. by C. Gabriel et al. Vol. 351. Astronomical Society of the Pacific Conference Series. July 2006, p. 735.
- [29] A. S. Bolton et al. “Spectral Classification and Redshift Measurement for the SDSS-III Baryon Oscillation Spectroscopic Survey”. In: *Astron. J.* 144, 144 (Nov. 2012), p. 144. arXiv: 1207.7326 [astro-ph.CO].
- [30] A. S. Bolton and D. J. Schlegel. “Spectro-Perfectionism: An Algorithmic Framework for Photon Noise-Limited Extraction of Optical Fiber Spectroscopy”. In: *Proc. Astron. Soc.-Pacific* 122 (Feb. 2010), pp. 248–257. arXiv: 0911.2689 [astro-ph.IM].

- [31] K. Horne. “An optimal extraction algorithm for CCD spectroscopy”. In: *Proc. Astron. Soc.-Pacific* 98 (June 1986), pp. 609–617.
- [32] A. S. Bolton et al. “What is a Spectrum?” In: *Astronomical Data Analysis Software and Systems XXI*. Ed. by P. Ballester, D. Egret, and N. P. F. Lorente. Vol. 461. Astronomical Society of the Pacific Conference Series. Sept. 2012, p. 509. arXiv: 1111.6525 [astro-ph.IM].
- [33] M. Fitzpatrick. “DTS: The NOAO Data Transport System”. In: *Astronomical Data Analysis Software and Systems XIX*. Ed. by Y. Mizumoto, K.-I. Morita, and M. Ohishi. Vol. 434. Astronomical Society of the Pacific Conference Series. Dec. 2010, p. 260.
- [34] Michael J. Fitzpatrick. “DTS: the NOAO Data Transport System”. In: *Observatory Operations: Strategies, Processes, and Systems III*. Ed. by David R. Silva, Alison B. Peck, and B. Thomas Soifer. Vol. 7737. Proc. SPIE. July 2010, 77371T. URL: <http://dx.doi.org/10.1117/12.857329>.
- [35] A. J. S. Hamilton and M. Tegmark. “A scheme to deal accurately and efficiently with complex angular masks in galaxy surveys”. In: *Mon. Not. R. Astron. Soc.* 349 (Mar. 2004), pp. 115–128. eprint: arXiv:astro-ph/0306324.
- [36] R. W. Hanuschik. “A flux-calibrated, high-resolution atlas of optical sky emission from UVES”. In: *Astron. Astrophys.* 407 (Sept. 2003), pp. 1157–1164.
- [37] A. Dey. private communication.
- [38] N. Mostek et al. “Mapping the universe with BigBOSS”. In: *Society of Photo-Optical Instrumentation Engineers (SPIE) Conference Series*. Vol. 8446. Society of Photo-Optical Instrumentation Engineers (SPIE) Conference Series. Sept. 2012.
- [39] Brian Nord, Adam Amara, and Alexandre Réfrégier. “SPOKES: an End-to-End Simulation Facility for Spectroscopic Cosmological Surveys”. in prep. 2013.
- [40] Alexandre Réfrégier and Adam Amara. “A Way Forward for Cosmic Shear: Monte-Carlo Control Loops”. In: *arXiv.org* (Mar. 2013). arXiv: 1303.4739v1 [astro-ph.CO].
- [41] LSST Science Collaboration et al. “LSST Science Book, Version 2.0”. In: *arXiv.org* (Dec. 2009), p. 201. arXiv: 0912.0201 [astro-ph.IM].